

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030743.D
 Acq On : 21 Apr 2023 02:04
 Operator : SY/MD
 Sample : 02440-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rVB	103963	112494	14.68%	1.821%
2	1.536	147	154	168	rVB	95800	113919	14.87%	1.844%
3	2.063	309	318	340	rVB	197195	289384	37.77%	4.684%
4	2.388	416	419	420	rBV3	1249	648	0.08%	0.010%
5	2.436	432	434	436	rBV3	1568	925	0.12%	0.015%
6	2.674	505	508	512	rBV5	1083	979	0.13%	0.016%
7	2.777	537	540	541	rBV3	1182	562	0.07%	0.009%
8	2.966	593	599	604	rVB10	2438	3161	0.41%	0.051%
9	2.995	604	608	609	rBV4	1146	678	0.09%	0.011%
10	3.031	617	619	621	rBV2	1101	547	0.07%	0.009%
11	3.079	633	634	639	rBV5	1183	945	0.12%	0.015%
12	3.281	690	697	698	rBV5	1668	1457	0.19%	0.024%
13	3.722	832	834	835	rBV2	1659	621	0.08%	0.010%
14	3.751	839	843	847	rBV7	971	1077	0.14%	0.017%
15	3.796	847	857	884	rBV	48889	140077	18.28%	2.267%
16	4.124	957	959	962	rBV4	1235	931	0.12%	0.015%
17	4.256	988	1000	1020	rBV	129322	310738	40.56%	5.029%
18	4.580	1098	1101	1102	rBV3	1476	943	0.12%	0.015%
19	4.706	1136	1140	1144	rBV7	1504	1246	0.16%	0.020%
20	4.732	1146	1148	1153	rVV5	1555	753	0.10%	0.012%
21	4.773	1158	1161	1165	rBV4	946	852	0.11%	0.014%
22	4.796	1165	1168	1171	rBV4	848	693	0.09%	0.011%
23	4.860	1184	1188	1190	rBV4	974	739	0.10%	0.012%
24	4.966	1203	1221	1248	rBV2	285411	766203	100.00%	12.401%
25	5.333	1333	1335	1336	rBV2	1236	572	0.07%	0.009%
26	5.420	1360	1362	1364	rBV3	1492	710	0.09%	0.011%
27	5.542	1387	1400	1423	rVV	278716	576957	75.30%	9.338%
28	5.802	1479	1481	1483	rBV2	1665	704	0.09%	0.011%
29	5.998	1529	1542	1561	rBV	166401	348258	45.45%	5.637%
30	6.420	1670	1673	1674	rBV3	1443	699	0.09%	0.011%
31	6.522	1703	1705	1709	rBV4	1391	1177	0.15%	0.019%
32	6.584	1722	1724	1727	rBV4	1061	646	0.08%	0.010%
33	6.641	1738	1742	1745	rBV6	1707	1272	0.17%	0.021%
34	6.712	1760	1764	1765	rBV3	1309	767	0.10%	0.012%
35	6.809	1790	1794	1798	rVB7	1623	1287	0.17%	0.021%
36	6.921	1819	1829	1846	rBV	82070	155329	20.27%	2.514%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030743.D
 Acq On : 21 Apr 2023 02:04
 Operator : SY/MD
 Sample : 02440-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.104	1884	1886	1890	rBV5	1140	688	0.09%	0.011%
38	7.201	1913	1916	1917	rBV3	1455	561	0.07%	0.009%
39	7.252	1920	1932	1952	rBV	320308	572033	74.66%	9.258%
40	7.448	1989	1993	1995	rBV4	1940	1464	0.19%	0.024%
41	7.503	2008	2010	2014	rBV5	1072	772	0.10%	0.012%
42	7.561	2019	2028	2042	rVV	62442	108241	14.13%	1.752%
43	8.034	2161	2175	2204	rBV	163977	336078	43.86%	5.439%
44	8.423	2294	2296	2299	rBV3	1134	808	0.11%	0.013%
45	8.583	2344	2346	2349	rBV3	1575	1166	0.15%	0.019%
46	8.616	2354	2356	2358	rBV3	1741	849	0.11%	0.014%
47	8.792	2400	2411	2437	rBV	426259	709024	92.54%	11.476%
48	9.008	2476	2478	2481	rVB4	2248	1175	0.15%	0.019%
49	9.024	2481	2483	2484	rBV2	1566	637	0.08%	0.010%
50	9.050	2488	2491	2494	rBV5	1372	1096	0.14%	0.018%
51	9.243	2549	2551	2554	rBV4	1356	632	0.08%	0.010%
52	9.468	2617	2621	2623	rBV5	1408	1007	0.13%	0.016%
53	9.526	2637	2639	2643	rBV5	1401	1088	0.14%	0.018%
54	9.947	2767	2770	2771	rBV3	1226	624	0.08%	0.010%
55	10.098	2813	2817	2821	rBV5	2402	2401	0.31%	0.039%
56	10.162	2826	2837	2853	rVV	232666	370850	48.40%	6.002%
57	10.288	2874	2876	2879	rBV4	1268	631	0.08%	0.010%
58	10.304	2879	2881	2882	rBV2	1235	564	0.07%	0.009%
59	10.358	2896	2898	2901	rBV3	1453	1157	0.15%	0.019%
60	10.484	2932	2937	2940	rBV6	1968	2018	0.26%	0.033%
61	10.554	2957	2959	2962	rBV3	1231	770	0.10%	0.012%
62	10.596	2967	2972	2973	rBV5	1367	1073	0.14%	0.017%
63	10.728	3009	3013	3015	rBV4	1391	972	0.13%	0.016%
64	10.738	3015	3016	3020	rBV4	914	622	0.08%	0.010%
65	10.821	3037	3042	3044	rBV6	1313	1228	0.16%	0.020%
66	10.863	3053	3055	3058	rVB4	1452	694	0.09%	0.011%
67	10.882	3058	3061	3066	rBV4	1582	1314	0.17%	0.021%
68	10.992	3091	3095	3098	rBV6	1540	1073	0.14%	0.017%
69	11.107	3129	3131	3134	rBV4	983	694	0.09%	0.011%
70	11.194	3147	3158	3178	rBV	408865	650120	84.85%	10.522%
71	11.378	3211	3215	3217	rBV5	1544	1160	0.15%	0.019%
72	11.487	3246	3249	3251	rBV4	1092	834	0.11%	0.013%
73	11.509	3254	3256	3259	rBV4	1527	848	0.11%	0.014%
74	11.570	3263	3275	3292	rVV	333127	538312	70.26%	8.713%
75	11.802	3343	3347	3348	rBV4	1167	689	0.09%	0.011%
76	11.898	3374	3377	3381	rBV6	1307	1179	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030743.D
 Acq On : 21 Apr 2023 02:04
 Operator : SY/MD
 Sample : 02440-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.995	3405	3407	3409	rBV3	1475	717	0.09%	0.012%
78	12.030	3415	3418	3420	rBV3	1345	780	0.10%	0.013%
79	12.069	3427	3430	3435	rBV7	1529	1595	0.21%	0.026%
80	12.300	3499	3502	3506	rBV4	1643	1137	0.15%	0.018%
81	12.320	3506	3508	3509	rBV2	1711	866	0.11%	0.014%
82	12.384	3526	3528	3535	rVB6	1092	636	0.08%	0.010%
83	12.503	3561	3565	3567	rBV5	1321	1119	0.15%	0.018%
84	12.545	3574	3578	3579	rBV4	1339	906	0.12%	0.015%
85	12.625	3601	3603	3606	rVV4	2297	942	0.12%	0.015%
86	12.651	3609	3611	3616	rBV5	1354	1192	0.16%	0.019%
87	12.779	3647	3651	3655	rVB6	1870	1167	0.15%	0.019%
88	12.943	3700	3702	3705	rBV3	1546	1035	0.14%	0.017%
89	13.008	3718	3722	3725	rVB4	998	671	0.09%	0.011%
90	13.027	3725	3728	3731	rBV4	1330	1114	0.15%	0.018%
91	13.207	3781	3784	3785	rBV2	1780	809	0.11%	0.013%
92	13.265	3799	3802	3803	rBV3	1144	670	0.09%	0.011%
93	13.503	3874	3876	3879	rBV4	1381	753	0.10%	0.012%
94	13.805	3968	3970	3973	rBV4	1622	1023	0.13%	0.017%
95	13.844	3980	3982	3985	rBV4	1724	994	0.13%	0.016%
96	13.943	4012	4013	4018	rVB4	1366	1042	0.14%	0.017%
97	14.268	4112	4114	4117	rBV4	995	545	0.07%	0.009%
98	14.422	4160	4162	4165	rBV4	1694	560	0.07%	0.009%
99	14.548	4198	4201	4202	rBV3	1222	810	0.11%	0.013%
100	14.892	4305	4308	4312	rBV6	1628	1309	0.17%	0.021%




Sum of corrected areas: 6178488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030743.D
Acq On : 21 Apr 2023 02:04
Operator : SY/MD
Sample : 02440-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

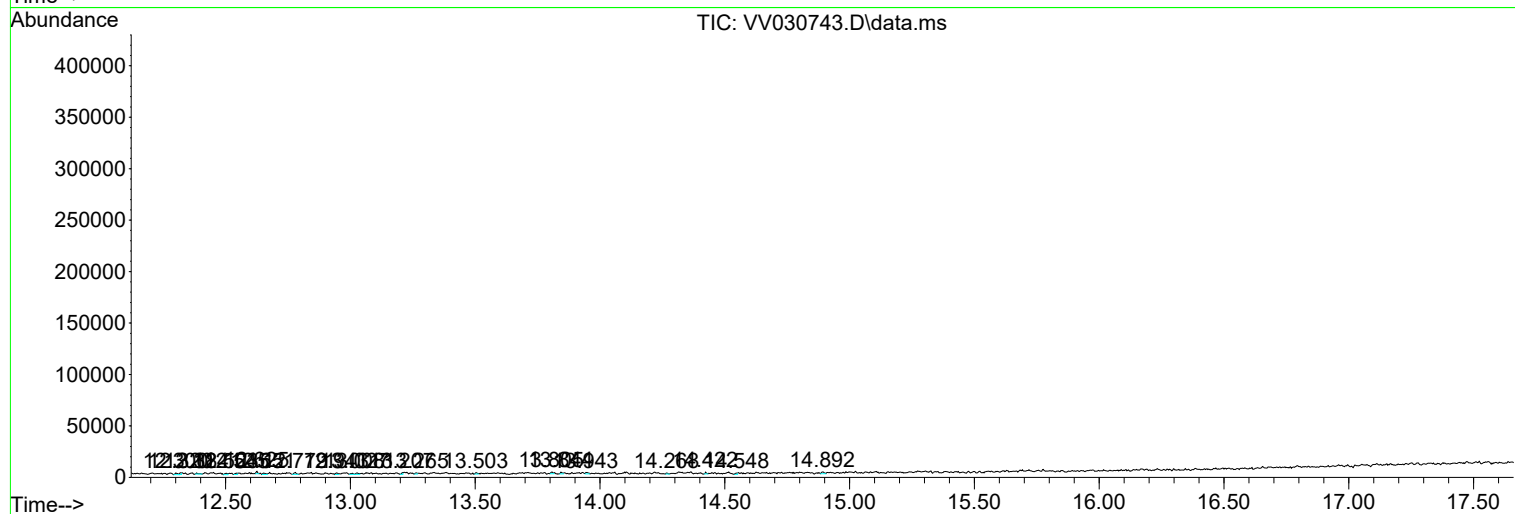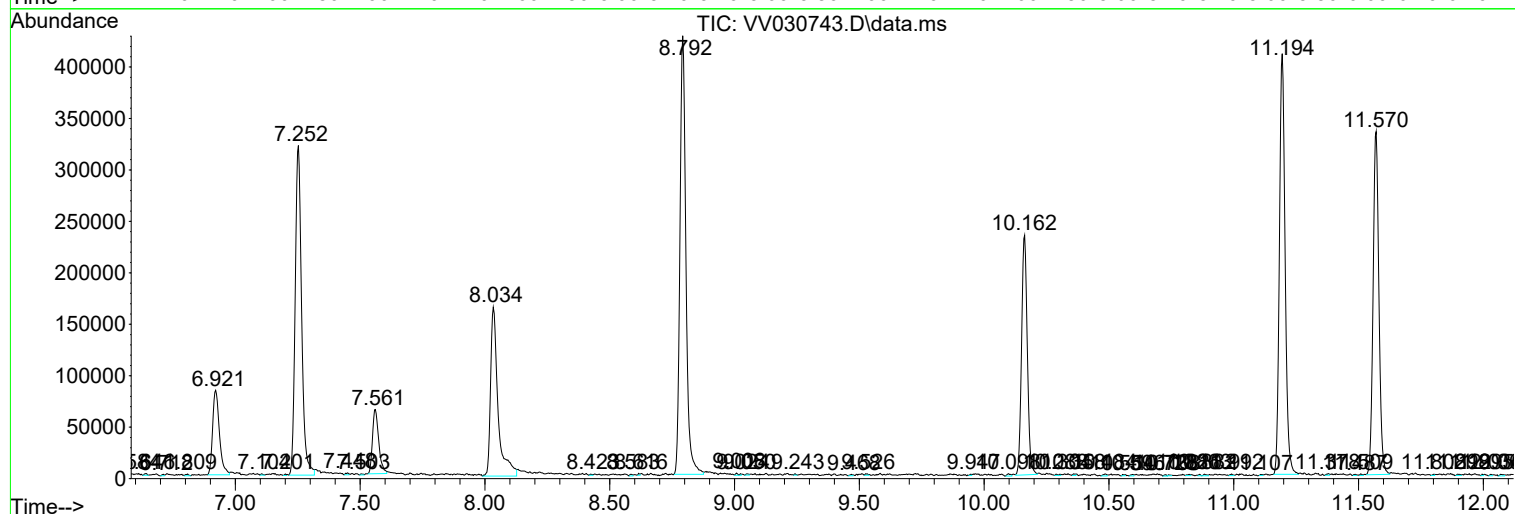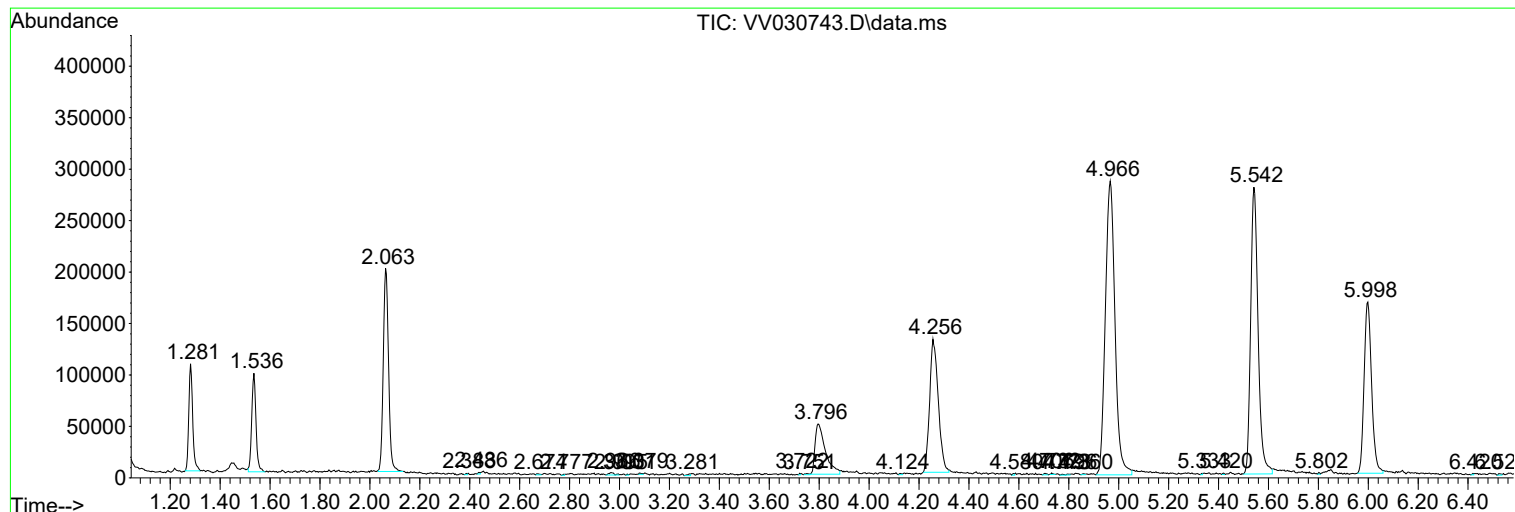

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030743.D
Acq On : 21 Apr 2023 02:04
Operator : SY/MD
Sample : 02440-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030743.D
Acq On : 21 Apr 2023 02:04
Operator : SY/MD
Sample : 02440-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc