

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030744.D
 Acq On : 21 Apr 2023 02:29
 Operator : SY/MD
 Sample : 02440-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rBV	103382	110604	14.78%	1.803%
2	1.532	147	153	167	rVB	91933	111973	14.97%	1.825%
3	2.063	310	318	334	rVB	198030	286806	38.33%	4.675%
4	2.384	416	418	422	rVB5	1250	716	0.10%	0.012%
5	2.455	435	440	445	rBV7	2629	3155	0.42%	0.051%
6	2.513	456	458	462	rVB5	2074	1488	0.20%	0.024%
7	2.732	523	526	530	rBV5	1090	1033	0.14%	0.017%
8	2.780	538	541	543	rBV4	1595	727	0.10%	0.012%
9	2.854	560	564	568	rBV7	1466	1094	0.15%	0.018%
10	2.889	571	575	578	rBV6	1504	1472	0.20%	0.024%
11	3.008	610	612	617	rVB6	1534	839	0.11%	0.014%
12	3.169	658	662	664	rBV4	941	956	0.13%	0.016%
13	3.346	715	717	721	rVB6	1785	1101	0.15%	0.018%
14	3.375	721	726	729	rBV6	1483	1374	0.18%	0.022%
15	3.410	734	737	741	rBV5	1661	1412	0.19%	0.023%
16	3.510	766	768	771	rVB4	1742	915	0.12%	0.015%
17	3.616	798	801	804	rBV5	1081	824	0.11%	0.013%
18	3.677	816	820	822	rBV5	1436	1225	0.16%	0.020%
19	3.796	848	857	879	rBV	51167	138647	18.53%	2.260%
20	4.031	925	930	933	rBV7	1444	1487	0.20%	0.024%
21	4.175	973	975	979	rBV4	1198	1028	0.14%	0.017%
22	4.259	987	1001	1025	rBV2	120767	307623	41.11%	5.015%
23	4.503	1075	1077	1078	rBV2	1869	868	0.12%	0.014%
24	4.658	1120	1125	1126	rBV5	1457	1104	0.15%	0.018%
25	4.690	1133	1135	1137	rBV3	2410	1381	0.18%	0.023%
26	4.806	1168	1171	1175	rVB5	1147	893	0.12%	0.015%
27	4.873	1186	1192	1196	rBV8	1885	2433	0.33%	0.040%
28	4.966	1204	1221	1248	rBV3	281896	748221	100.00%	12.197%
29	5.394	1349	1354	1355	rBV4	1180	984	0.13%	0.016%
30	5.542	1387	1400	1421	rBV	277500	580042	77.52%	9.455%
31	5.998	1527	1542	1562	rBV2	168103	350743	46.88%	5.718%
32	6.146	1586	1588	1589	rBV2	1615	691	0.09%	0.011%
33	6.388	1661	1663	1666	rVB4	1963	852	0.11%	0.014%
34	6.426	1672	1675	1681	rVB8	1219	1203	0.16%	0.020%
35	6.458	1681	1685	1695	rVB8	1402	2288	0.31%	0.037%
36	6.513	1698	1702	1704	rBV4	1178	938	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030744.D
 Acq On : 21 Apr 2023 02:29
 Operator : SY/MD
 Sample : 02440-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.744	1772	1774	1777	rBV3	1266	816	0.11%	0.013%
38	6.847	1801	1806	1808	rBV6	1861	1370	0.18%	0.022%
39	6.921	1819	1829	1856	rBV	83274	159040	21.26%	2.593%
40	7.130	1891	1894	1897	rBV4	1835	1626	0.22%	0.027%
41	7.172	1905	1907	1911	rBV5	1345	914	0.12%	0.015%
42	7.252	1920	1932	1956	rBV	312116	561623	75.06%	9.155%
43	7.478	1997	2002	2004	rBV6	1383	1147	0.15%	0.019%
44	7.561	2020	2028	2042	rBV2	58044	98437	13.16%	1.605%
45	7.725	2075	2079	2080	rBV4	1632	1020	0.14%	0.017%
46	7.899	2131	2133	2137	rVB4	1881	1247	0.17%	0.020%
47	7.998	2161	2164	2165	rBV3	1534	894	0.12%	0.015%
48	8.034	2165	2175	2191	rBV	163936	304596	40.71%	4.965%
49	8.452	2302	2305	2307	rVB4	1462	806	0.11%	0.013%
50	8.603	2351	2352	2357	rBV4	1839	1309	0.17%	0.021%
51	8.715	2385	2387	2391	rBV5	943	747	0.10%	0.012%
52	8.793	2399	2411	2430	rBV	433466	714982	95.56%	11.655%
53	9.346	2580	2583	2584	rBV3	1136	688	0.09%	0.011%
54	9.625	2667	2670	2673	rBV4	1139	673	0.09%	0.011%
55	9.641	2673	2675	2677	rVB3	1686	794	0.11%	0.013%
56	9.657	2677	2680	2682	rBV3	1759	1066	0.14%	0.017%
57	9.728	2698	2702	2707	rBV7	1286	1671	0.22%	0.027%
58	9.789	2717	2721	2726	rBV7	879	867	0.12%	0.014%
59	9.886	2748	2751	2755	rVB6	1255	980	0.13%	0.016%
60	9.966	2774	2776	2780	rBV5	1044	808	0.11%	0.013%
61	10.159	2825	2836	2854	rBV	225457	367740	49.15%	5.995%
62	10.317	2883	2885	2889	rBV5	1793	1204	0.16%	0.020%
63	10.484	2932	2937	2939	rBV7	1488	1396	0.19%	0.023%
64	10.526	2947	2950	2955	rBV7	1526	858	0.11%	0.014%
65	10.699	3000	3004	3006	rBV5	904	734	0.10%	0.012%
66	10.802	3033	3036	3041	rBV7	1399	885	0.12%	0.014%
67	10.937	3075	3078	3081	rBV4	1456	917	0.12%	0.015%
68	10.953	3081	3083	3085	rBV3	1708	916	0.12%	0.015%
69	10.992	3093	3095	3098	rVB4	1636	820	0.11%	0.013%
70	11.024	3100	3105	3109	rVV7	1219	1174	0.16%	0.019%
71	11.101	3126	3129	3132	rVB5	1183	803	0.11%	0.013%
72	11.124	3134	3136	3139	rBV3	1730	1194	0.16%	0.019%
73	11.194	3144	3158	3179	rBV	408010	661671	88.43%	10.786%
74	11.439	3231	3234	3236	rBV3	1526	1117	0.15%	0.018%
75	11.487	3247	3249	3255	rVB6	1374	1288	0.17%	0.021%
76	11.516	3255	3258	3261	rBV4	2000	1412	0.19%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030744.D
 Acq On : 21 Apr 2023 02:29
 Operator : SY/MD
 Sample : 02440-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.567	3261	3274	3290	rBV	333952	536056	71.64%	8.738%
78	11.915	3379	3382	3390	rBV9	2109	2312	0.31%	0.038%
79	11.953	3392	3394	3397	rVB5	1693	959	0.13%	0.016%
80	12.030	3415	3418	3421	rBV3	1302	944	0.13%	0.015%
81	12.217	3473	3476	3478	rBV4	1875	1116	0.15%	0.018%
82	12.272	3491	3493	3496	rBV4	1367	728	0.10%	0.012%
83	12.426	3538	3541	3544	rBV5	1232	1081	0.14%	0.018%
84	12.542	3574	3577	3580	rBV4	1281	767	0.10%	0.013%
85	12.574	3583	3587	3592	rVV7	2009	1630	0.22%	0.027%
86	12.645	3606	3609	3613	rBV5	1645	1204	0.16%	0.020%
87	12.825	3663	3665	3668	rBV4	1212	778	0.10%	0.013%
88	12.889	3683	3685	3692	rVB7	1929	1481	0.20%	0.024%
89	12.918	3692	3694	3697	rBV2	1385	888	0.12%	0.014%
90	12.953	3701	3705	3707	rBV5	1781	1314	0.18%	0.021%
91	12.995	3715	3718	3721	rBV5	1627	1047	0.14%	0.017%
92	13.358	3826	3831	3833	rBV5	1494	1237	0.17%	0.020%
93	13.567	3893	3896	3898	rBV4	1305	859	0.11%	0.014%
94	13.789	3963	3965	3969	rBV5	1719	1315	0.18%	0.021%
95	13.905	3996	4001	4003	rBV6	1393	1293	0.17%	0.021%
96	14.043	4041	4044	4047	rBV5	1500	1047	0.14%	0.017%
97	14.365	4142	4144	4147	rBV3	1360	898	0.12%	0.015%
98	14.564	4200	4206	4209	rBV7	1658	1612	0.22%	0.026%
99	14.841	4289	4292	4296	rVB6	1648	1521	0.20%	0.025%
100	14.931	4318	4320	4324	rBV3	1373	989	0.13%	0.016%




Sum of corrected areas: 6134466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030744.D
Acq On : 21 Apr 2023 02:29
Operator : SY/MD
Sample : 02440-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

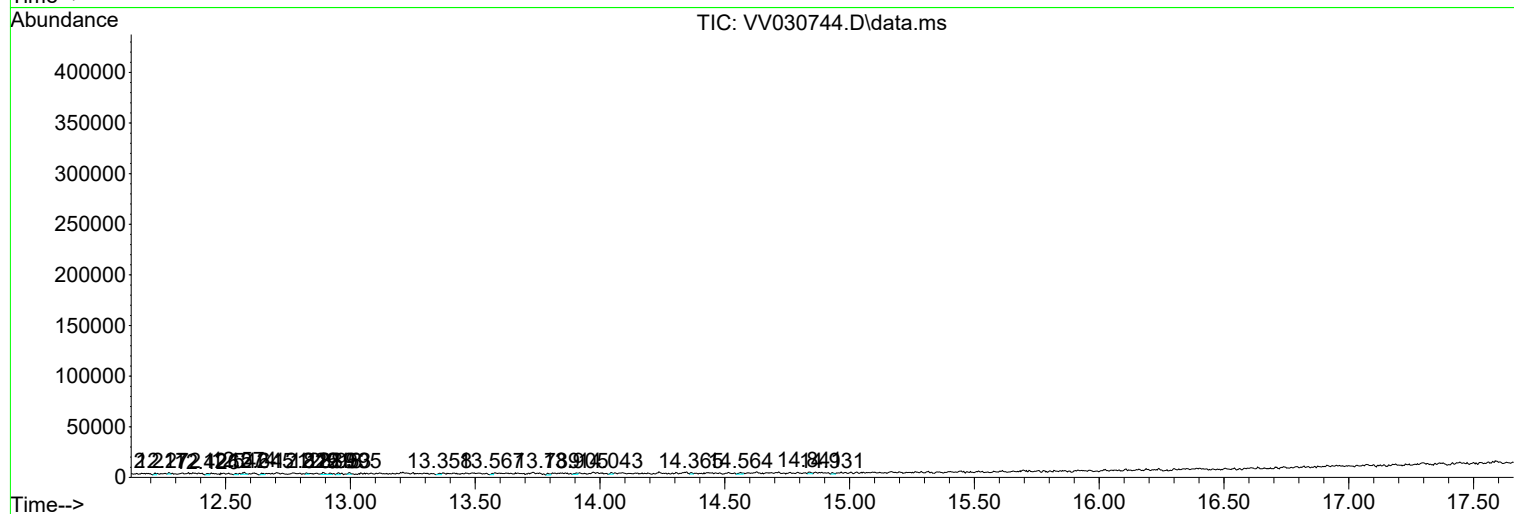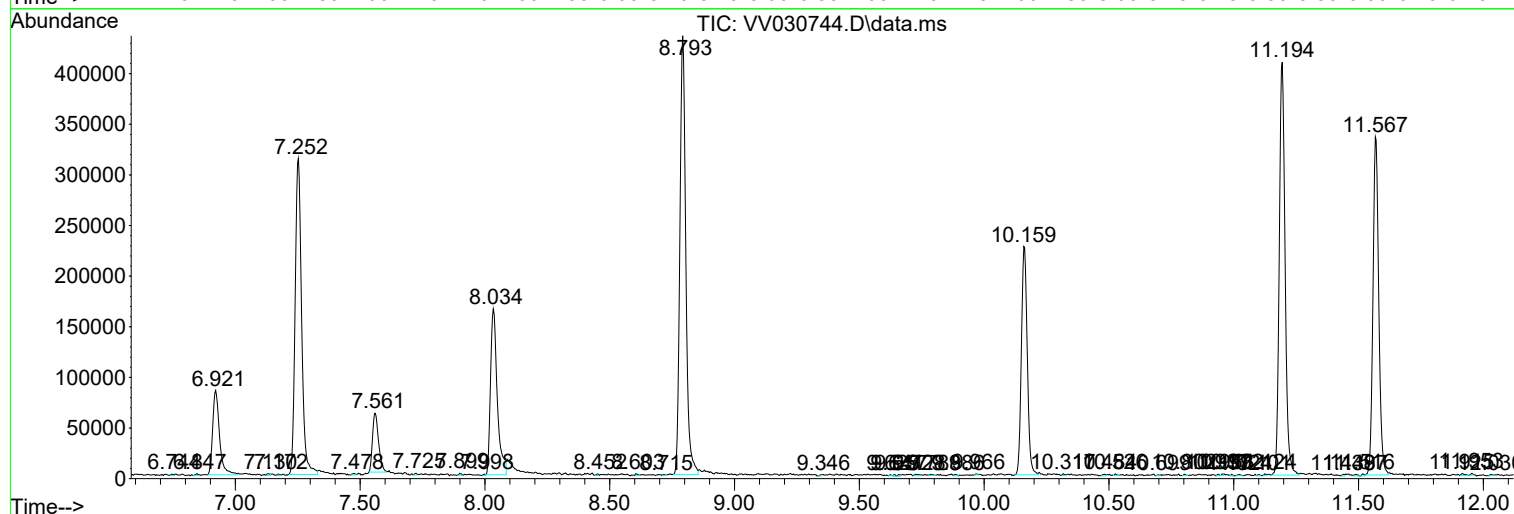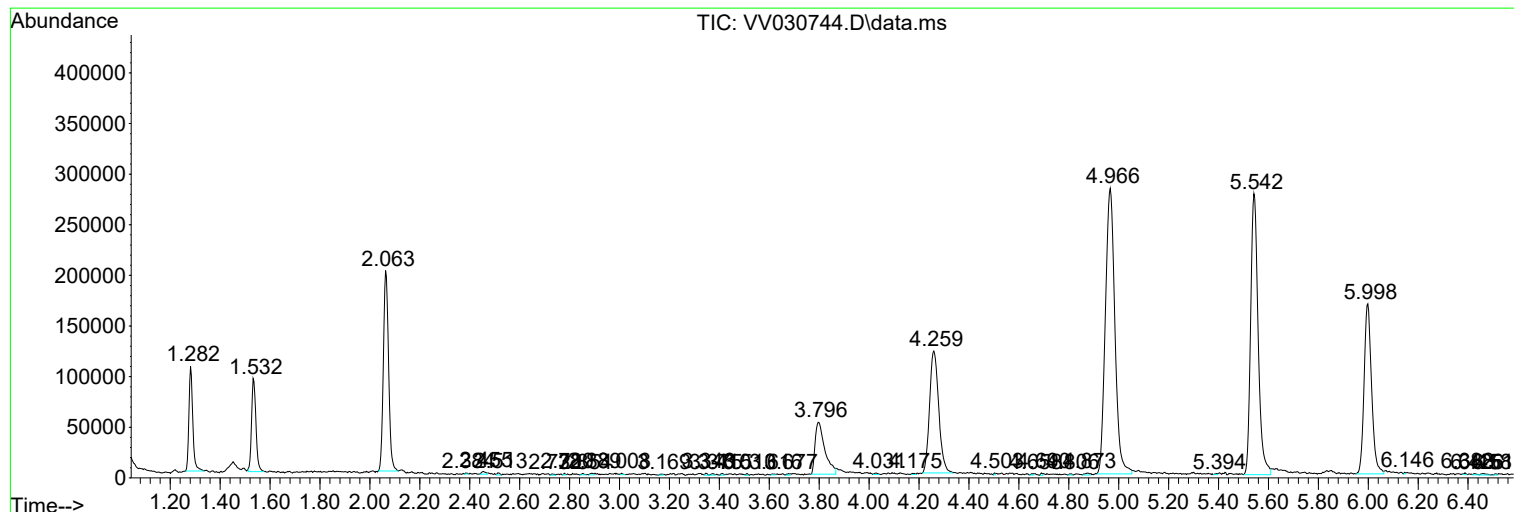

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030744.D
Acq On : 21 Apr 2023 02:29
Operator : SY/MD
Sample : 02440-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030744.D
Acq On : 21 Apr 2023 02:29
Operator : SY/MD
Sample : 02440-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc