

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030745.D
 Acq On : 21 Apr 2023 02:53
 Operator : SY/MD
 Sample : 02440-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	100961	108468	14.52%	1.784%
2	1.535	147	154	169	rVB	95868	114032	15.27%	1.875%
3	2.063	309	318	330	rBV	195886	285671	38.24%	4.697%
4	2.214	361	365	368	rVB6	1126	962	0.13%	0.016%
5	2.233	368	371	373	rBV3	1607	839	0.11%	0.014%
6	2.407	423	425	427	rBV3	951	474	0.06%	0.008%
7	2.436	431	434	435	rBV3	1548	717	0.10%	0.012%
8	2.452	435	439	447	rVV9	3498	4692	0.63%	0.077%
9	2.793	542	545	548	rBV5	1370	984	0.13%	0.016%
10	2.825	553	555	559	rVB4	1305	680	0.09%	0.011%
11	2.844	559	561	563	rBV3	952	584	0.08%	0.010%
12	2.918	581	584	585	rBV3	1350	871	0.12%	0.014%
13	2.937	589	590	594	rVV4	1710	970	0.13%	0.016%
14	3.310	702	706	708	rVB4	1245	848	0.11%	0.014%
15	3.323	708	710	711	rBV2	1321	517	0.07%	0.009%
16	3.359	719	721	723	rBV3	1242	638	0.09%	0.010%
17	3.445	745	748	751	rBV5	1149	753	0.10%	0.012%
18	3.465	751	754	755	rBV3	1156	616	0.08%	0.010%
19	3.545	777	779	782	rBV3	1200	644	0.09%	0.011%
20	3.609	796	799	801	rBV4	1260	926	0.12%	0.015%
21	3.796	849	857	877	rBV	49181	128845	17.25%	2.119%
22	4.104	951	953	955	rBV4	1355	645	0.09%	0.011%
23	4.259	987	1001	1019	rBV	123502	310227	41.53%	5.101%
24	4.532	1083	1086	1089	rBV5	1641	1222	0.16%	0.020%
25	4.693	1134	1136	1138	rBV3	1134	498	0.07%	0.008%
26	4.735	1147	1149	1153	rBV5	1490	882	0.12%	0.015%
27	4.815	1171	1174	1176	rBV4	1216	802	0.11%	0.013%
28	4.870	1188	1191	1196	rBV5	1566	1725	0.23%	0.028%
29	4.966	1204	1221	1243	rBV2	281235	747013	100.00%	12.283%
30	5.455	1368	1373	1376	rBV6	2428	1962	0.26%	0.032%
31	5.542	1387	1400	1418	rBV	275678	564185	75.53%	9.277%
32	5.995	1529	1541	1564	rBV	167751	347724	46.55%	5.718%
33	6.227	1609	1613	1616	rBV6	1377	1541	0.21%	0.025%
34	6.365	1653	1656	1658	rBV3	1548	912	0.12%	0.015%
35	6.458	1682	1685	1686	rBV2	1209	641	0.09%	0.011%
36	6.493	1694	1696	1697	rBV2	1075	506	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030745.D
 Acq On : 21 Apr 2023 02:53
 Operator : SY/MD
 Sample : 02440-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.561	1715	1717	1720	rBV4	1853	1175	0.16%	0.019%
38	6.661	1746	1748	1752	rBV4	1719	915	0.12%	0.015%
39	6.780	1782	1785	1787	rBV4	1480	729	0.10%	0.012%
40	6.863	1807	1811	1814	rBV6	1590	1584	0.21%	0.026%
41	6.921	1819	1829	1844	rBV	82791	155596	20.83%	2.558%
42	7.252	1920	1932	1947	rBV	313195	555961	74.42%	9.142%
43	7.561	2018	2028	2044	rBV3	61922	113311	15.17%	1.863%
44	7.821	2105	2109	2112	rBV6	1307	1224	0.16%	0.020%
45	7.960	2150	2152	2154	rBV4	1016	595	0.08%	0.010%
46	8.001	2162	2165	2166	rBV3	2022	1376	0.18%	0.023%
47	8.034	2166	2175	2205	rVV	163002	323237	43.27%	5.315%
48	8.638	2360	2363	2366	rBV5	1733	1247	0.17%	0.021%
49	8.792	2400	2411	2434	rBV	416426	696569	93.25%	11.454%
50	9.011	2477	2479	2482	rBV4	1473	973	0.13%	0.016%
51	9.345	2581	2583	2586	rBV4	974	593	0.08%	0.010%
52	9.403	2599	2601	2604	rBV4	1037	801	0.11%	0.013%
53	9.448	2611	2615	2616	rBV3	1188	719	0.10%	0.012%
54	9.940	2765	2768	2770	rBV4	1077	780	0.10%	0.013%
55	10.162	2825	2837	2852	rBV	227528	363183	48.62%	5.972%
56	10.419	2915	2917	2919	rBV3	1112	571	0.08%	0.009%
57	10.490	2934	2939	2940	rBV4	1495	1041	0.14%	0.017%
58	10.522	2947	2949	2952	rBV4	1185	538	0.07%	0.009%
59	10.558	2957	2960	2962	rBV4	895	604	0.08%	0.010%
60	10.599	2970	2973	2979	rBV8	1127	1269	0.17%	0.021%
61	10.628	2979	2982	2984	rBV4	844	587	0.08%	0.010%
62	10.731	3012	3014	3017	rBV4	836	568	0.08%	0.009%
63	10.808	3035	3038	3043	rVV7	1532	1319	0.18%	0.022%
64	10.992	3092	3095	3096	rBV3	982	626	0.08%	0.010%
65	11.056	3112	3115	3121	rVB6	1581	1571	0.21%	0.026%
66	11.082	3121	3123	3126	rBV4	1552	908	0.12%	0.015%
67	11.194	3143	3158	3178	rBV	402091	649203	86.91%	10.675%
68	11.358	3207	3209	3212	rVB3	1455	622	0.08%	0.010%
69	11.416	3224	3227	3228	rBV2	1269	661	0.09%	0.011%
70	11.471	3241	3244	3245	rBV3	1513	754	0.10%	0.012%
71	11.567	3262	3274	3290	rBV	328542	533532	71.42%	8.773%
72	11.744	3326	3329	3334	rVB7	2054	1556	0.21%	0.026%
73	11.808	3345	3349	3350	rBV4	1334	1061	0.14%	0.017%
74	11.818	3350	3352	3355	rVB4	1807	836	0.11%	0.014%
75	11.927	3383	3386	3388	rVB4	1735	899	0.12%	0.015%
76	11.953	3391	3394	3395	rBV3	1111	495	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030745.D
 Acq On : 21 Apr 2023 02:53
 Operator : SY/MD
 Sample : 02440-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.021	3411	3415	3417	rBV4	1431	1020	0.14%	0.017%
78	12.316	3502	3507	3509	rBV5	1642	1433	0.19%	0.024%
79	12.503	3562	3565	3569	rBV6	1632	1380	0.18%	0.023%
80	12.673	3615	3618	3619	rBV3	1201	718	0.10%	0.012%
81	12.715	3628	3631	3634	rBV4	1477	1079	0.14%	0.018%
82	12.812	3658	3661	3664	rBV4	1379	898	0.12%	0.015%
83	12.876	3679	3681	3684	rVB5	1598	681	0.09%	0.011%
84	12.898	3684	3688	3692	rBV6	2365	2083	0.28%	0.034%
85	12.969	3707	3710	3712	rBV3	1440	854	0.11%	0.014%
86	13.017	3722	3725	3726	rBV3	1022	555	0.07%	0.009%
87	13.204	3779	3783	3784	rBV4	1120	692	0.09%	0.011%
88	13.294	3804	3811	3814	rVV8	1803	1980	0.27%	0.033%
89	13.316	3817	3818	3821	rBV3	1771	885	0.12%	0.015%
90	13.374	3832	3836	3839	rVB5	2059	1505	0.20%	0.025%
91	13.432	3851	3854	3855	rBV3	1338	776	0.10%	0.013%
92	13.461	3860	3863	3866	rBV4	1072	885	0.12%	0.015%
93	13.811	3969	3972	3974	rBV4	1406	937	0.13%	0.015%
94	13.947	4012	4014	4016	rVB3	1470	777	0.10%	0.013%
95	13.985	4024	4026	4030	rVB4	1505	723	0.10%	0.012%
96	14.165	4077	4082	4091	rBV9	2685	4086	0.55%	0.067%
97	14.201	4091	4093	4095	rVB3	1197	614	0.08%	0.010%
98	14.393	4151	4153	4156	rBV4	1501	717	0.10%	0.012%
99	14.467	4174	4176	4178	rBV3	1045	494	0.07%	0.008%
100	14.995	4337	4340	4346	rBV8	1852	1824	0.24%	0.030%




Sum of corrected areas: 6081601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030745.D
Acq On : 21 Apr 2023 02:53
Operator : SY/MD
Sample : 02440-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

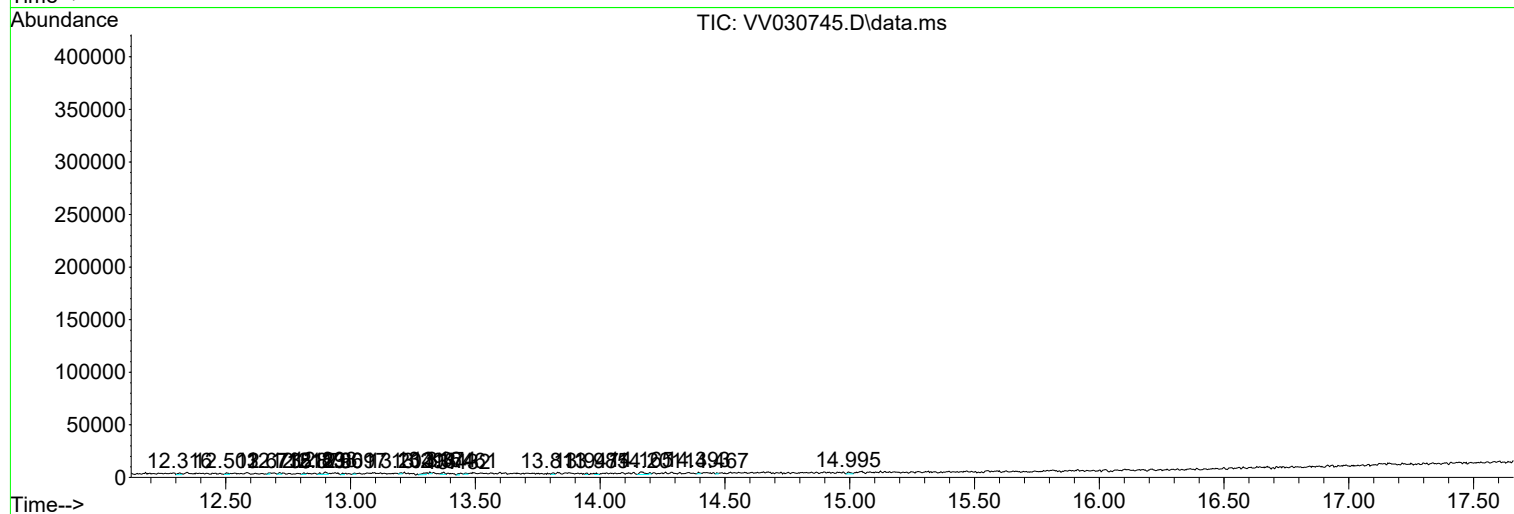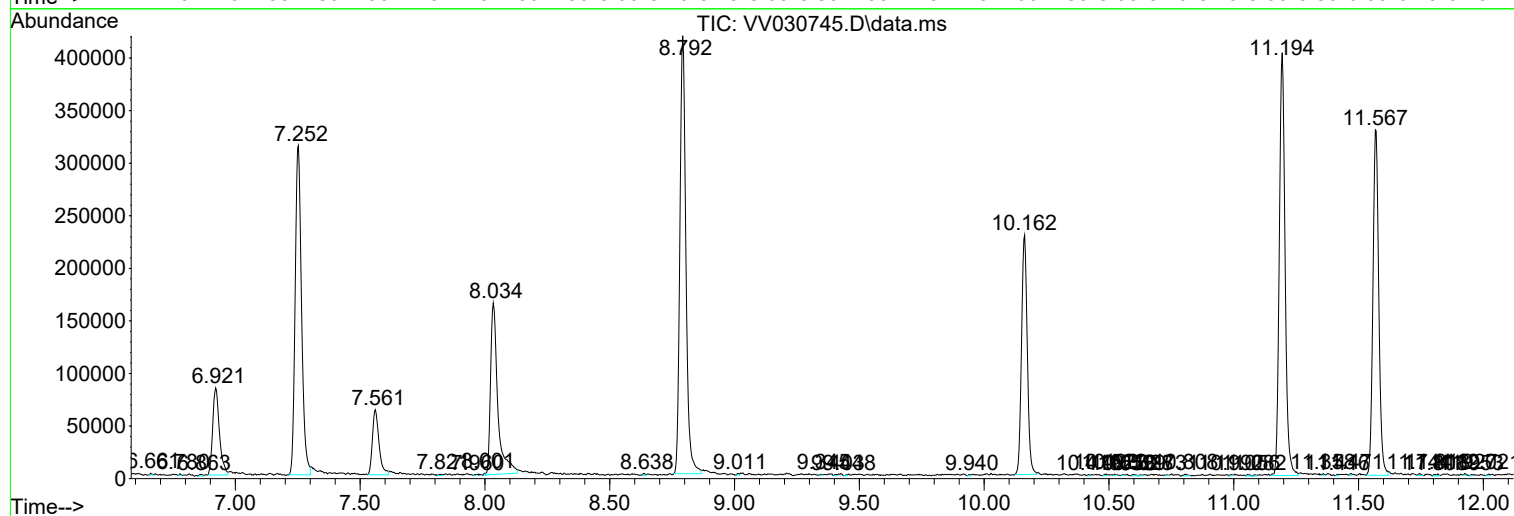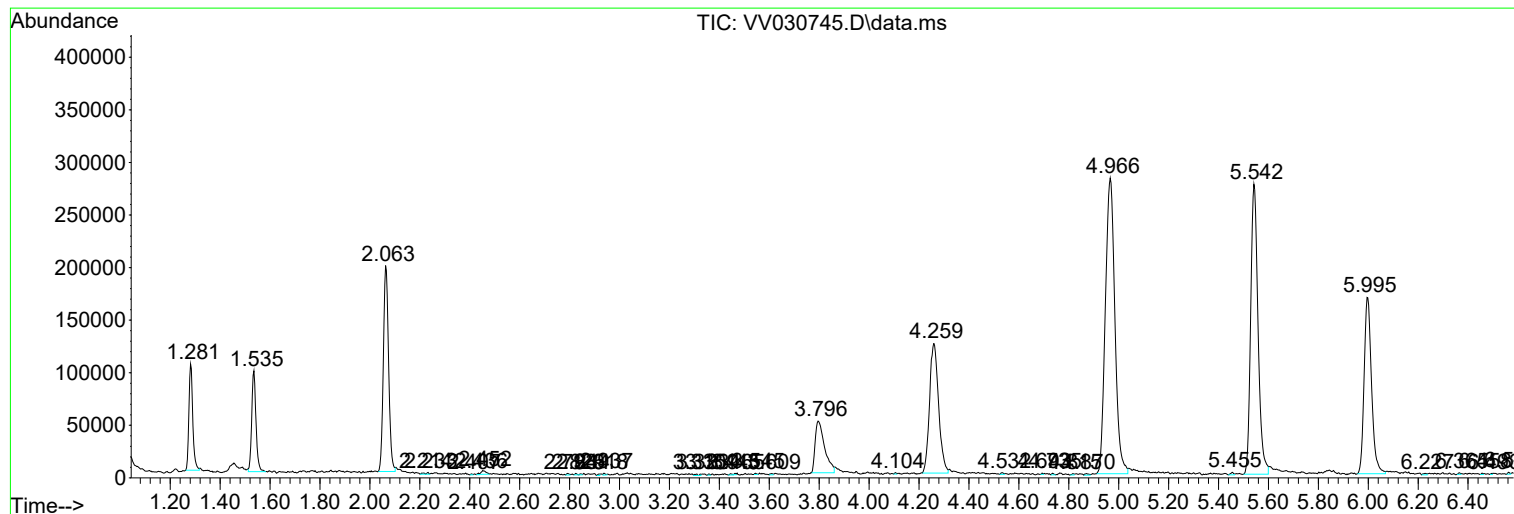

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030745.D
Acq On : 21 Apr 2023 02:53
Operator : SY/MD
Sample : 02440-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030745.D
Acq On : 21 Apr 2023 02:53
Operator : SY/MD
Sample : 02440-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc