

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030746.D
 Acq On : 21 Apr 2023 03:17
 Operator : SY/MD
 Sample : 02440-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	103175	112505	13.67%	1.741%
2	1.536	148	154	170	rVB	95219	114250	13.88%	1.768%
3	2.063	310	318	331	rVB	196766	279615	33.98%	4.327%
4	2.417	426	428	430	rVB3	1524	583	0.07%	0.009%
5	2.587	479	481	484	rBV4	809	613	0.07%	0.009%
6	2.712	518	520	522	rVB3	1409	474	0.06%	0.007%
7	2.744	528	530	534	rBV5	1568	843	0.10%	0.013%
8	2.764	534	536	538	rVB3	1109	435	0.05%	0.007%
9	2.777	538	540	541	rBV2	1470	668	0.08%	0.010%
10	2.815	550	552	558	rVB6	1612	1044	0.13%	0.016%
11	2.847	560	562	564	rBV3	1027	458	0.06%	0.007%
12	2.947	588	593	594	rBV4	1244	996	0.12%	0.015%
13	3.002	606	610	614	rBV6	1046	921	0.11%	0.014%
14	3.027	614	618	624	rBV8	1051	1361	0.17%	0.021%
15	3.111	641	644	646	rBV3	1145	710	0.09%	0.011%
16	3.159	655	659	663	rBV6	1743	1639	0.20%	0.025%
17	3.256	687	689	691	rBV3	1022	449	0.05%	0.007%
18	3.349	715	718	720	rBV4	1310	743	0.09%	0.011%
19	3.439	743	746	749	rBV3	1577	1183	0.14%	0.018%
20	3.513	763	769	770	rBV4	1482	995	0.12%	0.015%
21	3.587	790	792	793	rBV2	1378	501	0.06%	0.008%
22	3.703	823	828	832	rBV6	2087	2087	0.25%	0.032%
23	3.735	836	838	844	rVB6	1331	1005	0.12%	0.016%
24	3.799	849	858	883	rVV	49189	135179	16.43%	2.092%
25	4.259	989	1001	1024	rVB	123807	311506	37.85%	4.820%
26	4.683	1130	1133	1134	rBV3	1873	968	0.12%	0.015%
27	4.834	1177	1180	1181	rBV2	630	379	0.05%	0.006%
28	4.966	1203	1221	1248	rBV3	285655	765318	92.99%	11.842%
29	5.542	1388	1400	1424	rBV	269576	563422	68.46%	8.718%
30	5.998	1530	1542	1565	rBV2	168187	345573	41.99%	5.347%
31	6.265	1621	1625	1627	rBV4	1581	1335	0.16%	0.021%
32	6.375	1656	1659	1662	rBV4	1381	988	0.12%	0.015%
33	6.471	1686	1689	1692	rBV4	1376	932	0.11%	0.014%
34	6.564	1716	1718	1721	rBV3	2125	1364	0.17%	0.021%
35	6.603	1728	1730	1732	rBV3	1126	502	0.06%	0.008%
36	6.773	1780	1783	1789	rVB7	1891	1588	0.19%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030746.D
 Acq On : 21 Apr 2023 03:17
 Operator : SY/MD
 Sample : 02440-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.799	1789	1791	1792	rBV2	1235	508	0.06%	0.008%
38	6.822	1796	1798	1800	rBV3	1466	588	0.07%	0.009%
39	6.921	1818	1829	1846	rBV	84218	159381	19.37%	2.466%
40	7.252	1920	1932	1954	rBV	316875	567619	68.97%	8.783%
41	7.561	2020	2028	2042	rBV2	59645	100118	12.17%	1.549%
42	8.034	2164	2175	2190	rBV	164049	305135	37.08%	4.721%
43	8.481	2311	2314	2318	rVB6	1528	1095	0.13%	0.017%
44	8.500	2318	2320	2321	rBV2	1067	534	0.06%	0.008%
45	8.670	2369	2373	2376	rBV6	1428	1138	0.14%	0.018%
46	8.793	2400	2411	2433	rBV	420618	714153	86.78%	11.050%
47	9.165	2525	2527	2529	rBV3	1130	566	0.07%	0.009%
48	9.336	2578	2580	2582	rBV3	1313	693	0.08%	0.011%
49	9.506	2631	2633	2634	rBV2	1112	377	0.05%	0.006%
50	9.574	2652	2654	2659	rBV5	1377	877	0.11%	0.014%
51	9.747	2706	2708	2710	rBV4	1853	1038	0.13%	0.016%
52	9.879	2747	2749	2753	rBV5	1131	709	0.09%	0.011%
53	10.024	2792	2794	2796	rBV3	1147	560	0.07%	0.009%
54	10.159	2825	2836	2856	rBV	228780	376278	45.72%	5.822%
55	10.362	2897	2899	2902	rVB4	2272	930	0.11%	0.014%
56	10.381	2902	2905	2908	rVB5	1409	1131	0.14%	0.018%
57	10.410	2910	2914	2917	rBV4	1085	958	0.12%	0.015%
58	10.436	2920	2922	2925	rVB3	1596	679	0.08%	0.011%
59	10.452	2925	2927	2930	rBV4	753	516	0.06%	0.008%
60	10.471	2930	2933	2935	rBV4	1755	1493	0.18%	0.023%
61	10.529	2947	2951	2952	rBV4	847	644	0.08%	0.010%
62	10.664	2990	2993	2996	rBV6	1168	621	0.08%	0.010%
63	10.683	2996	2999	3001	rBV4	1554	714	0.09%	0.011%
64	10.751	3017	3020	3023	rBV4	1517	1099	0.13%	0.017%
65	10.789	3028	3032	3033	rBV4	1531	979	0.12%	0.015%
66	10.841	3046	3048	3050	rBV3	746	402	0.05%	0.006%
67	10.854	3050	3052	3054	rVV3	789	436	0.05%	0.007%
68	10.876	3056	3059	3060	rVV3	1229	791	0.10%	0.012%
69	10.895	3063	3065	3069	rVB5	1606	927	0.11%	0.014%
70	10.944	3076	3080	3081	rBV4	1281	665	0.08%	0.010%
71	11.037	3106	3109	3111	rBV3	1193	824	0.10%	0.013%
72	11.194	3147	3158	3179	rBV	410377	689493	83.78%	10.669%
73	11.461	3239	3241	3242	rBV2	1160	502	0.06%	0.008%
74	11.571	3264	3275	3297	rBV2	386818	822984	100.00%	12.734%
75	11.802	3345	3347	3350	rVB4	2181	1128	0.14%	0.017%
76	11.870	3366	3368	3372	rVB5	2082	1196	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030746.D
 Acq On : 21 Apr 2023 03:17
 Operator : SY/MD
 Sample : 02440-15 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.985	3402	3404	3410	rVB5	1403	903	0.11%	0.014%
78	12.088	3434	3436	3437	rBV2	1253	448	0.05%	0.007%
79	12.165	3458	3460	3462	rBV3	1015	532	0.06%	0.008%
80	12.204	3469	3472	3474	rBV4	1157	758	0.09%	0.012%
81	12.217	3474	3476	3479	rVV4	994	635	0.08%	0.010%
82	12.288	3496	3498	3500	rBV3	822	393	0.05%	0.006%
83	12.455	3548	3550	3553	rVB4	1255	674	0.08%	0.010%
84	12.471	3553	3555	3558	rBV4	1336	863	0.10%	0.013%
85	12.554	3579	3581	3582	rBV2	894	390	0.05%	0.006%
86	12.596	3588	3594	3596	rBV5	1604	1492	0.18%	0.023%
87	12.696	3622	3625	3627	rBV4	716	500	0.06%	0.008%
88	12.751	3638	3642	3645	rBV5	1378	867	0.11%	0.013%
89	12.767	3645	3647	3652	rVB5	1092	731	0.09%	0.011%
90	13.062	3738	3739	3740	rBV	1077	370	0.04%	0.006%
91	13.210	3778	3785	3796	rVB4	19930	31612	3.84%	0.489%
92	13.284	3806	3808	3809	rBV2	1164	367	0.04%	0.006%
93	13.320	3816	3819	3824	rVB5	1858	1263	0.15%	0.020%
94	13.522	3879	3882	3883	rBV3	1294	679	0.08%	0.011%
95	13.596	3902	3905	3906	rBV3	1047	547	0.07%	0.008%
96	13.744	3947	3951	3955	rBV7	1617	1362	0.17%	0.021%
97	13.934	4005	4010	4013	rVB7	1868	1568	0.19%	0.024%
98	13.950	4013	4015	4017	rBV2	1171	628	0.08%	0.010%
99	14.345	4134	4138	4139	rBV3	1025	849	0.10%	0.013%
100	14.805	4278	4281	4282	rBV3	1955	803	0.10%	0.012%




Sum of corrected areas: 6462845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030746.D
Acq On : 21 Apr 2023 03:17
Operator : SY/MD
Sample : 02440-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMRO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

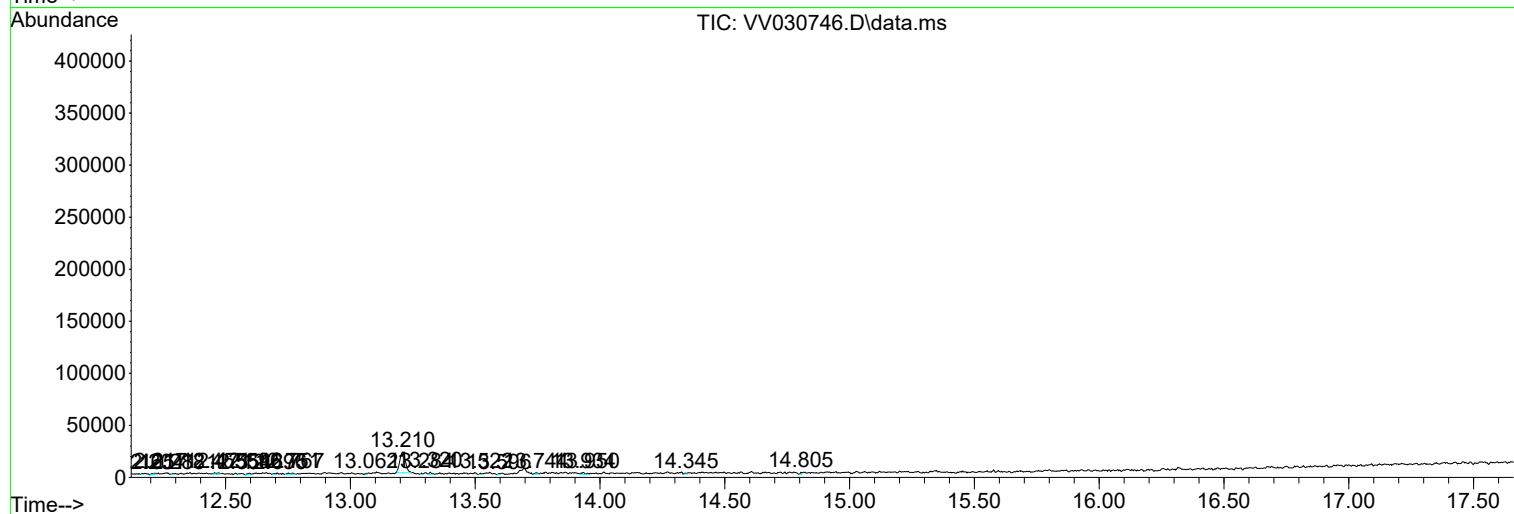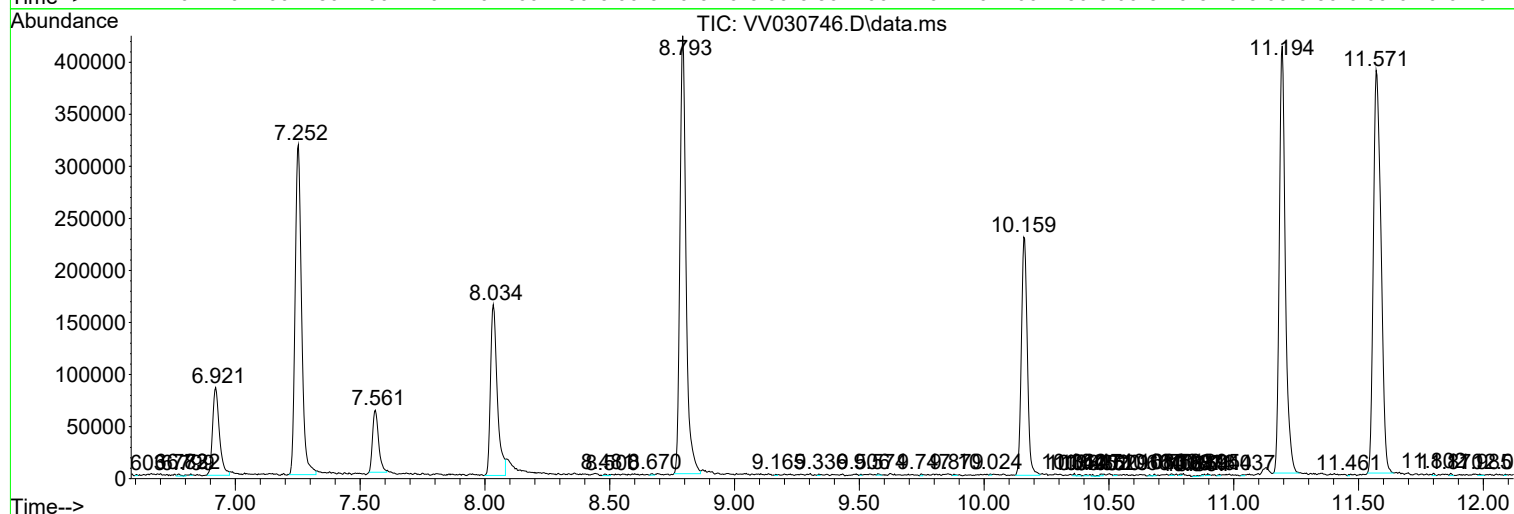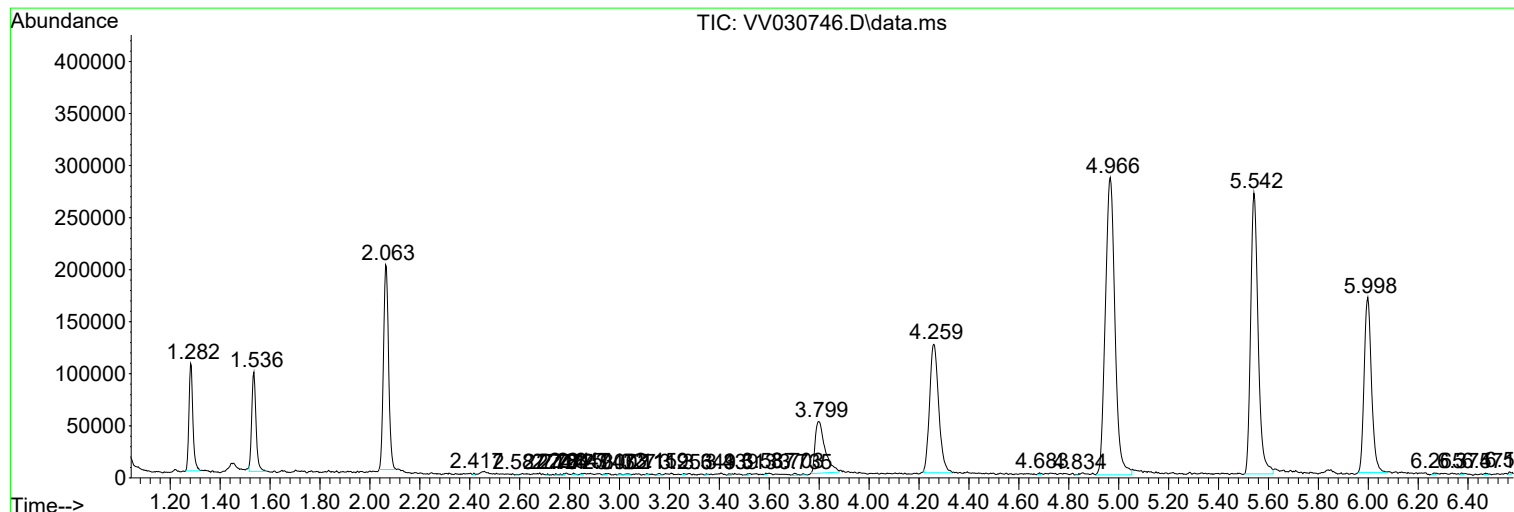

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030746.D
Acq On : 21 Apr 2023 03:17
Operator : SY/MD
Sample : 02440-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030746.D
Acq On : 21 Apr 2023 03:17
Operator : SY/MD
Sample : 02440-15 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc