

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030747.D
 Acq On : 21 Apr 2023 03:41
 Operator : SY/MD
 Sample : 02440-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rBV	101536	109465	14.77%	1.824%
2	1.536	147	154	169	rVB	88761	108934	14.70%	1.815%
3	2.063	309	318	330	rBV	191570	282014	38.05%	4.699%
4	2.224	364	368	369	rBV4	1099	927	0.13%	0.015%
5	2.407	423	425	429	rVB3	1716	1056	0.14%	0.018%
6	2.455	435	440	443	rBV7	2190	2236	0.30%	0.037%
7	2.526	458	462	463	rBV4	1798	1141	0.15%	0.019%
8	2.574	474	477	479	rVB3	1345	715	0.10%	0.012%
9	2.613	487	489	492	rVB4	1345	687	0.09%	0.011%
10	2.638	492	497	498	rBV4	1924	1313	0.18%	0.022%
11	2.687	508	512	515	rBV6	1804	1498	0.20%	0.025%
12	2.812	548	551	553	rBV4	1310	1064	0.14%	0.018%
13	2.960	595	597	600	rBV3	1701	970	0.13%	0.016%
14	3.027	613	618	619	rBV5	1212	821	0.11%	0.014%
15	3.066	628	630	633	rVB4	1666	745	0.10%	0.012%
16	3.118	642	646	650	rBV5	1798	1629	0.22%	0.027%
17	3.204	671	673	675	rBV3	1423	839	0.11%	0.014%
18	3.243	684	685	690	rVV4	1176	692	0.09%	0.012%
19	3.291	698	700	702	rBV3	1408	840	0.11%	0.014%
20	3.320	705	709	712	rBV7	1098	1051	0.14%	0.018%
21	3.384	723	729	731	rBV6	1807	1388	0.19%	0.023%
22	3.532	772	775	777	rBV4	1004	681	0.09%	0.011%
23	3.799	848	858	882	rBV	49051	141968	19.16%	2.366%
24	4.259	988	1001	1025	rVB	120913	300323	40.52%	5.004%
25	4.455	1056	1062	1065	rBV7	2034	2415	0.33%	0.040%
26	4.593	1101	1105	1108	rBV6	1783	1497	0.20%	0.025%
27	4.654	1121	1124	1127	rBV5	2010	1536	0.21%	0.026%
28	4.767	1157	1159	1162	rBV4	1288	860	0.12%	0.014%
29	4.818	1173	1175	1177	rBV3	1671	993	0.13%	0.017%
30	4.867	1186	1190	1192	rBV5	1319	932	0.13%	0.016%
31	4.966	1204	1221	1248	rBV2	273712	741143	100.00%	12.350%
32	5.449	1368	1371	1373	rBV3	1611	1186	0.16%	0.020%
33	5.542	1388	1400	1422	rBV	262850	548717	74.04%	9.144%
34	5.998	1529	1542	1558	rBV2	162287	334792	45.17%	5.579%
35	6.236	1614	1616	1618	rBV3	1467	680	0.09%	0.011%
36	6.304	1634	1637	1641	rBV5	1584	986	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030747.D
 Acq On : 21 Apr 2023 03:41
 Operator : SY/MD
 Sample : 02440-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.436	1676	1678	1681	rBV3	1753	1077	0.15%	0.018%
38	6.754	1771	1777	1780	rBV8	1508	1370	0.18%	0.023%
39	6.921	1815	1829	1846	rBV	82662	156407	21.10%	2.606%
40	7.211	1916	1919	1920	rBV3	1340	727	0.10%	0.012%
41	7.252	1921	1932	1948	rVV	305320	542694	73.22%	9.043%
42	7.490	2004	2006	2008	rBV3	1554	856	0.12%	0.014%
43	7.561	2013	2028	2045	rBV	60587	118370	15.97%	1.972%
44	8.034	2162	2175	2204	rBV	157569	328566	44.33%	5.475%
45	8.612	2352	2355	2356	rBV3	996	664	0.09%	0.011%
46	8.793	2400	2411	2432	rBV	409543	683161	92.18%	11.384%
47	9.008	2475	2478	2481	rVB5	2154	1248	0.17%	0.021%
48	9.275	2558	2561	2565	rBV6	1582	1140	0.15%	0.019%
49	9.394	2596	2598	2601	rVB3	1390	664	0.09%	0.011%
50	9.516	2632	2636	2639	rBV6	1339	1202	0.16%	0.020%
51	9.571	2649	2653	2656	rBV6	2415	1955	0.26%	0.033%
52	9.751	2705	2709	2711	rVB5	1973	1319	0.18%	0.022%
53	9.770	2711	2715	2717	rBV4	1238	889	0.12%	0.015%
54	9.792	2718	2722	2724	rVV5	1539	831	0.11%	0.014%
55	9.979	2776	2780	2781	rBV3	1183	926	0.12%	0.015%
56	10.162	2824	2837	2855	rBV	223387	364737	49.21%	6.078%
57	10.349	2891	2895	2901	rBV9	2015	1643	0.22%	0.027%
58	10.374	2901	2903	2909	rVB6	920	782	0.11%	0.013%
59	10.407	2909	2913	2918	rBV7	980	1368	0.18%	0.023%
60	10.461	2927	2930	2936	rBV8	1545	1726	0.23%	0.029%
61	10.503	2941	2943	2946	rVB4	1411	677	0.09%	0.011%
62	10.522	2946	2949	2950	rBV3	1313	779	0.11%	0.013%
63	10.561	2959	2961	2965	rVB5	1052	725	0.10%	0.012%
64	11.117	3130	3134	3139	rVB8	791	782	0.11%	0.013%
65	11.194	3147	3158	3175	rBV	394246	633966	85.54%	10.564%
66	11.323	3196	3198	3202	rVB5	1437	783	0.11%	0.013%
67	11.413	3221	3226	3228	rBV6	1385	1106	0.15%	0.018%
68	11.439	3231	3234	3238	rBV5	1445	1517	0.20%	0.025%
69	11.571	3263	3275	3293	rBV	318994	516853	69.74%	8.613%
70	11.760	3332	3334	3338	rVB4	1623	842	0.11%	0.014%
71	11.989	3403	3405	3408	rBV4	1377	940	0.13%	0.016%
72	12.082	3431	3434	3438	rBV6	1014	886	0.12%	0.015%
73	12.149	3452	3455	3459	rBV5	1494	1147	0.15%	0.019%
74	12.169	3459	3461	3465	rVB5	972	680	0.09%	0.011%
75	12.198	3465	3470	3473	rBV6	1451	1198	0.16%	0.020%
76	12.217	3473	3476	3478	rBV4	1959	1012	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030747.D
 Acq On : 21 Apr 2023 03:41
 Operator : SY/MD
 Sample : 02440-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.243	3482	3484	3485	rBV2	1327	707	0.10%	0.012%
78	12.275	3490	3494	3497	rBV5	1423	1275	0.17%	0.021%
79	12.320	3506	3508	3513	rVB6	1729	1169	0.16%	0.019%
80	12.352	3513	3518	3521	rBV6	1291	1023	0.14%	0.017%
81	12.416	3535	3538	3543	rVB7	1608	1755	0.24%	0.029%
82	12.474	3553	3556	3558	rBV4	1284	761	0.10%	0.013%
83	12.513	3566	3568	3571	rBV3	1345	871	0.12%	0.015%
84	12.628	3600	3604	3607	rVB4	1405	999	0.13%	0.017%
85	12.654	3607	3612	3613	rBV5	1140	969	0.13%	0.016%
86	12.786	3651	3653	3656	rBV4	1340	750	0.10%	0.012%
87	13.140	3761	3763	3767	rBV5	1732	1519	0.20%	0.025%
88	13.358	3828	3831	3835	rBV5	1331	1006	0.14%	0.017%
89	13.416	3846	3849	3854	rBV5	1170	818	0.11%	0.014%
90	13.590	3900	3903	3908	rVB5	1659	1479	0.20%	0.025%
91	13.609	3908	3909	3913	rVB3	1507	884	0.12%	0.015%
92	13.657	3921	3924	3925	rBV2	1551	848	0.11%	0.014%
93	13.686	3930	3933	3935	rBV4	1757	1109	0.15%	0.018%
94	13.892	3994	3997	3998	rBV3	1603	763	0.10%	0.013%
95	13.966	4018	4020	4025	rBV6	919	720	0.10%	0.012%
96	14.001	4028	4031	4033	rBV4	831	646	0.09%	0.011%
97	14.114	4063	4066	4068	rBV4	1577	1059	0.14%	0.018%
98	14.156	4075	4079	4082	rBV5	1521	1211	0.16%	0.020%
99	14.609	4218	4220	4224	rBV5	1260	927	0.13%	0.015%
100	14.998	4338	4341	4342	rBV4	1539	924	0.12%	0.015%




Sum of corrected areas: 6001141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030747.D
Acq On : 21 Apr 2023 03:41
Operator : SY/MD
Sample : 02440-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

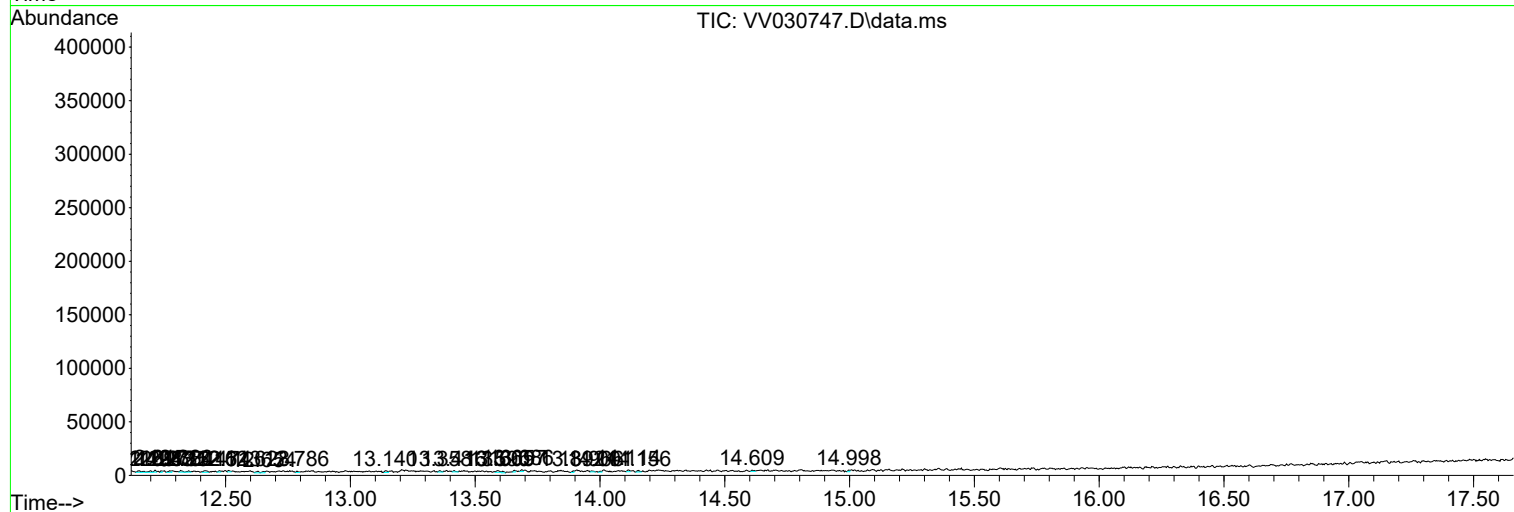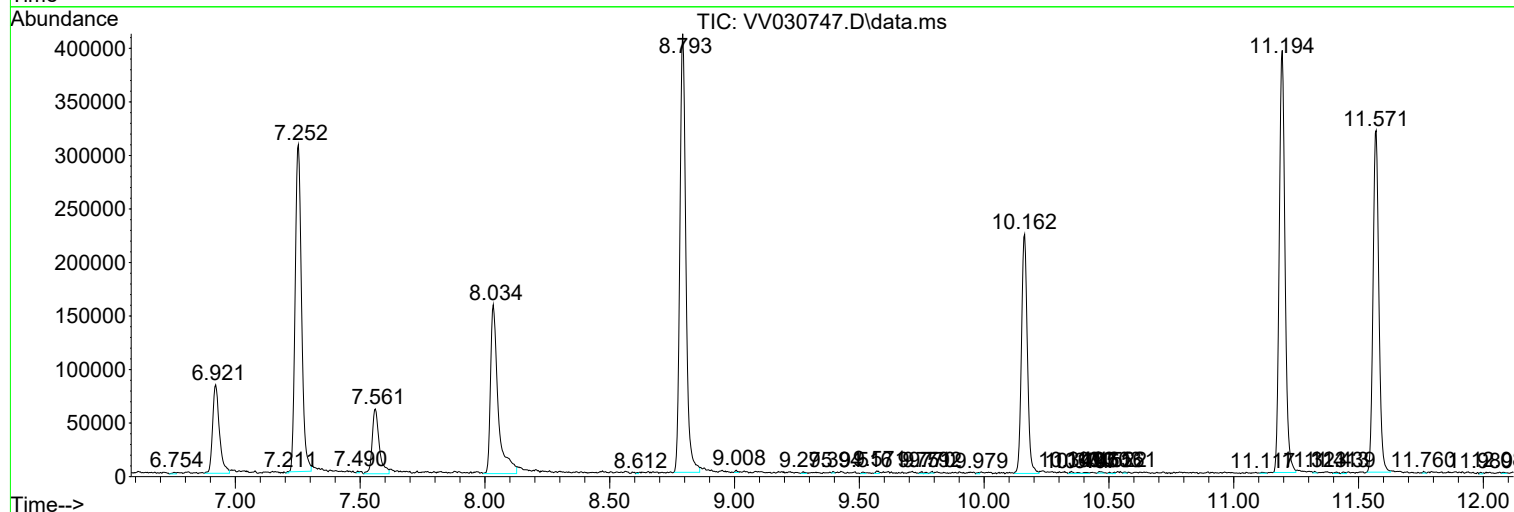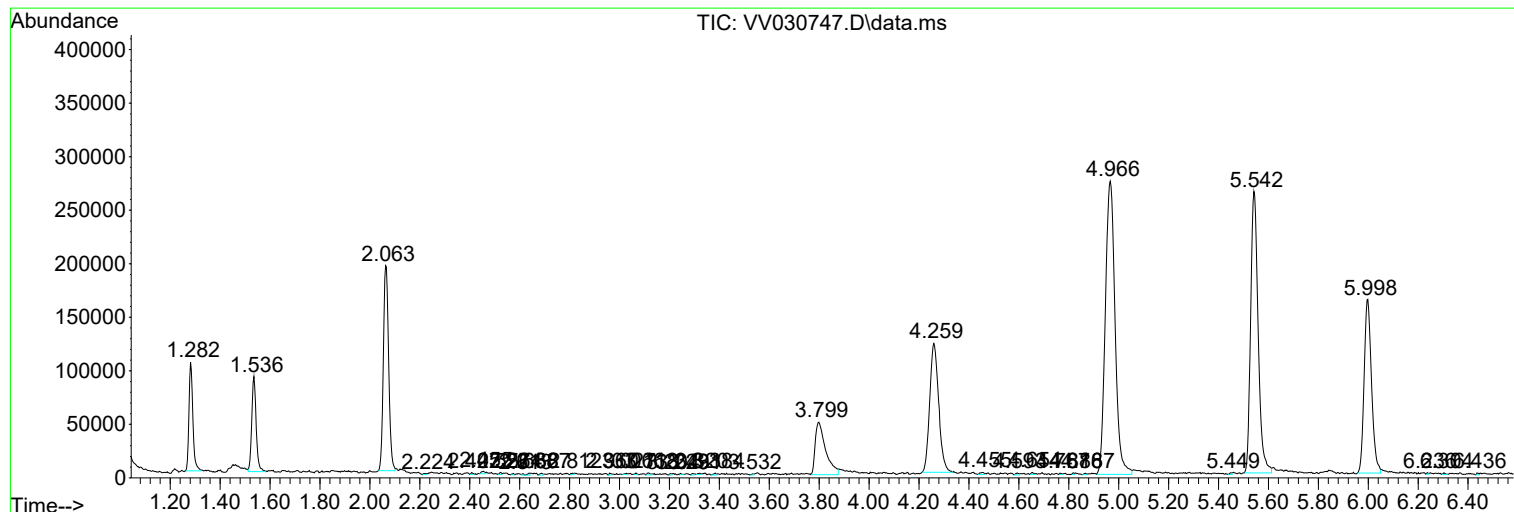

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030747.D
Acq On : 21 Apr 2023 03:41
Operator : SY/MD
Sample : 02440-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030747.D
Acq On : 21 Apr 2023 03:41
Operator : SY/MD
Sample : 02440-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------