

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030748.D
 Acq On : 21 Apr 2023 04:05
 Operator : SY/MD
 Sample : 02440-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	84	rBV	105103	107936	12.09%	1.642%
2	1.535	148	154	168	rVB	87166	105566	11.82%	1.605%
3	2.063	309	318	331	rBV	190431	278128	31.15%	4.230%
4	2.342	402	405	407	rBV4	1360	682	0.08%	0.010%
5	2.384	416	418	423	rVB6	1627	1070	0.12%	0.016%
6	2.416	423	428	429	rBV5	1364	1162	0.13%	0.018%
7	2.567	473	475	479	rBV6	1250	620	0.07%	0.009%
8	2.603	482	486	489	rBV6	1415	849	0.10%	0.013%
9	2.796	542	546	550	rBV7	1169	1161	0.13%	0.018%
10	2.822	550	554	556	rBV4	966	588	0.07%	0.009%
11	2.854	562	564	567	rBV4	1159	595	0.07%	0.009%
12	2.937	585	590	595	rVB9	1594	1763	0.20%	0.027%
13	2.973	595	601	603	rBV7	1537	1242	0.14%	0.019%
14	3.024	613	617	618	rBV4	1014	668	0.07%	0.010%
15	3.053	623	626	628	rBV5	1255	755	0.08%	0.011%
16	3.069	628	631	635	rVB5	1748	1443	0.16%	0.022%
17	3.095	635	639	641	rBV4	1933	1252	0.14%	0.019%
18	3.182	663	666	668	rBV3	1399	731	0.08%	0.011%
19	3.243	682	685	687	rBV3	1286	855	0.10%	0.013%
20	3.278	693	696	699	rBV5	1467	999	0.11%	0.015%
21	3.301	699	703	704	rBV3	1102	616	0.07%	0.009%
22	3.381	725	728	730	rBV4	878	594	0.07%	0.009%
23	3.619	799	802	805	rVV5	1207	697	0.08%	0.011%
24	3.674	814	819	821	rBV4	1835	1451	0.16%	0.022%
25	3.796	848	857	885	rBV2	52099	144856	16.22%	2.203%
26	4.072	941	943	945	rBV3	1230	581	0.07%	0.009%
27	4.259	986	1001	1023	rVV	121834	314178	35.19%	4.778%
28	4.641	1116	1120	1123	rBV5	1957	1268	0.14%	0.019%
29	4.764	1157	1158	1163	rVB5	1485	839	0.09%	0.013%
30	4.966	1203	1221	1243	rBV2	277881	749709	83.96%	11.402%
31	5.204	1293	1295	1300	rBV6	1659	1334	0.15%	0.020%
32	5.310	1326	1328	1334	rBV4	1708	1819	0.20%	0.028%
33	5.448	1369	1371	1375	rBV5	1080	797	0.09%	0.012%
34	5.542	1388	1400	1428	rBV	352281	728331	81.57%	11.077%
35	5.995	1531	1541	1563	rVB	166284	335210	37.54%	5.098%
36	6.445	1678	1681	1682	rBV3	1210	763	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030748.D
 Acq On : 21 Apr 2023 04:05
 Operator : SY/MD
 Sample : 02440-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.564	1715	1718	1719	rBV3	1098	666	0.07%	0.010%
38	6.706	1759	1762	1767	rBV4	1058	1269	0.14%	0.019%
39	6.921	1819	1829	1844	rBV2	82375	153512	17.19%	2.335%
40	7.252	1921	1932	1954	rBV	305791	542327	60.74%	8.248%
41	7.529	2010	2018	2019	rBV7	2084	2158	0.24%	0.033%
42	7.561	2019	2028	2049	rVV	64942	114073	12.78%	1.735%
43	8.034	2166	2175	2192	rBV	163879	308926	34.60%	4.698%
44	8.603	2350	2352	2354	rBV2	1551	823	0.09%	0.013%
45	8.696	2378	2381	2382	rBV3	1409	703	0.08%	0.011%
46	8.792	2399	2411	2432	rBV	546232	892890	100.00%	13.579%
47	8.953	2459	2461	2462	rBV2	1761	750	0.08%	0.011%
48	9.011	2475	2479	2480	rBV4	1073	766	0.09%	0.012%
49	9.191	2532	2535	2536	rBV3	1193	636	0.07%	0.010%
50	9.246	2550	2552	2555	rVB3	1170	629	0.07%	0.010%
51	9.284	2562	2564	2569	rBV6	1329	1123	0.13%	0.017%
52	9.361	2585	2588	2590	rBV4	1435	821	0.09%	0.012%
53	9.612	2664	2666	2669	rBV3	1421	917	0.10%	0.014%
54	9.725	2697	2701	2702	rBV4	2165	1324	0.15%	0.020%
55	9.844	2733	2738	2741	rBV6	1337	1443	0.16%	0.022%
56	9.947	2767	2770	2775	rBV6	1901	2126	0.24%	0.032%
57	10.088	2809	2814	2816	rVB5	1232	1076	0.12%	0.016%
58	10.104	2816	2819	2821	rBV4	1087	779	0.09%	0.012%
59	10.162	2824	2837	2859	rVV	229350	374537	41.95%	5.696%
60	10.323	2885	2887	2890	rBV4	1067	571	0.06%	0.009%
61	10.458	2925	2929	2933	rBV7	1903	1633	0.18%	0.025%
62	10.551	2955	2958	2959	rBV3	1204	577	0.06%	0.009%
63	10.744	3013	3018	3022	rBV8	1094	1153	0.13%	0.018%
64	10.911	3067	3070	3072	rBV4	1270	604	0.07%	0.009%
65	11.008	3096	3100	3101	rBV4	1466	1143	0.13%	0.017%
66	11.088	3120	3125	3127	rBV5	2092	1677	0.19%	0.026%
67	11.127	3134	3137	3140	rBV5	1192	863	0.10%	0.013%
68	11.194	3147	3158	3177	rBV	522665	816722	91.47%	12.421%
69	11.352	3206	3207	3210	rVB3	1677	618	0.07%	0.009%
70	11.371	3211	3213	3214	rBV2	1360	612	0.07%	0.009%
71	11.419	3226	3228	3232	rVB4	1071	603	0.07%	0.009%
72	11.464	3237	3242	3243	rBV3	1967	1140	0.13%	0.017%
73	11.487	3246	3249	3252	rBV5	1393	707	0.08%	0.011%
74	11.570	3263	3275	3293	rBV	323689	526912	59.01%	8.014%
75	11.693	3311	3313	3317	rVB5	1404	653	0.07%	0.010%
76	11.731	3321	3325	3326	rBV4	1191	765	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030748.D
 Acq On : 21 Apr 2023 04:05
 Operator : SY/MD
 Sample : 02440-17 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.937	3387	3389	3392	rVB4	1160	716	0.08%	0.011%
78	11.956	3392	3395	3397	rBV4	1269	641	0.07%	0.010%
79	12.033	3416	3419	3421	rBV3	1155	646	0.07%	0.010%
80	12.043	3421	3422	3425	rVB3	1499	576	0.06%	0.009%
81	12.085	3430	3435	3439	rBV6	1599	1574	0.18%	0.024%
82	12.104	3439	3441	3444	rVV4	1190	833	0.09%	0.013%
83	12.303	3501	3503	3504	rBV2	1426	649	0.07%	0.010%
84	12.532	3571	3574	3578	rBV6	1350	1301	0.15%	0.020%
85	12.590	3587	3592	3594	rBV6	1082	910	0.10%	0.014%
86	12.686	3619	3622	3624	rBV3	1310	836	0.09%	0.013%
87	12.847	3670	3672	3675	rBV4	1913	1343	0.15%	0.020%
88	12.943	3698	3702	3703	rBV3	1547	863	0.10%	0.013%
89	13.117	3754	3756	3760	rBV4	1325	1136	0.13%	0.017%
90	13.146	3762	3765	3768	rVB5	1779	1158	0.13%	0.018%
91	13.458	3857	3862	3863	rBV5	1073	902	0.10%	0.014%
92	13.538	3884	3887	3890	rBV5	1160	932	0.10%	0.014%
93	13.763	3956	3957	3961	rBV3	1208	731	0.08%	0.011%
94	14.036	4040	4042	4044	rBV3	1432	823	0.09%	0.013%
95	14.155	4077	4079	4081	rVV2	1160	631	0.07%	0.010%
96	14.271	4108	4115	4119	rVB9	1630	2078	0.23%	0.032%
97	14.352	4137	4140	4143	rBV4	1393	1003	0.11%	0.015%
98	14.522	4191	4193	4197	rBV4	1686	1306	0.15%	0.020%
99	14.683	4240	4243	4244	rBV3	1080	644	0.07%	0.010%
100	15.020	4346	4348	4350	rBV3	1310	726	0.08%	0.011%




Sum of corrected areas: 6575293

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030748.D
Acq On : 21 Apr 2023 04:05
Operator : SY/MD
Sample : 02440-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

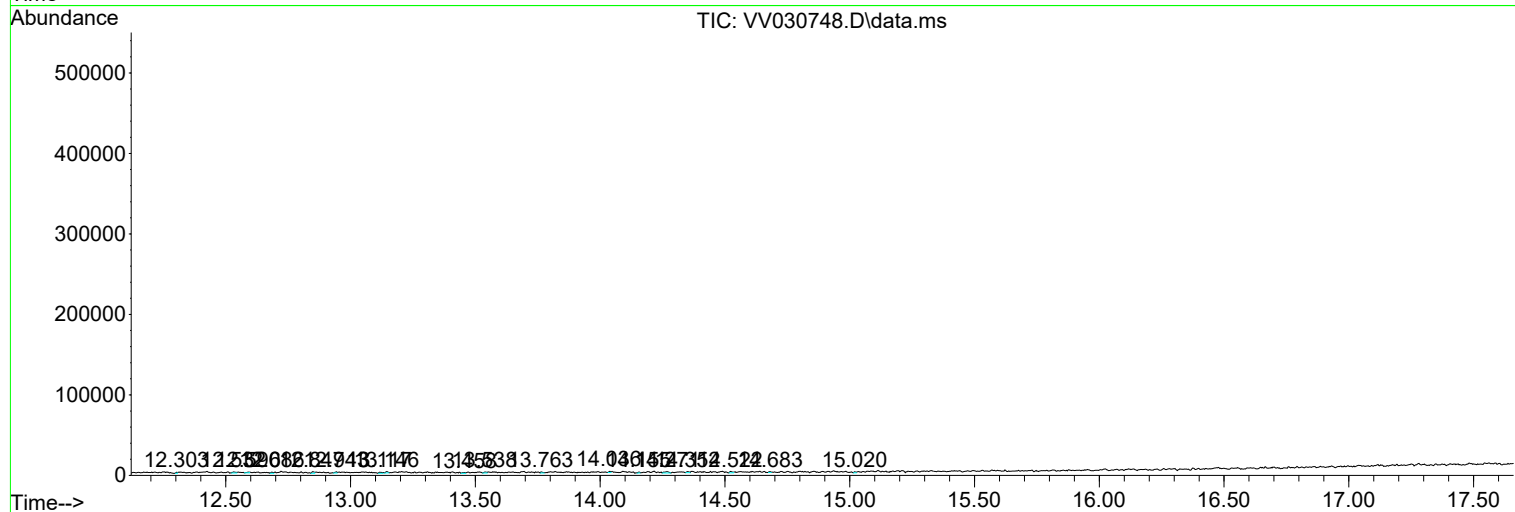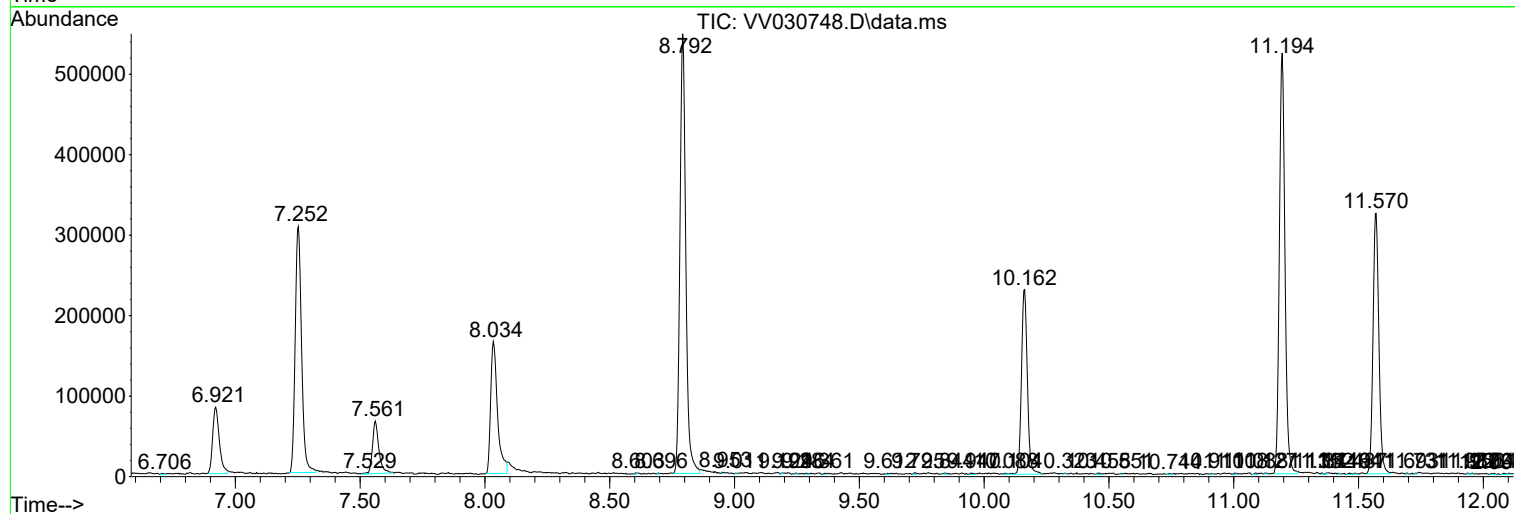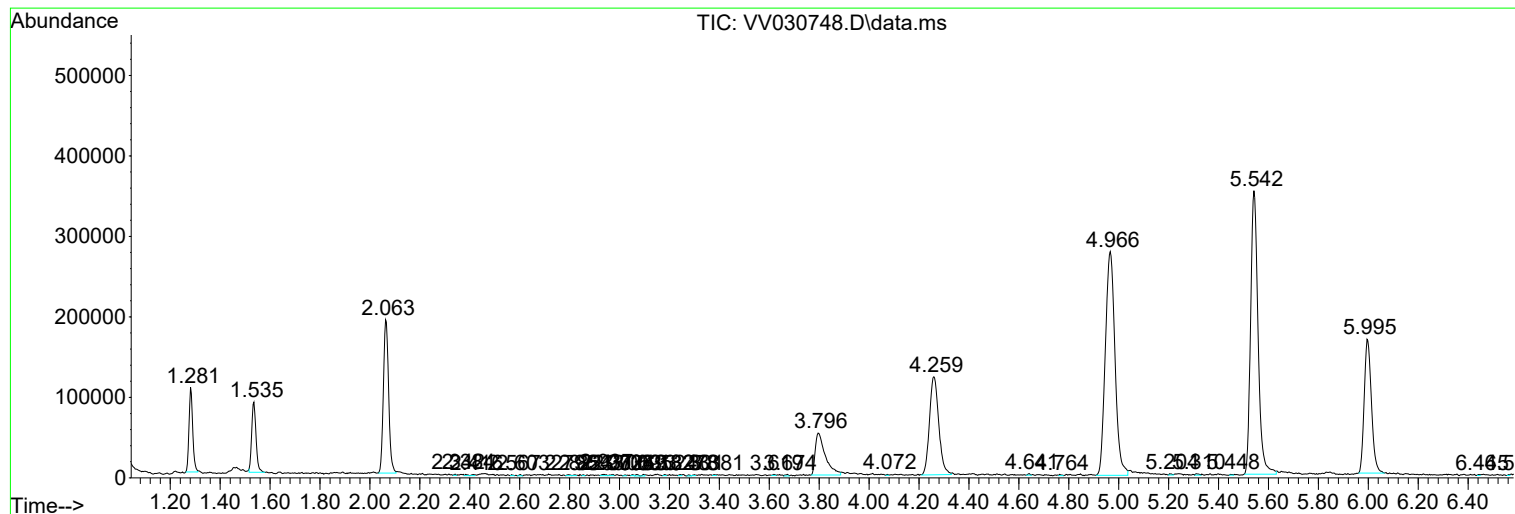

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030748.D
Acq On : 21 Apr 2023 04:05
Operator : SY/MD
Sample : 02440-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030748.D
Acq On : 21 Apr 2023 04:05
Operator : SY/MD
Sample : 02440-17 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
