

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030749.D
 Acq On : 21 Apr 2023 04:29
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	97	rVB	103104	116662	15.57%	1.931%
2	1.535	148	154	169	rVB	94125	110375	14.73%	1.827%
3	2.066	309	319	332	rBV	194120	286521	38.25%	4.743%
4	2.510	451	457	459	rBV7	1845	1746	0.23%	0.029%
5	2.555	467	471	473	rBV5	1069	821	0.11%	0.014%
6	2.667	503	506	511	rBV6	1363	1379	0.18%	0.023%
7	2.773	537	539	541	rBV3	1009	506	0.07%	0.008%
8	2.802	545	548	552	rVV7	1633	1211	0.16%	0.020%
9	2.822	552	554	558	rVV5	1298	943	0.13%	0.016%
10	2.966	597	599	601	rBV3	1220	540	0.07%	0.009%
11	3.059	625	628	629	rBV3	1056	517	0.07%	0.009%
12	3.117	643	646	650	rBV7	1375	1188	0.16%	0.020%
13	3.159	656	659	664	rBV7	1190	1032	0.14%	0.017%
14	3.323	708	710	715	rBV6	1111	772	0.10%	0.013%
15	3.349	715	718	723	rVB7	1219	960	0.13%	0.016%
16	3.375	723	726	729	rVB4	1575	987	0.13%	0.016%
17	3.394	729	732	733	rBV3	1178	878	0.12%	0.015%
18	3.426	740	742	745	rBV4	831	521	0.07%	0.009%
19	3.567	784	786	788	rBV2	1604	663	0.09%	0.011%
20	3.580	788	790	792	rBV3	1458	728	0.10%	0.012%
21	3.619	800	802	807	rVB5	1368	1190	0.16%	0.020%
22	3.648	810	811	815	rVV4	958	687	0.09%	0.011%
23	3.764	843	847	848	rBV4	845	537	0.07%	0.009%
24	3.796	848	857	881	rBV	49743	140559	18.76%	2.327%
25	4.162	968	971	973	rBV3	2210	1148	0.15%	0.019%
26	4.259	987	1001	1025	rBV	122843	306376	40.90%	5.071%
27	4.648	1120	1122	1128	rVB6	1577	854	0.11%	0.014%
28	4.776	1160	1162	1163	rBV2	1335	550	0.07%	0.009%
29	4.834	1178	1180	1182	rBV2	1357	594	0.08%	0.010%
30	4.860	1186	1188	1189	rBV3	1266	533	0.07%	0.009%
31	4.966	1204	1221	1241	rBV2	279761	749109	100.00%	12.400%
32	5.542	1388	1400	1421	rBV	270971	557040	74.36%	9.220%
33	5.998	1529	1542	1564	rBV	168070	348981	46.59%	5.776%
34	6.516	1700	1703	1704	rBV3	964	541	0.07%	0.009%
35	6.529	1704	1707	1708	rBV3	1626	787	0.11%	0.013%
36	6.645	1741	1743	1747	rVB4	1480	889	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030749.D
 Acq On : 21 Apr 2023 04:29
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.699	1758	1760	1764	rVB5	1760	1117	0.15%	0.018%
38	6.725	1766	1768	1771	rBV4	1340	933	0.12%	0.015%
39	6.921	1819	1829	1850	rBV	81809	151017	20.16%	2.500%
40	7.136	1894	1896	1900	rBV4	2009	1141	0.15%	0.019%
41	7.252	1920	1932	1951	rBV	317624	561391	74.94%	9.292%
42	7.561	2019	2028	2043	rBV	59096	107127	14.30%	1.773%
43	7.837	2112	2114	2119	rVB7	1857	1267	0.17%	0.021%
44	7.876	2124	2126	2130	rVV4	1055	639	0.09%	0.011%
45	7.937	2143	2145	2147	rBV3	1002	546	0.07%	0.009%
46	7.953	2147	2150	2152	rBV3	1361	968	0.13%	0.016%
47	8.034	2166	2175	2192	rBV	157595	299461	39.98%	4.957%
48	8.426	2293	2297	2299	rBV4	1583	1259	0.17%	0.021%
49	8.471	2308	2311	2314	rBV4	2184	1509	0.20%	0.025%
50	8.792	2400	2411	2433	rBV	423431	700231	93.48%	11.591%
51	9.124	2511	2514	2517	rBV4	1387	1125	0.15%	0.019%
52	9.316	2572	2574	2578	rBV5	1215	738	0.10%	0.012%
53	9.394	2596	2598	2600	rBV2	1010	453	0.06%	0.007%
54	9.625	2668	2670	2672	rBV2	1387	625	0.08%	0.010%
55	9.747	2706	2708	2711	rBV4	1659	930	0.12%	0.015%
56	9.770	2713	2715	2717	rBV3	1259	572	0.08%	0.009%
57	9.934	2764	2766	2768	rVB3	1276	453	0.06%	0.007%
58	10.053	2801	2803	2804	rBV2	919	448	0.06%	0.007%
59	10.082	2810	2812	2814	rBV3	1700	1028	0.14%	0.017%
60	10.162	2826	2837	2854	rVB	227280	368445	49.18%	6.099%
61	10.291	2874	2877	2880	rVB4	1336	866	0.12%	0.014%
62	10.561	2959	2961	2963	rBV3	962	647	0.09%	0.011%
63	10.657	2989	2991	2998	rVB6	995	847	0.11%	0.014%
64	10.815	3036	3040	3041	rBV3	1055	696	0.09%	0.012%
65	10.869	3052	3057	3062	rVB8	1793	2011	0.27%	0.033%
66	10.902	3062	3067	3068	rBV5	1780	1157	0.15%	0.019%
67	10.995	3093	3096	3097	rBV2	1077	572	0.08%	0.009%
68	11.056	3112	3115	3120	rVB6	1599	1219	0.16%	0.020%
69	11.095	3124	3127	3130	rBV5	1234	1085	0.14%	0.018%
70	11.194	3146	3158	3177	rBV	403374	640647	85.52%	10.604%
71	11.570	3263	3275	3289	rBV	319403	521891	69.67%	8.639%
72	11.728	3322	3324	3329	rVV6	1257	863	0.12%	0.014%
73	11.767	3332	3336	3338	rBV4	1126	732	0.10%	0.012%
74	11.786	3340	3342	3348	rBV5	1022	851	0.11%	0.014%
75	11.969	3396	3399	3400	rBV3	1560	638	0.09%	0.011%
76	12.046	3421	3423	3426	rBV3	1180	769	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030749.D
 Acq On : 21 Apr 2023 04:29
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.252	3485	3487	3490	rBV4	1095	729	0.10%	0.012%
78	12.519	3564	3570	3572	rBV6	1901	1981	0.26%	0.033%
79	12.564	3581	3584	3586	rBV4	1107	767	0.10%	0.013%
80	12.693	3618	3624	3627	rBV8	1925	2348	0.31%	0.039%
81	12.721	3630	3633	3638	rVB7	953	758	0.10%	0.013%
82	12.741	3638	3639	3641	rBV2	817	436	0.06%	0.007%
83	12.911	3690	3692	3694	rBV3	1162	707	0.09%	0.012%
84	12.943	3700	3702	3704	rBV3	1086	658	0.09%	0.011%
85	13.014	3722	3724	3726	rVB3	1178	513	0.07%	0.008%
86	13.027	3726	3728	3730	rVB3	1616	708	0.09%	0.012%
87	13.040	3730	3732	3735	rBV2	1545	868	0.12%	0.014%
88	13.059	3735	3738	3740	rBV4	2338	1554	0.21%	0.026%
89	13.223	3786	3789	3791	rBV4	1239	626	0.08%	0.010%
90	13.512	3877	3879	3881	rBV3	1619	783	0.10%	0.013%
91	13.779	3960	3962	3963	rBV2	1249	515	0.07%	0.009%
92	13.879	3992	3993	3995	rVB2	2086	634	0.08%	0.010%
93	13.898	3995	3999	4002	rBV5	1595	1365	0.18%	0.023%
94	14.075	4051	4054	4056	rBV5	1038	622	0.08%	0.010%
95	14.229	4100	4102	4107	rBV6	1046	870	0.12%	0.014%
96	14.577	4208	4210	4211	rBV2	2208	929	0.12%	0.015%
97	14.889	4305	4307	4309	rBV2	1455	766	0.10%	0.013%
98	15.117	4376	4378	4380	rBV3	1711	867	0.12%	0.014%
99	15.226	4410	4412	4417	rVB6	2139	1340	0.18%	0.022%
100	15.255	4417	4421	4424	rBV5	1774	1828	0.24%	0.030%


Sum of corrected areas: 6041411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030749.D
Acq On : 21 Apr 2023 04:29
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

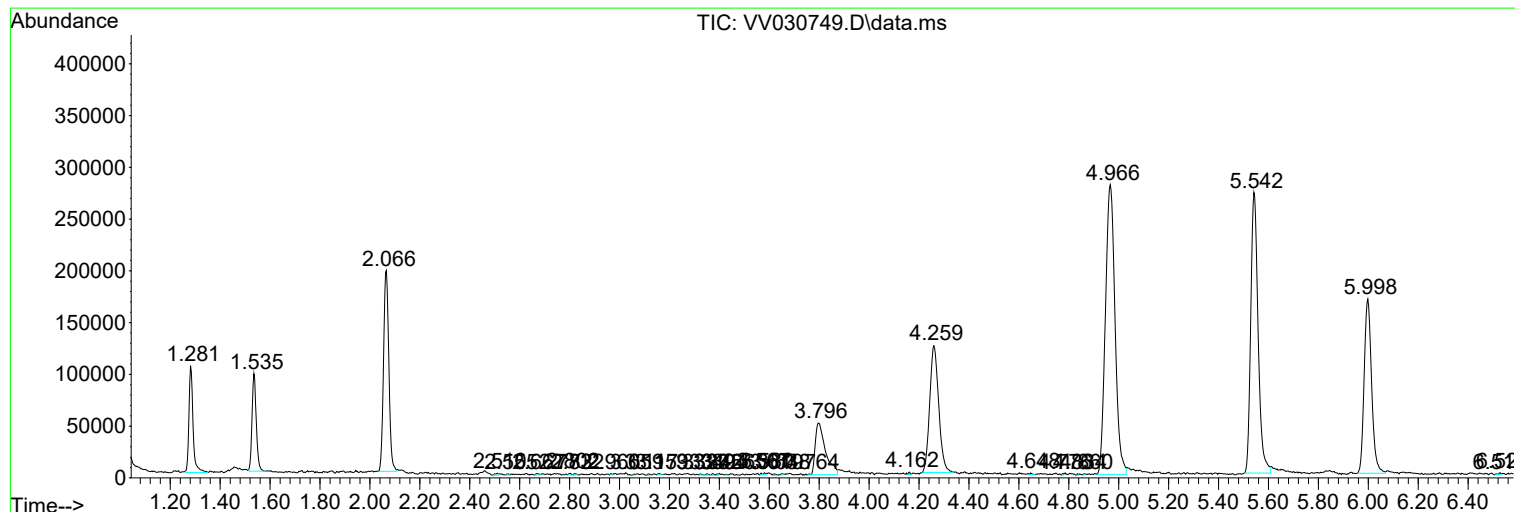

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030749.D
Acq On : 21 Apr 2023 04:29
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030749.D
Acq On : 21 Apr 2023 04:29
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------