


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030702.D
 Acq On : 20 Apr 2023 09:07
 Operator : SY/MD
 Sample : BFB369
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB369

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 21 01:37:39 2023

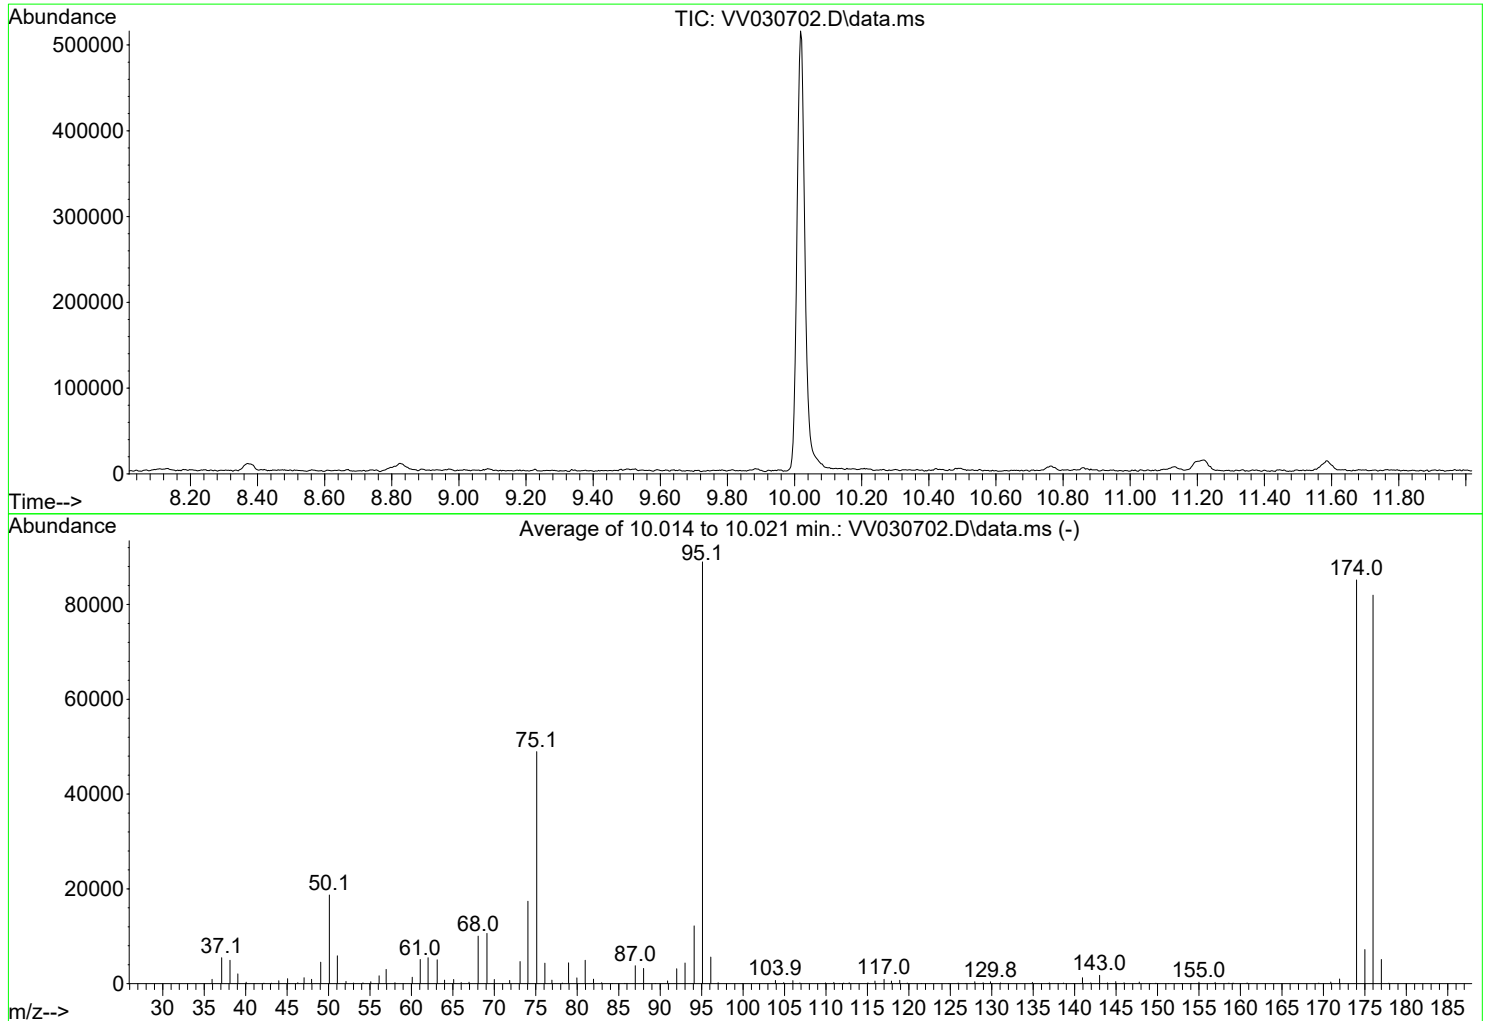

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	18699	PASS
75	95	30	80	55.0	48944	PASS
95	95	100	100	100.0	88989	PASS
96	95	5	9	6.3	5593	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.7	85160	PASS
175	174	5	9	8.4	7178	PASS
176	174	95	105	96.3	81968	PASS
177	176	5	10	6.2	5097	PASS

m/z	Abundance
35.30	216.0
35.90	231.0
36.80	134.0
37.40	151.0
38.30	160.0
39.00	110.0
39.50	186.0
41.60	197.0
42.60	151.0
43.20	129.0
43.90	254.0
44.60	112.0
45.30	134.0
45.90	132.0
51.00	102.0
51.50	115.0
53.00	103.0
54.50	122.0
56.90	116.0
60.80	124.0
62.60	149.0
64.50	109.0
65.50	122.0
77.60	155.0
101.40	117.0
178.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.20	139.0
36.00	1089.0
37.10	5377.0
38.10	4753.0
39.10	2076.0
40.10	286.0
41.60	124.0
43.00	244.0
44.00	922.0
45.10	1030.0
46.30	218.0
47.10	1214.0
48.00	862.0
49.00	4437.0
50.10	17808.0
51.10	5892.0
52.10	433.0
53.00	239.0
54.10	199.0
55.10	446.0
56.10	1557.0
57.00	2936.0
58.00	166.0
59.00	108.0
60.10	1316.0
61.00	4975.0
62.00	5086.0
63.10	4973.0
64.00	758.0
65.10	760.0
66.00	337.0
66.90	299.0
68.00	9735.0
69.10	10201.0
70.00	848.0
71.80	732.0
73.10	4393.0
74.10	17112.0
75.10	47520.0
76.10	4202.0
77.00	777.0
78.20	378.0
78.90	4327.0
80.00	1187.0
80.90	4729.0
82.00	887.0
82.90	182.0
85.70	111.0
87.00	3800.0
88.00	3430.0
89.40	110.0
90.90	481.0
92.00	3124.0
93.00	4058.0
94.10	11708.0
95.10	85472.0
96.10	5435.0
97.00	215.0
99.90	103.0
103.90	677.0
104.80	235.0
106.00	604.0
107.00	157.0
110.00	171.0
110.90	238.0
111.60	101.0
112.20	104.0
112.80	225.0
115.10	176.0
115.90	471.0
117.00	803.0
117.90	600.0
118.90	737.0
119.80	120.0
121.50	101.0
124.80	118.0
126.00	104.0
126.90	125.0
127.90	400.0
129.00	213.0
129.80	396.0
131.10	166.0
134.90	248.0
136.80	191.0
138.60	152.0
139.90	113.0
141.00	1133.0
141.90	153.0
143.00	1613.0
143.90	184.0
145.00	419.0
145.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

147.80	355.0
149.80	138.0
152.90	111.0
154.10	109.0
155.00	303.0
156.90	297.0
158.60	116.0
159.10	120.0
160.80	163.0
169.50	111.0
170.80	338.0
171.90	929.0
174.00	80528.0
175.00	6670.0
176.00	76840.0
177.00	4987.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.20	143.0
36.00	1224.0
37.10	5714.0
38.10	5281.0
39.10	2282.0
40.00	328.0
41.60	126.0
42.20	120.0
43.00	240.0
44.10	894.0
45.10	1053.0
46.30	216.0
47.00	1334.0
47.90	973.0
49.00	4639.0
50.10	19312.0
51.10	6201.0
52.10	507.0
53.00	236.0
54.20	184.0
55.10	427.0
56.10	1714.0
57.00	3235.0
58.00	203.0
60.10	1393.0
61.10	5234.0
62.00	5713.0
63.10	5257.0
64.00	774.0
65.10	893.0
66.00	256.0
66.90	311.0
68.00	10364.0
69.10	10974.0
70.00	906.0
71.80	704.0
73.10	4786.0
74.00	17888.0
75.10	50552.0
76.10	4435.0
76.90	759.0
78.90	4500.0
79.90	1289.0
80.90	5133.0
82.00	976.0
83.00	207.0
85.80	147.0
87.00	3946.0
88.00	3203.0
90.90	601.0
92.00	3209.0
93.00	4502.0
94.10	12610.0
95.10	91808.0
96.10	5765.0
97.00	249.0
103.90	702.0
104.90	264.0
106.00	672.0
106.80	160.0
110.00	185.0
110.90	291.0
112.10	133.0
112.80	232.0
115.10	183.0
115.90	547.0
117.00	963.0
117.90	576.0
118.90	756.0
119.80	153.0
126.00	136.0
126.90	123.0
127.90	417.0
129.00	221.0
129.80	433.0
131.10	168.0
134.90	278.0
137.00	264.0
138.70	144.0
140.90	1286.0
142.00	186.0
143.00	1863.0
143.90	186.0
145.00	484.0
146.00	197.0
147.80	359.0
149.80	131.0
151.30	101.0
155.00	323.0
156.90	264.0
158.60	132.0
159.10	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

160.80	174.0
169.40	143.0
170.90	340.0
171.90	997.0
174.00	87808.0
175.00	7459.0
176.00	84368.0
177.00	5297.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

m/z	Abundance
35.20	134.0
36.00	1144.0
37.10	5343.0
38.10	5243.0
39.10	2183.0
40.00	351.0
41.00	117.0
41.60	115.0
42.20	148.0
43.10	220.0
44.10	802.0
45.00	1029.0
46.30	217.0
47.00	1234.0
47.90	859.0
49.10	4503.0
50.10	18976.0
51.10	5845.0
52.10	483.0
53.00	220.0
54.20	168.0
55.10	358.0
56.10	1718.0
57.00	3209.0
58.00	212.0
60.10	1320.0
61.00	5092.0
62.00	5609.0
63.10	4902.0
64.00	718.0
65.10	988.0
66.10	164.0
67.00	330.0
68.10	10014.0
69.10	10607.0
70.00	852.0
71.90	644.0
73.10	4769.0
74.00	17200.0
75.10	48760.0
76.10	4292.0
76.90	651.0
77.70	250.0
79.00	4317.0
79.90	1181.0
81.00	4940.0
81.90	980.0
83.00	219.0
84.20	124.0
86.00	193.0
87.00	3566.0
88.00	3022.0
90.90	630.0
92.00	3142.0
93.00	4463.0
94.10	12253.0
95.10	89688.0
96.10	5579.0
97.00	186.0
103.90	679.0
105.00	231.0
106.00	630.0
106.80	153.0
109.90	175.0
111.00	280.0
112.10	149.0
112.80	208.0
114.90	175.0
115.90	592.0
117.00	1024.0
117.90	500.0
118.90	675.0
119.80	144.0
125.90	128.0
128.00	387.0
128.90	229.0
129.90	430.0
131.00	148.0
134.90	278.0
136.90	298.0
138.00	101.0
138.70	117.0
140.90	1296.0
142.00	207.0
143.00	1823.0
144.00	187.0
144.90	471.0
146.00	203.0
147.80	316.0
149.10	107.0
150.00	134.0
155.00	291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369

157.00	243.0
158.60	157.0
159.10	178.0
160.80	160.0
169.40	130.0
171.00	314.0
172.00	1061.0
174.00	87144.0
175.00	7406.0
176.00	84696.0
177.00	5008.0
177.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB369