

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042120\
 Data File : VV015596.D
 Acq On : 21 Apr 2020 13:32
 Operator : SY/MD
 Sample : L2366-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKG6

Quant Time: Apr 22 01:44:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 22 00:11:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	136183	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	131927	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	63499	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35675	5.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.00%
7) Chloroethane-d5	1.58	69	33982	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.12	63	54952	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	3.91	46	104207	52.52	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.04%
24) Chloroform-d	4.38	84	76566	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.06	65	44233	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.08	84	150940	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
36) 1,2-Dichloropropane-d6	6.09	67	47290	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.34	98	138744	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
43) trans-1,3-Dichloropropene-	7.64	79	17544	4.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.40%
46) 2-Hexanone-d5	8.11	63	86986	45.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.00%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	33100	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	52574	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
53) m,p-xylene	9.16	106	3347	0.180 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042120\
Data File : VV015596.D
Acq On : 21 Apr 2020 13:32
Operator : SY/MD
Sample : L2366-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKG6

Quant Time: Apr 22 01:44:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 22 00:11:50 2020
Response via : Initial Calibration

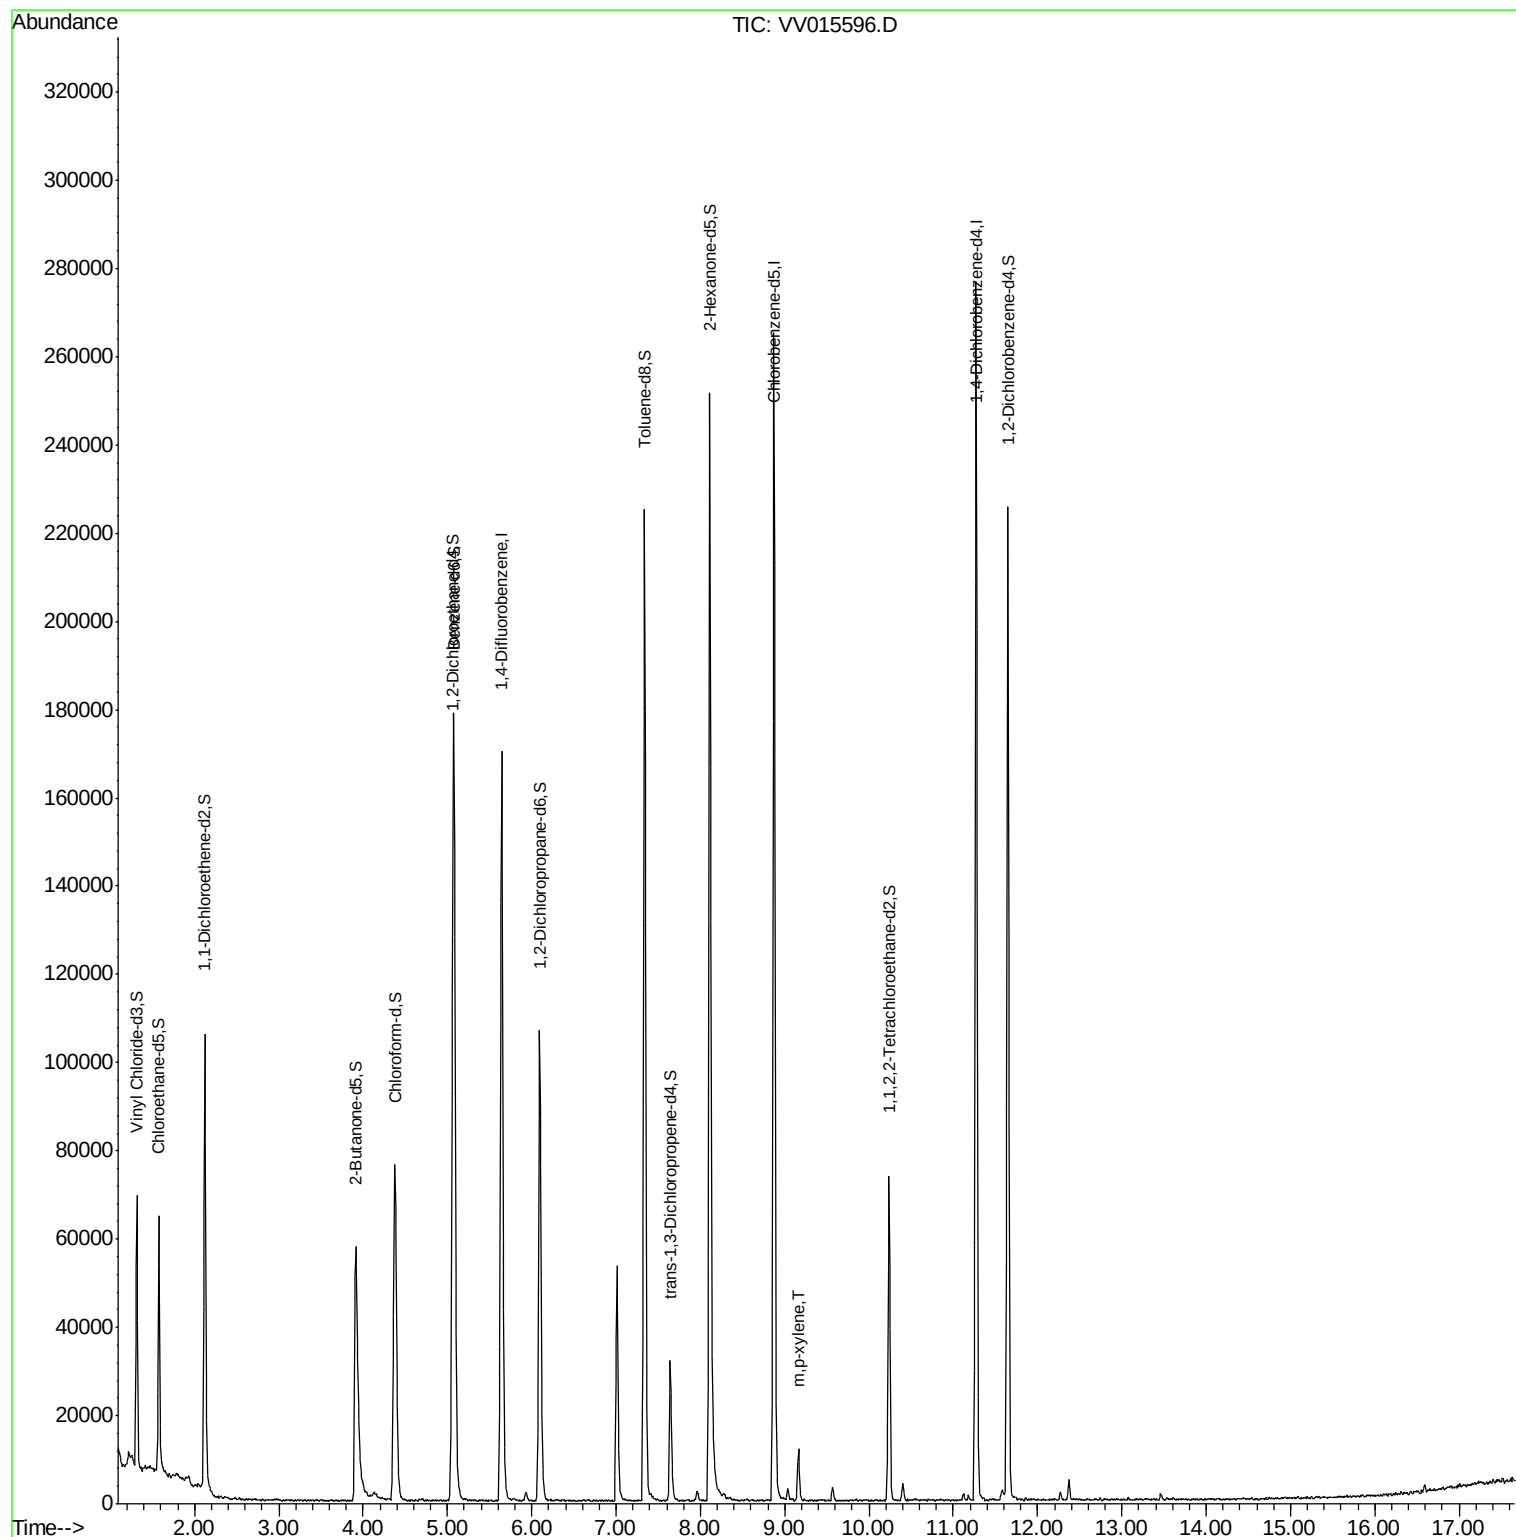

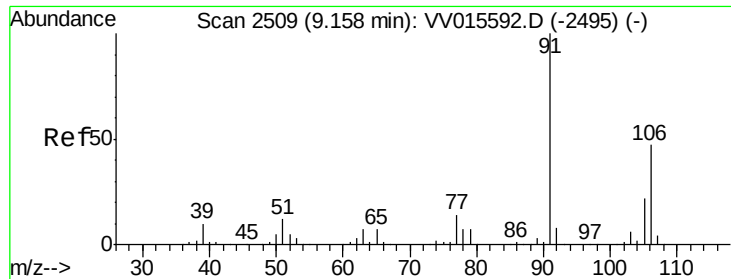

#53

m,p-xylene

Concen: 0.180 ug/L

RT: 9.16 min Scan# 2510

Delta R.T. 0.00 min

Lab File: VV015596.D

Acq: 21 Apr 2020 13:32

Instrument :
MSVOA_V
ClientSampleId :
ETKG6

Tot Ion:106 Resp: 3347

Ion Ratio Lower Upper

106 100

91 193.6 147.9 274.7

