

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042120\
 Data File : VV015604.D
 Acq On : 21 Apr 2020 16:40
 Operator : SY/MD
 Sample : L2366-09
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKH5

Quant Time: Apr 22 02:54:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 22 00:11:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	133045	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	128783	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	62877	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	35023	5.07	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.40%
7) Chloroethane-d5	1.58	69	32447	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.12	63	52639	3.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.40%
20) 2-Butanone-d5	3.95	46	106605	55.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.00%
24) Chloroform-d	4.38	84	76502	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
26) 1,2-Dichloroethane-d4	5.06	65	44667	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
32) Benzene-d6	5.07	84	146102	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.10	67	46104	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.34	98	135743	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
43) trans-1,3-Dichloropropene-	7.64	79	15050	3.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.80%
46) 2-Hexanone-d5	8.12	63	85476	45.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.60%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	33306	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	52169	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.94	96	1133	0.116 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042120\
Data File : VV015604.D
Acq On : 21 Apr 2020 16:40
Operator : SY/MD
Sample : L2366-09
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKH5

Quant Time: Apr 22 02:54:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 22 00:11:50 2020
Response via : Initial Calibration

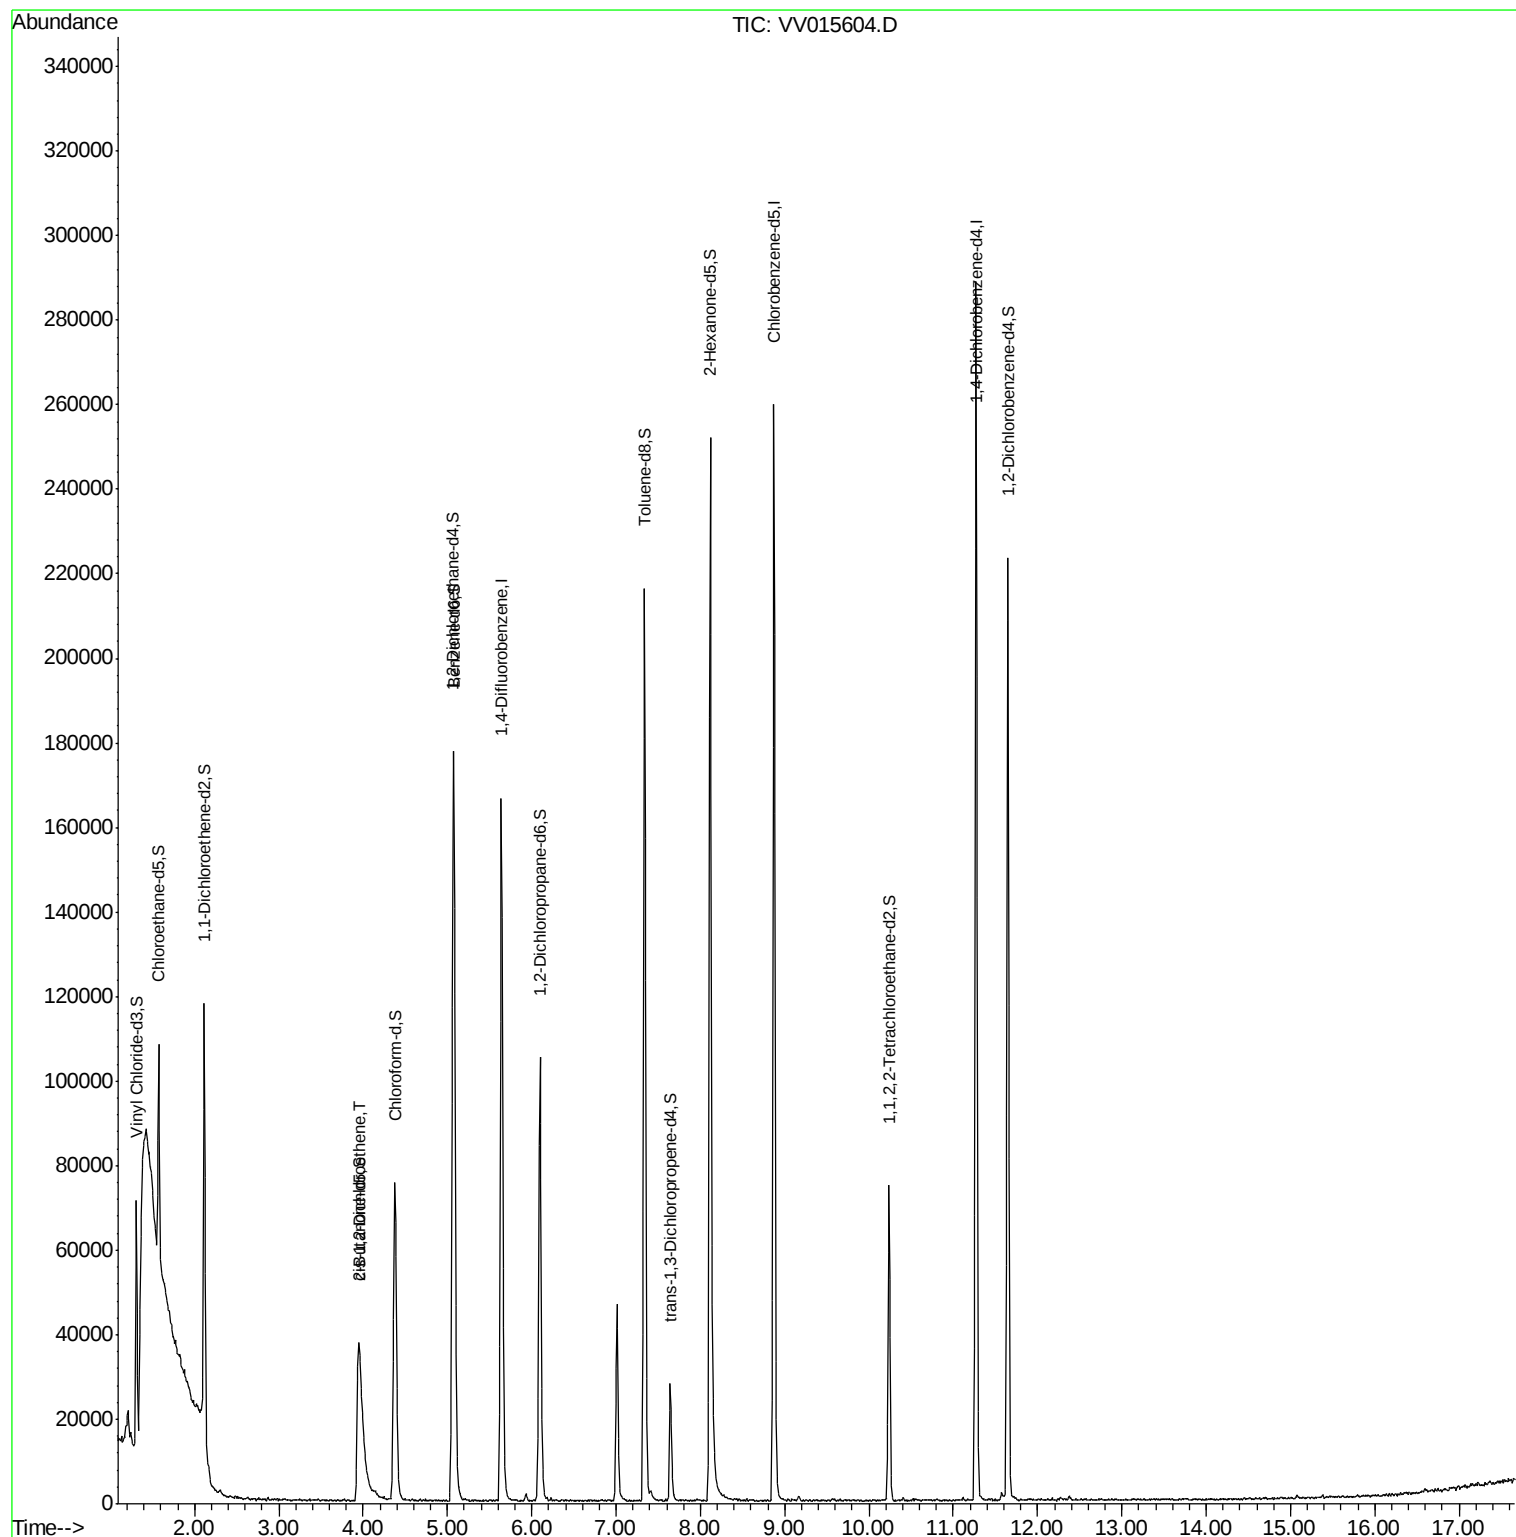

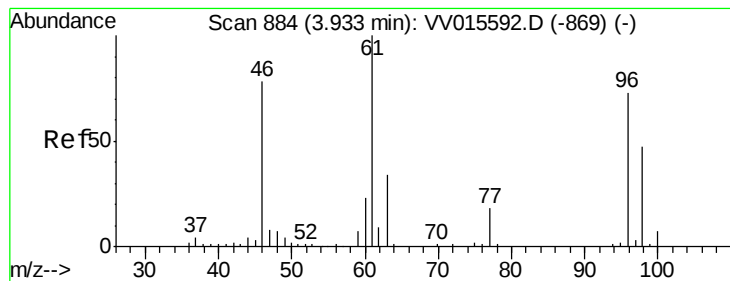

#22

cis-1,2-Dichloroethene

Concen: 0.116 ug/L

RT: 3.94 min Scan# 887

Delta R.T. 0.01 min

Lab File: VV015604.D

Acq: 21 Apr 2020 16:40

Instrument :
MSVOA_V
ClientSampleId :
ETKH5

Tot Ion: 96 Resp: 1133

Ion Ratio Lower Upper

96 100

61 128.0 100.0 185.8

68 0.0 0.0 0.0

