

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042120\
 Data File : VV015610.D
 Acq On : 21 Apr 2020 19:00
 Operator : SY/MD
 Sample : L2366-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKJ1

Quant Time: Apr 22 03:26:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 22 00:11:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	131214	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	124667	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	60797	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	37622	5.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.40%
7) Chloroethane-d5	1.58	69	33125	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.60%
11) 1,1-Dichloroethene-d2	2.12	63	53811	3.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.00%
20) 2-Butanone-d5	3.91	46	105538	55.21	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.42%
24) Chloroform-d	4.38	84	77029	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
26) 1,2-Dichloroethane-d4	5.06	65	43480	5.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	5.08	84	148142	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
36) 1,2-Dichloropropane-d6	6.09	67	45876	5.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.60%
41) Toluene-d8	7.34	98	136227	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
43) trans-1,3-Dichloropropene-	7.64	79	14209	3.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.80%
46) 2-Hexanone-d5	8.11	63	81963	45.37	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.74%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	32424	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	51365	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
42) Toluene	7.42	91	3270	0.081 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042120\
Data File : VV015610.D
Acq On : 21 Apr 2020 19:00
Operator : SY/MD
Sample : L2366-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKJ1

Quant Time: Apr 22 03:26:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 22 00:11:50 2020
Response via : Initial Calibration

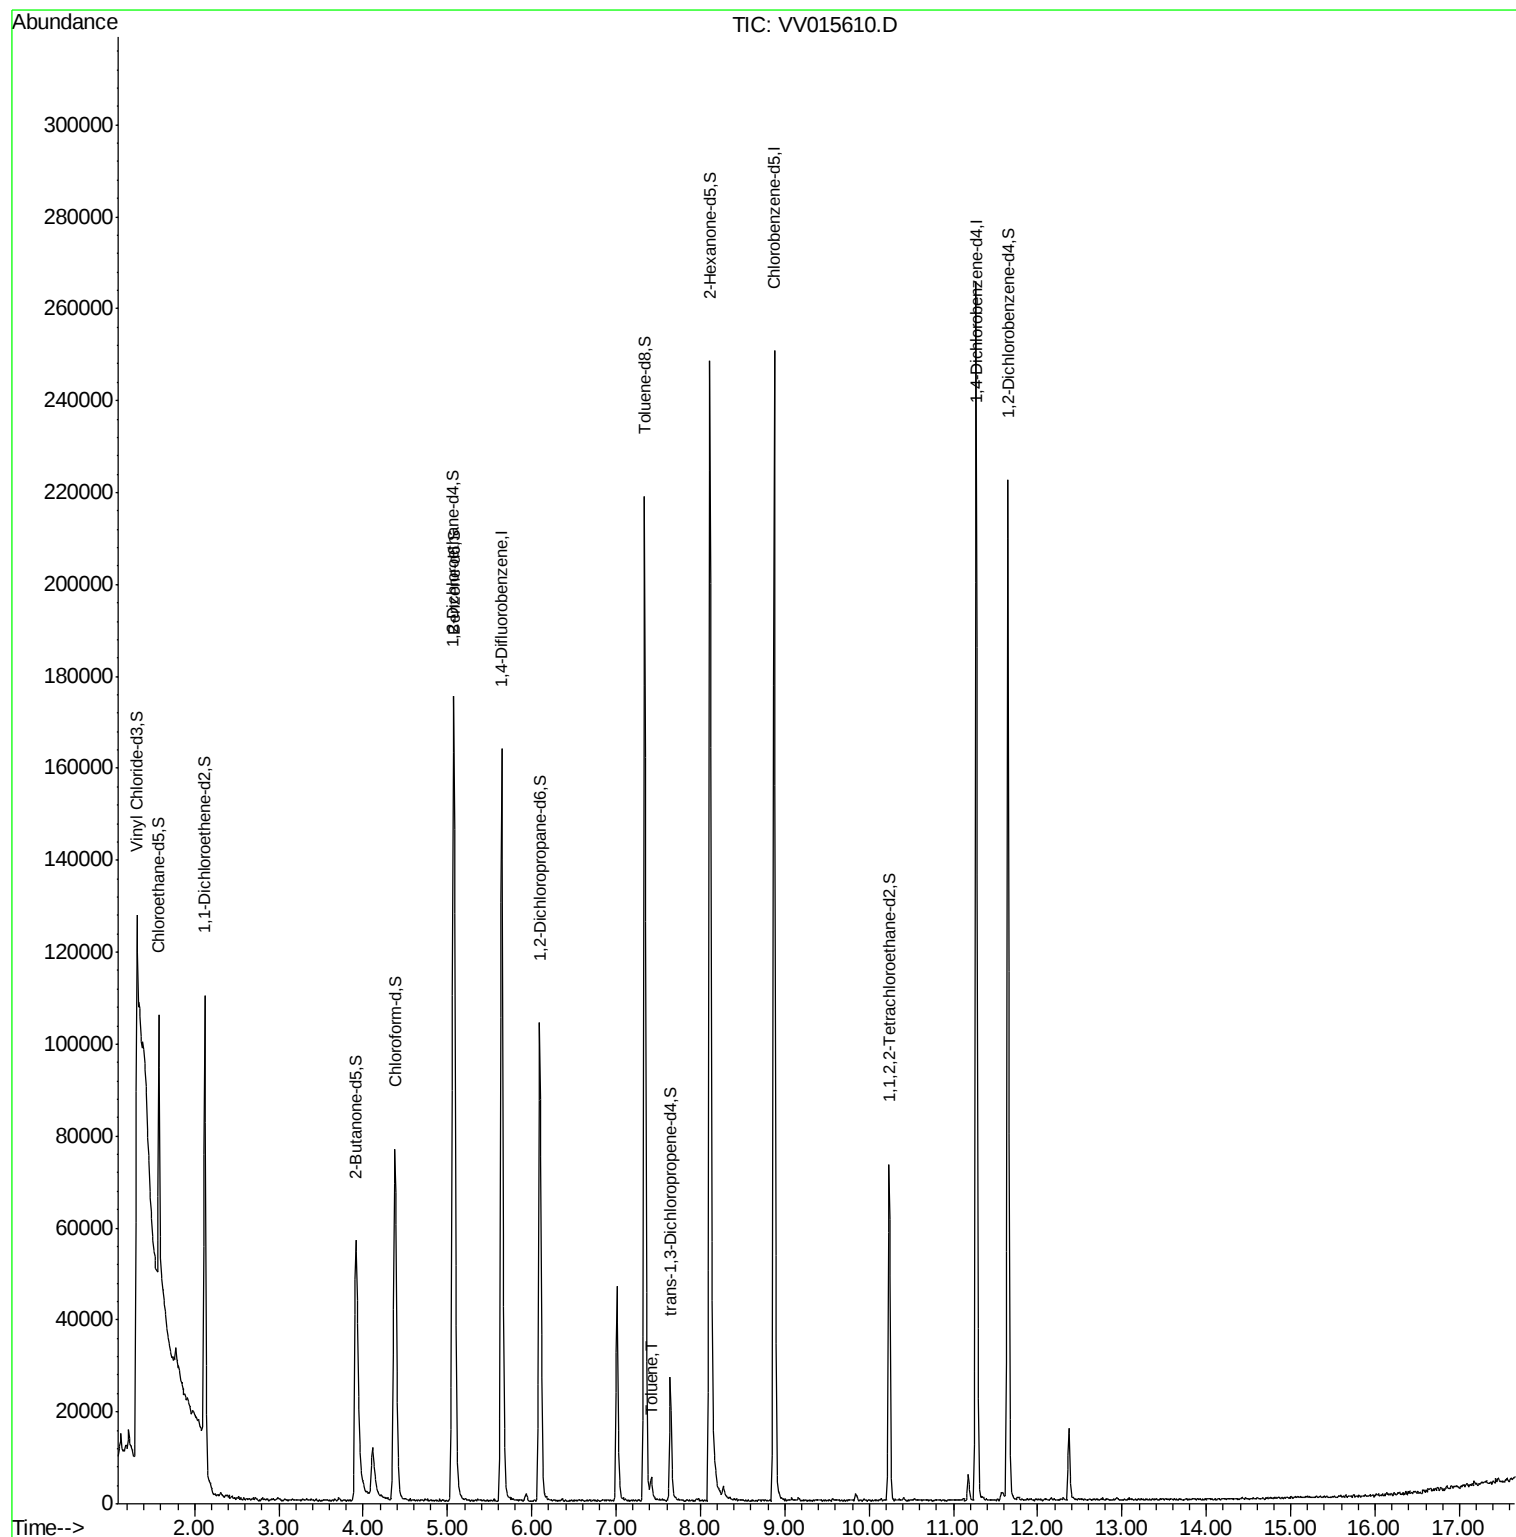

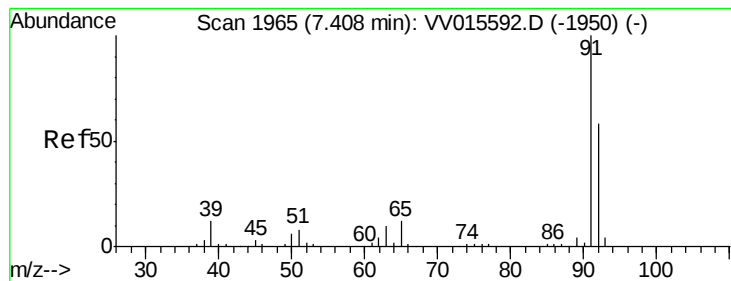

#42

Toluene

Concen: 0.081 ug/L

RT: 7.42 min Scan# 1968

Delta R.T. 0.01 min

Lab File: VV015610.D

Acq: 21 Apr 2020 19:00

Instrument :
MSVOA_V
ClientSampleId :
ETKJ1

Tot Ion: 91 Resp: 3270

Ion Ratio Lower Upper

91 100

92 53.2 40.2 74.6

