


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042120\
 Data File : VV015591.D
 Acq On : 21 Apr 2020 09:30
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Apr 22 00:11:50 2020

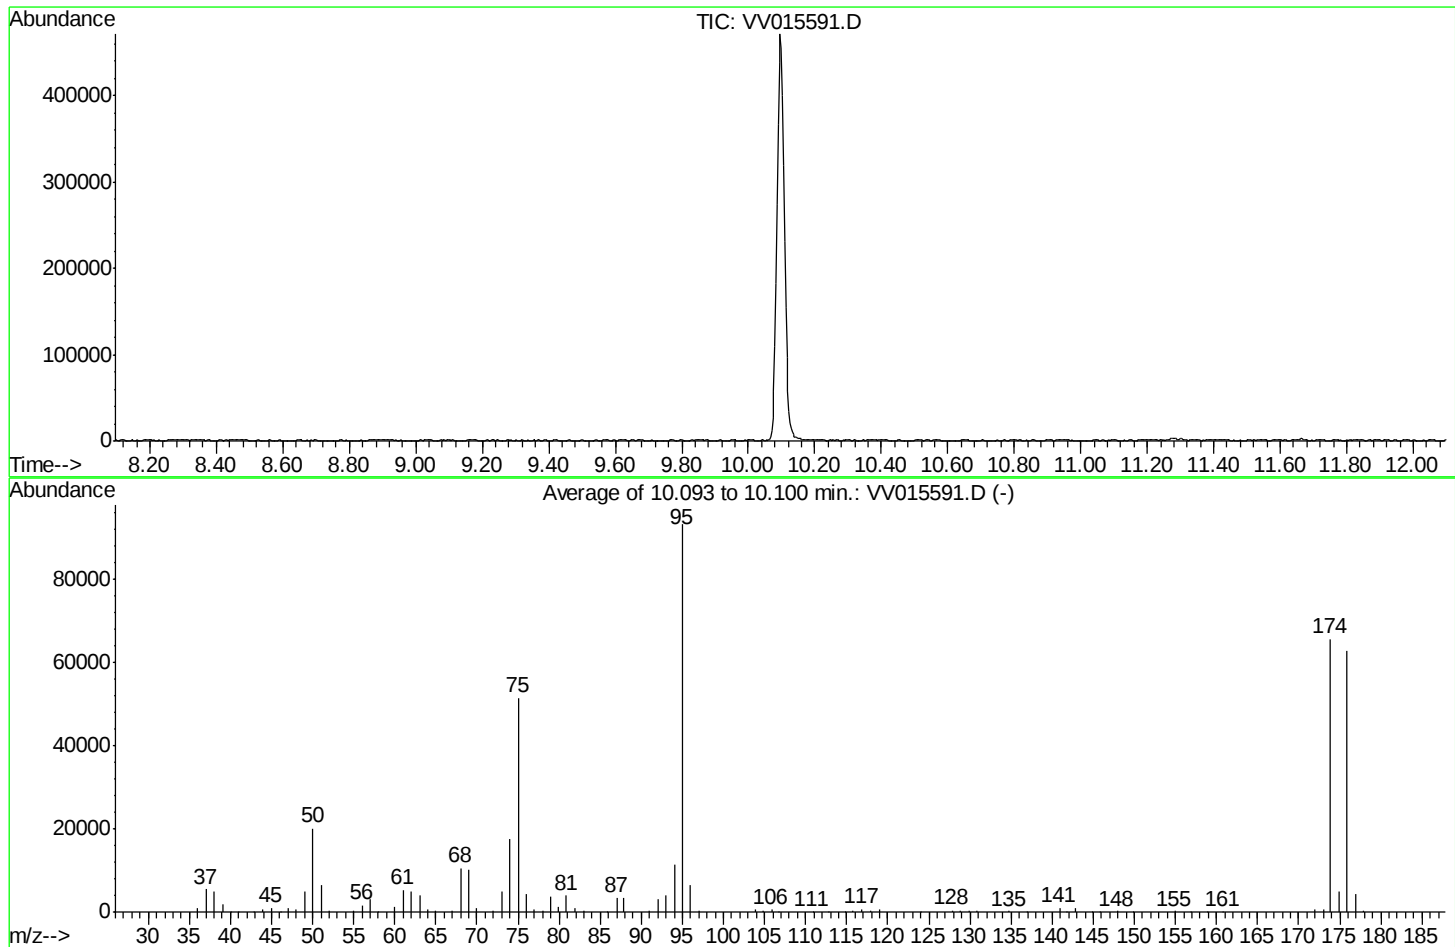

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	20040	PASS
75	95	30	80	55.2	51461	PASS
95	95	100	100	100.0	93152	PASS
96	95	5	9	6.9	6391	PASS
173	174	0.00	2	0.9	593	PASS
174	95	50	120	70.4	65597	PASS
175	174	5	9	7.4	4845	PASS
176	174	95	101	95.6	62741	PASS
177	176	5	9	6.8	4258	PASS

m/z	Abundance
36.00	1027.0
37.00	5335.0
38.00	4620.0
39.10	1919.0
40.00	406.0
42.80	105.0
44.00	993.0
45.00	963.0
46.10	162.0
47.00	984.0
48.00	658.0
49.00	4761.0
50.00	19776.0
51.00	6331.0
52.00	383.0
54.90	338.0
56.00	1570.0
57.00	2969.0
57.90	175.0
60.00	994.0
61.00	5092.0
62.00	5013.0
63.00	3712.0
64.00	446.0
64.90	398.0
66.90	294.0
68.00	10434.0
69.00	9875.0
70.00	779.0
72.00	489.0
73.00	4606.0
74.00	17168.0
75.00	50240.0
76.00	4147.0
77.00	678.0
78.00	369.0
78.90	3840.0
79.90	1127.0
80.90	3975.0
81.90	783.0
83.00	154.0
85.90	155.0
87.00	3447.0
87.90	3112.0
90.90	365.0
92.00	2788.0
93.00	3864.0
94.00	11221.0
95.00	89880.0
96.00	6205.0
97.00	226.0
103.90	491.0
104.80	193.0
105.90	593.0
106.80	137.0
110.80	103.0
112.80	116.0
114.80	143.0
115.80	348.0
116.80	653.0
117.80	387.0
118.90	617.0
127.90	313.0
128.90	224.0
129.80	275.0
130.90	167.0
134.80	191.0
136.90	183.0
140.90	1009.0
142.90	1069.0
144.80	114.0
145.90	147.0
147.90	198.0
149.90	122.0
154.90	189.0
156.80	116.0
160.80	128.0
171.90	566.0
173.00	837.0
173.90	62304.0
174.90	4613.0
175.90	58640.0
176.90	3969.0
177.80	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	1041.0
37.00	5601.0
38.00	5092.0
39.00	1959.0
40.00	413.0
42.80	109.0
44.00	1033.0
45.00	1045.0
46.10	134.0
47.00	1085.0
47.90	733.0
49.00	4983.0
50.00	20656.0
51.00	6827.0
52.00	423.0
54.90	330.0
56.00	1684.0
57.00	3140.0
57.90	164.0
60.00	1134.0
61.00	5476.0
62.00	5253.0
63.00	4132.0
64.00	484.0
64.90	393.0
66.90	278.0
68.00	10932.0
69.00	10292.0
70.00	932.0
72.00	446.0
73.00	5108.0
74.00	18056.0
75.00	53336.0
76.00	4353.0
77.00	679.0
78.00	385.0
78.90	3998.0
79.90	1196.0
80.90	4093.0
81.90	816.0
83.00	188.0
85.80	163.0
87.00	3613.0
87.90	3412.0
90.90	423.0
92.00	3081.0
93.00	4253.0
94.00	11846.0
95.00	96544.0
96.00	6671.0
97.10	258.0
103.90	510.0
104.90	204.0
105.90	613.0
106.80	138.0
110.90	108.0
112.80	111.0
114.80	161.0
115.70	357.0
116.90	678.0
117.90	386.0
119.00	646.0
123.90	104.0
127.90	348.0
128.90	209.0
129.90	310.0
130.90	170.0
134.80	227.0
137.00	169.0
140.90	1102.0
142.90	1089.0
144.80	121.0
145.80	160.0
148.00	208.0
149.90	162.0
155.00	198.0
156.90	152.0
158.80	113.0
160.80	167.0
171.90	536.0
173.00	943.0
173.90	67712.0
175.00	5007.0
175.90	64872.0
176.90	4462.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	936.0
37.00	5467.0
38.00	4953.0
39.00	1839.0
40.00	386.0
41.00	104.0
42.90	118.0
44.00	962.0
45.00	1003.0
46.00	108.0
47.00	1102.0
47.90	751.0
49.00	4661.0
50.00	19688.0
51.00	6557.0
52.00	376.0
55.00	347.0
56.00	1678.0
57.00	2963.0
57.90	139.0
60.00	1149.0
61.00	5297.0
62.00	4895.0
63.00	4131.0
64.00	497.0
65.00	403.0
66.90	242.0
68.00	10375.0
69.00	9918.0
70.00	951.0
72.00	415.0
73.00	5046.0
74.00	17288.0
75.00	50808.0
76.00	4100.0
77.00	565.0
78.00	339.0
78.90	3699.0
79.90	1075.0
80.90	3801.0
81.90	779.0
83.00	175.0
85.80	166.0
87.00	3452.0
87.90	3420.0
90.90	429.0
92.00	2976.0
93.00	4185.0
94.00	11370.0
95.00	93032.0
96.00	6298.0
97.10	276.0
103.90	443.0
104.90	189.0
105.90	563.0
106.70	129.0
110.90	105.0
114.80	141.0
115.70	326.0
116.90	662.0
117.90	404.0
118.90	624.0
123.90	115.0
127.80	381.0
128.80	197.0
129.80	296.0
130.90	171.0
134.80	208.0
136.90	129.0
140.90	1077.0
141.80	102.0
142.90	1020.0
144.80	122.0
145.80	168.0
147.90	197.0
149.90	190.0
155.00	186.0
156.90	172.0
158.80	109.0
160.80	167.0
171.90	497.0
173.90	66776.0
175.00	4917.0
175.90	64712.0
176.90	4343.0
177.90	175.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
39.90	271.0
43.90	480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39