

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042121\
 Data File : VW021086.D
 Acq On : 21 Apr 2021 18:20
 Operator : SY/MD
 Sample : M2067-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0

Manual Integrations
 APPROVED

MMDadoda
 4/23/2021 2:50:03 PM

Quant Time: Apr 22 06:44:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 22 06:32:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	610154	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	583268	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	273833	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	217564	43.39	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.78%		
7) Chloroethane-d5	1.568	69	169252	45.89	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.78%		
11) 1,1-Dichloroethene-d2	2.108	63	318222	34.41	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.82%		
21) 2-Butanone-d5	3.905	46	237593	97.04	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.04%		
24) Chloroform-d	4.352	84	416641	46.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.22%		
26) 1,2-Dichloroethane-d4	5.037	65	288721	50.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.64%		
32) Benzene-d6	5.053	84	772091	49.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.40%		
36) 1,2-Dichloropropane-d6	6.072	67	229776	49.56	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.12%		
41) Toluene-d8	7.320	98	707467	47.06	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.12%		
43) trans-1,3-Dichloroprop...	7.625	79	119089	47.00	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.00%		
47) 2-Hexanone-d5	8.095	63	196526	106.86	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	106.86%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	334225	47.79	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.58%		
66) 1,2-Dichlorobenzene-d4	11.631	152	289077	53.44	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.88%		
Target Compounds						Qvalue
13) Acetone	2.201	43	5703m	2.49	ug/L	
18) Methyl tert-butyl Ether	2.770	73	6974966	542.90	ug/L	99
33) Benzene	5.104	78	189321	11.64	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021086.D
Acq On : 21 Apr 2021 18:20
Operator : SY/MD
Sample : M2067-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG7B0

Manual Integrations
APPROVED

MMDadoda
4/23/2021 2:50:03 PM


Quant Time: Apr 22 06:44:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 22 06:32:19 2021
Response via : Initial Calibration

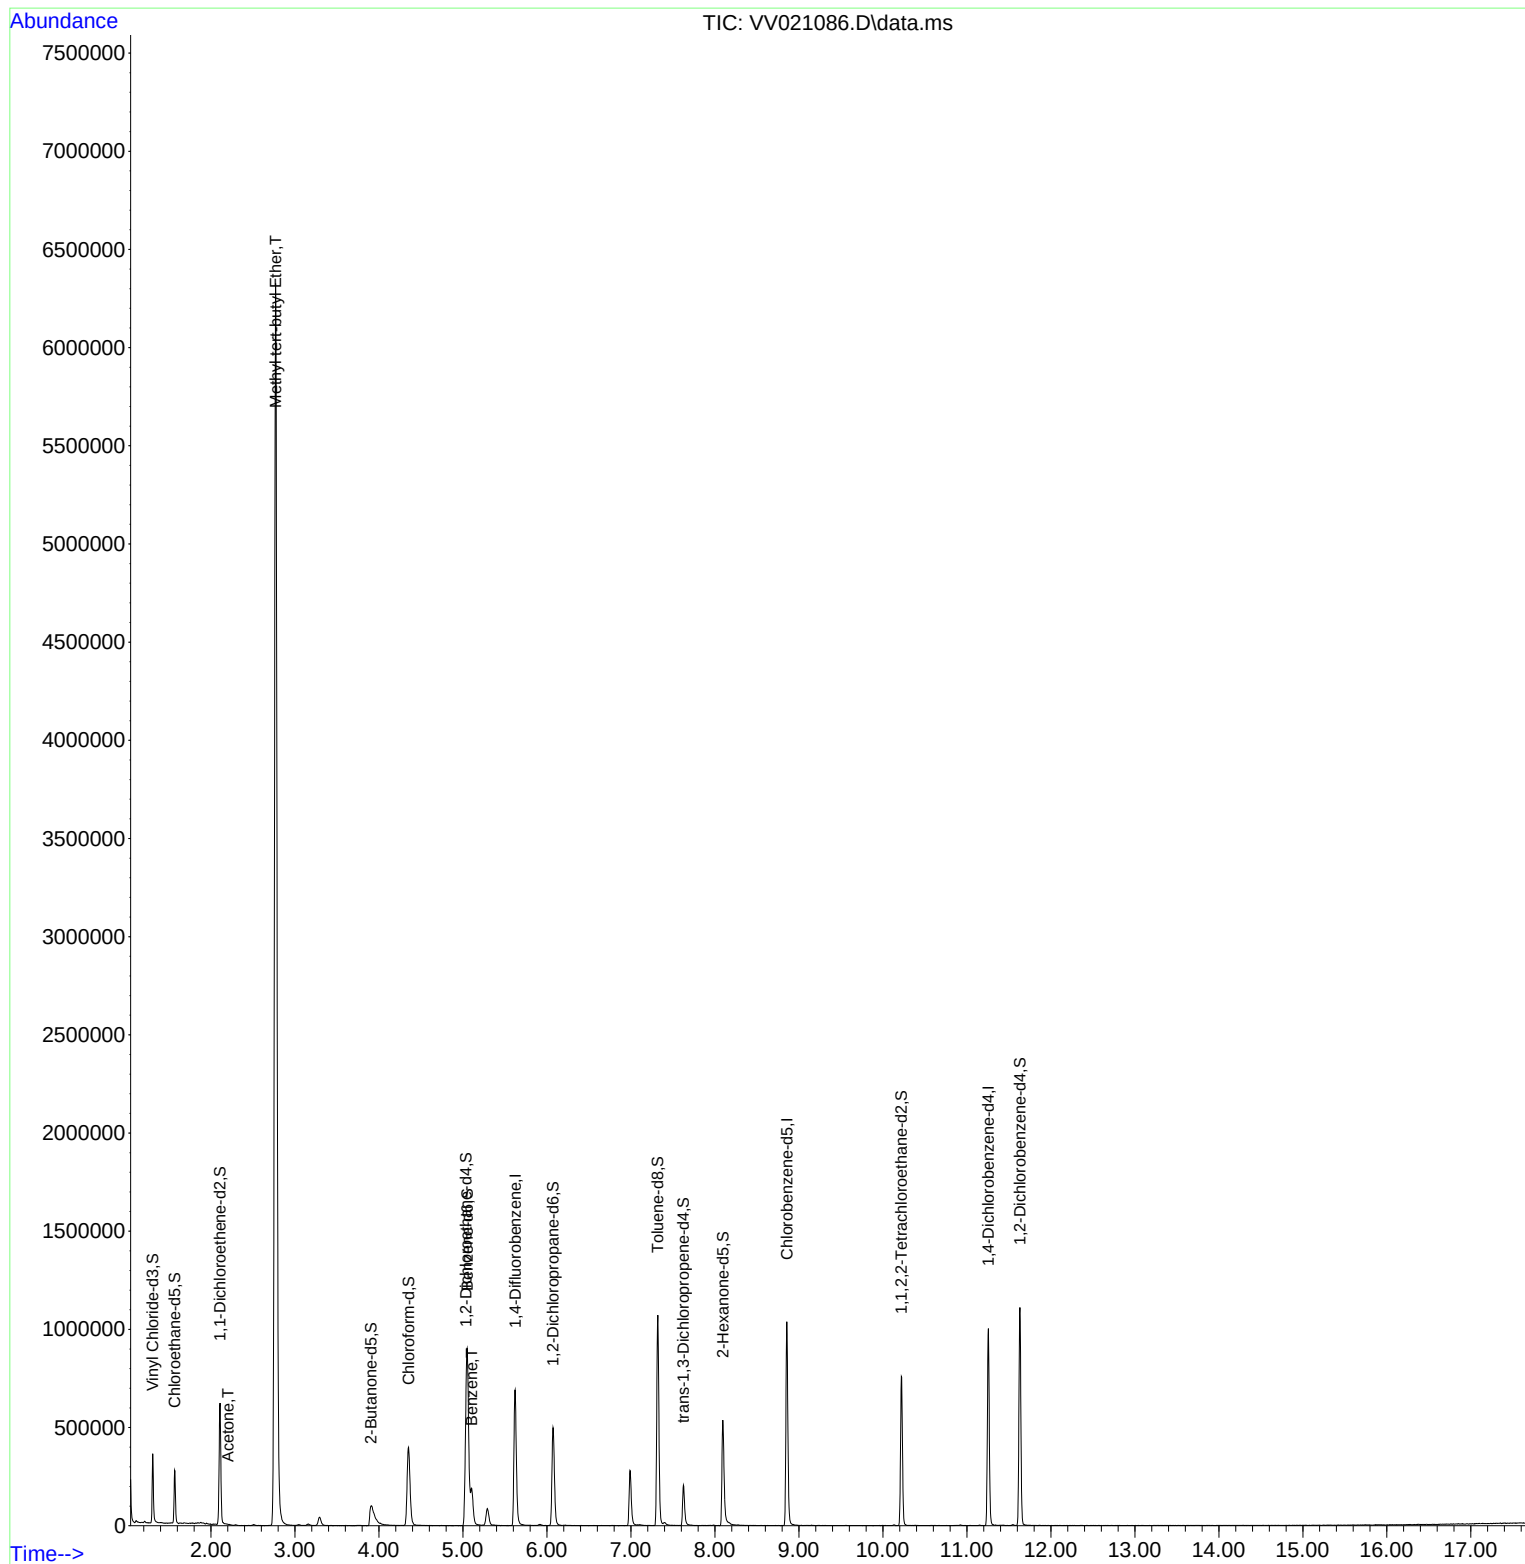

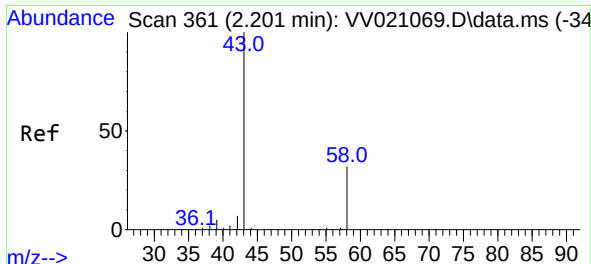

#13
Acetone
Concen: 2.49 ug/L m
RT: 2.201 min Scan# 361
Delta R.T. -0.000 min
Lab File: VV021086.D
Acq: 21 Apr 2021 18:20




Instrument :
MSVOA_V
ClientSampled :
BG7B0

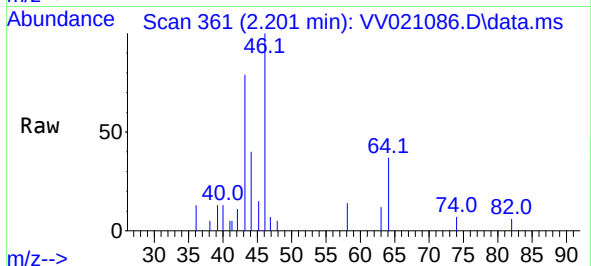


Tgt Ion: 43 Resp: 5703
Ion Ratio Lower Upper
43 100
58 0.8 0.0 30.8

Manual Integrations
APPROVED



MMDadoda
4/23/2021 2:50:03 PM

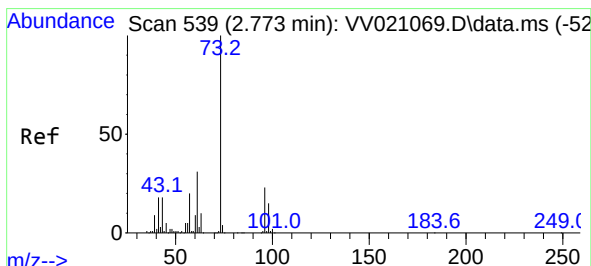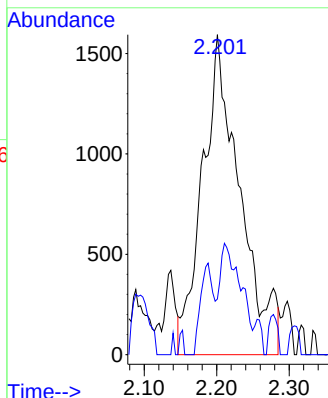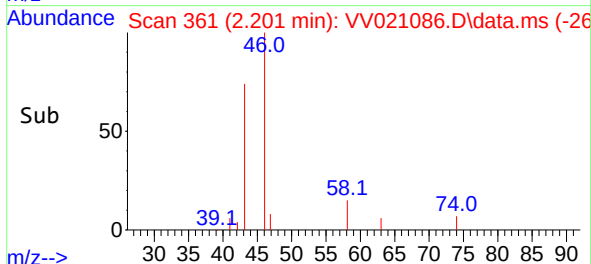


#18
Methyl tert-butyl Ether
Concen: 542.90 ug/L
RT: 2.770 min Scan# 538
Delta R.T. -0.003 min
Lab File: VV021086.D
Acq: 21 Apr 2021 18:20

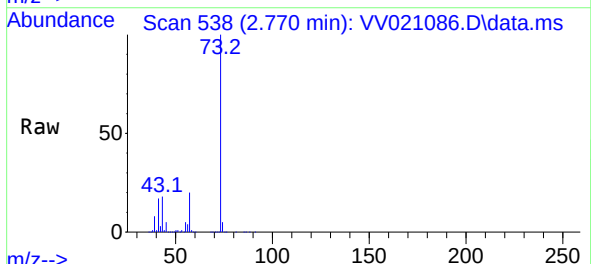

Tgt Ion: 73 Resp: 6974966
Ion Ratio Lower Upper
73 100
43 18.1 14.7 22.1
57 20.2 15.9 23.9

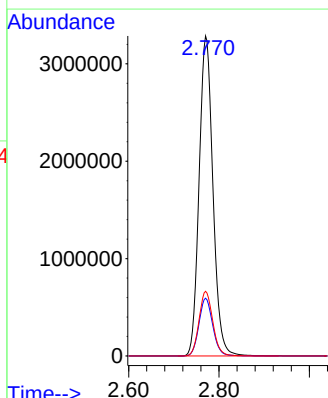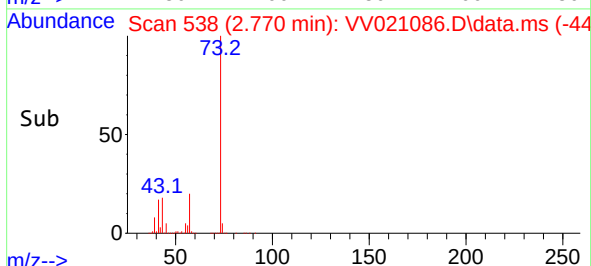

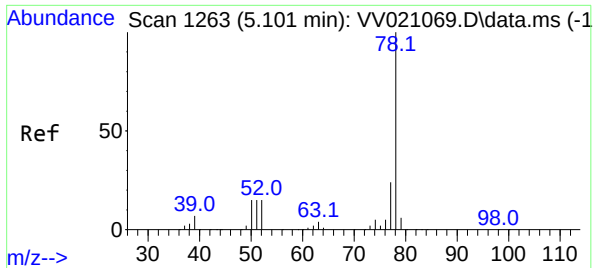

#33

Benzene

Concen: 11.64 ug/L

RT: 5.104 min Scan# 1264

Delta R.T. 0.003 min

Lab File: VV021086.D

Acq: 21 Apr 2021 18:20

Tgt Ion: 78 Resp: 189321

Instrument :
MSVOA_V
ClientSampleId :
BG7B0

Manual Integrations
APPROVED

MMDadoda
4/23/2021 2:50:03 PM

