

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021075.D
 Acq On : 21 Apr 2021 14:03
 Operator : SY/MD
 Sample : M2067-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	79	84	95	rVB	57109	60044	5.25%	1.218%
2	1.571	160	165	178	rVB	55986	62446	5.47%	1.267%
3	2.111	325	333	345	rVB	115896	166780	14.60%	3.383%
4	2.388	416	419	422	rBV3	917	538	0.05%	0.011%
5	2.510	449	457	470	rVB2	7273	13136	1.15%	0.266%
6	2.561	470	473	476	rBV3	455	265	0.02%	0.005%
7	2.603	480	486	489	rBV4	1330	1540	0.13%	0.031%
8	2.716	519	521	523	rVB2	599	272	0.02%	0.006%
9	2.773	523	539	556	rBV2	54382	119328	10.44%	2.420%
10	2.918	581	584	588	rBV2	629	391	0.03%	0.008%
11	2.986	604	605	608	rVB	632	248	0.02%	0.005%
12	3.008	608	612	613	rBV	521	342	0.03%	0.007%
13	3.053	619	626	631	rBV2	884	1129	0.10%	0.023%
14	3.230	677	681	683	rBV2	538	420	0.04%	0.009%
15	3.542	772	778	783	rBV2	686	619	0.05%	0.013%
16	3.593	793	794	799	rVB2	430	254	0.02%	0.005%
17	3.622	799	803	806	rBV3	401	326	0.03%	0.007%
18	3.661	811	815	818	rVB4	365	240	0.02%	0.005%
19	3.680	818	821	823	rBV	683	410	0.04%	0.008%
20	3.809	858	861	865	rVB3	600	392	0.03%	0.008%
21	3.828	865	867	871	rVB2	564	333	0.03%	0.007%
22	3.908	880	892	934	rBV2	128629	525224	45.97%	10.653%
23	4.355	1017	1031	1054	rBV2	85940	212849	18.63%	4.317%
24	4.564	1092	1096	1099	rBV3	990	881	0.08%	0.018%
25	4.674	1127	1130	1131	rBV2	510	300	0.03%	0.006%
26	4.748	1149	1153	1157	rBV3	799	829	0.07%	0.017%
27	4.815	1171	1174	1176	rBV2	477	294	0.03%	0.006%
28	4.831	1176	1179	1184	rBV5	677	606	0.05%	0.012%
29	4.931	1206	1210	1211	rBV2	359	270	0.02%	0.005%
30	5.050	1232	1247	1271	rBV3	183683	486673	42.59%	9.871%
31	5.262	1311	1313	1316	rVB2	504	275	0.02%	0.006%
32	5.326	1331	1333	1337	rVB2	820	493	0.04%	0.010%
33	5.352	1337	1341	1343	rBV	441	257	0.02%	0.005%
34	5.371	1343	1347	1350	rBV3	1102	872	0.08%	0.018%
35	5.404	1355	1357	1360	rVV	493	291	0.03%	0.006%
36	5.461	1368	1375	1377	rBV3	711	655	0.06%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021075.D
 Acq On : 21 Apr 2021 14:03
 Operator : SY/MD
 Sample : M2067-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.625	1414	1426	1448	rBV	107591	233512	20.44%	4.736%
38	5.796	1476	1479	1480	rBV	489	253	0.02%	0.005%
39	5.847	1492	1495	1498	rVB	795	413	0.04%	0.008%
40	5.863	1498	1500	1503	rBV2	625	369	0.03%	0.007%
41	5.918	1510	1517	1519	rBV5	1831	2015	0.18%	0.041%
42	5.986	1534	1538	1544	rVB2	922	874	0.08%	0.018%
43	6.018	1544	1548	1552	rBV3	544	472	0.04%	0.010%
44	6.076	1552	1566	1585	rBV2	104445	224335	19.63%	4.550%
45	6.240	1614	1617	1619	rBV2	525	391	0.03%	0.008%
46	6.278	1626	1629	1631	rBV2	574	402	0.04%	0.008%
47	6.323	1641	1643	1646	rVB2	620	299	0.03%	0.006%
48	6.407	1666	1669	1672	rVB3	598	440	0.04%	0.009%
49	6.445	1673	1681	1685	rVB4	413	575	0.05%	0.012%
50	6.474	1685	1690	1691	rBV	392	312	0.03%	0.006%
51	6.494	1694	1696	1698	rBV	527	333	0.03%	0.007%
52	6.526	1704	1706	1708	rBV	398	246	0.02%	0.005%
53	6.587	1722	1725	1729	rVV2	365	326	0.03%	0.007%
54	6.680	1750	1754	1759	rVB3	887	881	0.08%	0.018%
55	6.719	1763	1766	1770	rVB3	857	454	0.04%	0.009%
56	6.995	1842	1852	1866	rBV	50416	96496	8.45%	1.957%
57	7.175	1904	1908	1911	rBV3	454	365	0.03%	0.007%
58	7.249	1929	1931	1932	rBV2	741	279	0.02%	0.006%
59	7.323	1939	1954	1974	rBV	195205	354552	31.03%	7.191%
60	7.632	2039	2050	2068	rBV2	34371	67798	5.93%	1.375%
61	7.799	2099	2102	2103	rBV2	444	274	0.02%	0.006%
62	7.924	2138	2141	2143	rBV3	584	332	0.03%	0.007%
63	8.053	2176	2181	2183	rBV2	610	541	0.05%	0.011%
64	8.095	2183	2194	2219	rBV	618690	1142625	100.00%	23.176%
65	8.632	2358	2361	2364	rVB3	656	415	0.04%	0.008%
66	8.670	2370	2373	2377	rBV3	698	480	0.04%	0.010%
67	8.719	2383	2388	2391	rBV2	921	713	0.06%	0.014%
68	8.735	2391	2393	2397	rBV2	372	265	0.02%	0.005%
69	8.754	2397	2399	2400	rBV	557	264	0.02%	0.005%
70	8.860	2421	2432	2447	rBV	171104	285887	25.02%	5.799%
71	9.059	2492	2494	2497	rBV2	870	419	0.04%	0.008%
72	9.288	2561	2565	2566	rBV2	576	433	0.04%	0.009%
73	9.336	2576	2580	2582	rBV2	526	327	0.03%	0.007%
74	9.410	2596	2603	2606	rBV3	634	809	0.07%	0.016%
75	9.513	2630	2635	2639	rBV6	975	1170	0.10%	0.024%
76	9.805	2723	2726	2727	rBV	407	262	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021075.D
 Acq On : 21 Apr 2021 14:03
 Operator : SY/MD
 Sample : M2067-16 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.895	2751	2754	2756	rBV	524	334	0.03%	0.007%
78	10.008	2787	2789	2794	rVB3	497	365	0.03%	0.007%
79	10.095	2813	2816	2817	rBV2	526	275	0.02%	0.006%
80	10.223	2845	2856	2871	rBV	168786	267068	23.37%	5.417%
81	10.355	2895	2897	2900	rVB2	483	277	0.02%	0.006%
82	10.426	2916	2919	2925	rVB3	1024	679	0.06%	0.014%
83	10.500	2939	2942	2945	rBV	930	625	0.05%	0.013%
84	10.519	2945	2948	2952	rVV2	538	533	0.05%	0.011%
85	10.545	2952	2956	2960	rVV3	1007	1104	0.10%	0.022%
86	10.802	3030	3036	3039	rBV2	618	686	0.06%	0.014%
87	10.834	3044	3046	3048	rBV2	516	249	0.02%	0.005%
88	11.059	3113	3116	3118	rVB	477	236	0.02%	0.005%
89	11.098	3123	3128	3132	rBV2	793	781	0.07%	0.016%
90	11.149	3142	3144	3145	rBV2	517	248	0.02%	0.005%
91	11.178	3151	3153	3155	rBV	537	301	0.03%	0.006%
92	11.255	3167	3177	3197	rBV2	151610	244718	21.42%	4.964%
93	11.390	3217	3219	3223	rVB3	1141	654	0.06%	0.013%
94	11.419	3224	3228	3229	rBV2	538	339	0.03%	0.007%
95	11.513	3254	3257	3260	rBV2	652	426	0.04%	0.009%
96	11.632	3283	3294	3313	rBV	201784	326147	28.54%	6.615%
97	12.024	3414	3416	3418	rBV	598	250	0.02%	0.005%
98	12.612	3593	3599	3603	rBV2	569	738	0.06%	0.015%
99	12.779	3647	3651	3655	rBV4	743	799	0.07%	0.016%
100	12.934	3696	3699	3702	rBV3	862	642	0.06%	0.013%




Sum of corrected areas: 4930304

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021075.D
Acq On : 21 Apr 2021 14:03
Operator : SY/MD
Sample : M2067-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

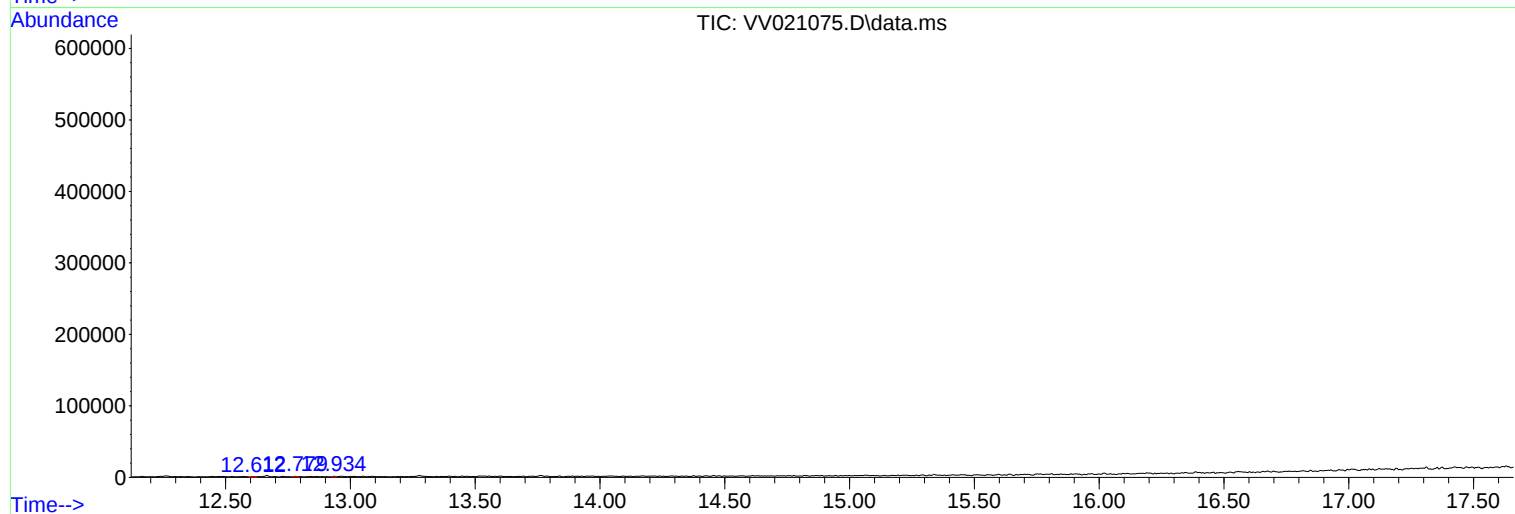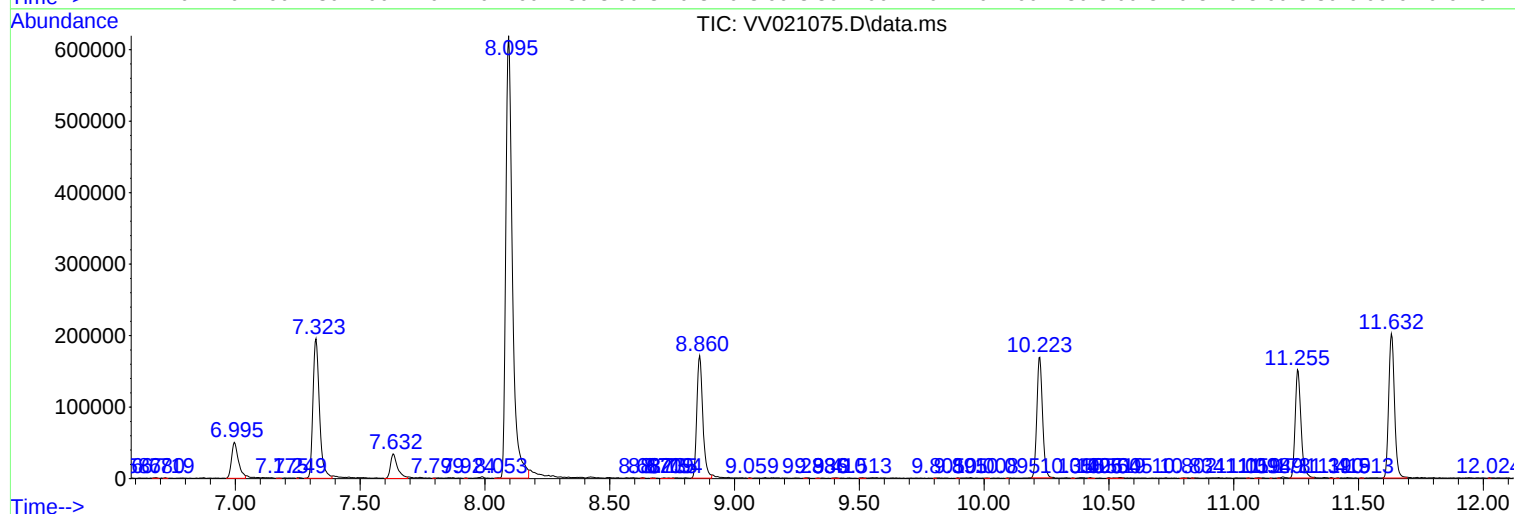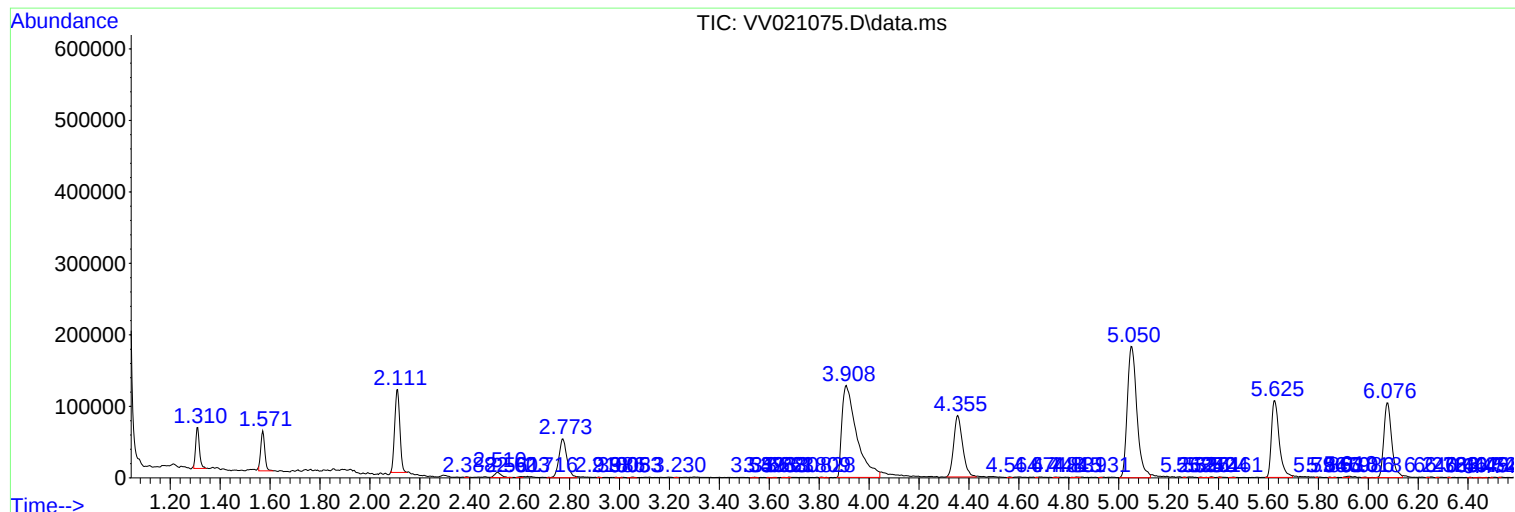

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021075.D
Acq On : 21 Apr 2021 14:03
Operator : SY/MD
Sample : M2067-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021075.D
Acq On : 21 Apr 2021 14:03
Operator : SY/MD
Sample : M2067-16 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
