

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021077.D
 Acq On : 21 Apr 2021 14:49
 Operator : SY/MD
 Sample : VIBLK24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	412684	419905	16.72%	2.219%
2	1.571	158	165	180	rVB	313121	356312	14.19%	1.883%
3	2.108	323	332	346	rBV	684224	976792	38.90%	5.163%
4	2.346	404	406	408	rBV2	827	354	0.01%	0.002%
5	2.407	421	425	427	rBV3	846	746	0.03%	0.004%
6	2.671	502	507	509	rBV2	1499	1417	0.06%	0.007%
7	3.047	616	624	635	rVV7	4925	9549	0.38%	0.050%
8	3.089	635	637	640	rVB2	768	362	0.01%	0.002%
9	3.134	649	651	657	rVB3	468	355	0.01%	0.002%
10	3.179	663	665	667	rBV2	456	203	0.01%	0.001%
11	3.188	667	668	669	rBV2	410	109	0.00%	0.001%
12	3.224	677	679	684	rVB4	691	397	0.02%	0.002%
13	3.294	686	701	714	rBV3	24797	56035	2.23%	0.296%
14	3.410	734	737	739	rBV2	599	428	0.02%	0.002%
15	3.529	773	774	777	rBV2	181	108	0.00%	0.001%
16	3.558	780	783	786	rBV2	215	143	0.01%	0.001%
17	3.577	786	789	792	rBV	391	246	0.01%	0.001%
18	3.642	807	809	810	rBV	416	158	0.01%	0.001%
19	3.658	810	814	817	rVB	623	452	0.02%	0.002%
20	3.706	827	829	832	rBV	180	86	0.00%	0.000%
21	3.735	835	838	839	rBV	756	328	0.01%	0.002%
22	3.847	871	873	875	rBV	502	201	0.01%	0.001%
23	3.908	879	892	930	rBV2	111215	441550	17.58%	2.334%
24	4.352	1013	1030	1055	rBV	434727	1070889	42.65%	5.660%
25	4.732	1145	1148	1151	rVB2	612	339	0.01%	0.002%
26	4.777	1159	1162	1167	rBV2	897	1021	0.04%	0.005%
27	4.822	1172	1176	1179	rVV3	734	562	0.02%	0.003%
28	4.841	1180	1182	1184	rBB3	754	329	0.01%	0.002%
29	4.854	1184	1186	1187	rBV3	345	133	0.01%	0.001%
30	4.924	1206	1208	1210	rBV	441	209	0.01%	0.001%
31	4.979	1223	1225	1228	rVB	548	238	0.01%	0.001%
32	5.050	1228	1247	1276	rBV2	969821	2510970	100.00%	13.271%
33	5.481	1379	1381	1383	rBV2	304	165	0.01%	0.001%
34	5.551	1400	1403	1406	rBV2	940	551	0.02%	0.003%
35	5.622	1412	1425	1453	rBV	594763	1200825	47.82%	6.347%
36	5.924	1506	1519	1535	rBV6	35065	76151	3.03%	0.402%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021077.D
 Acq On : 21 Apr 2021 14:49
 Operator : SY/MD
 Sample : VIBLK24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.072	1552	1565	1590	rBV	538196	1106958	44.08%	5.850%
38	6.307	1636	1638	1642	rVB3	974	578	0.02%	0.003%
39	6.410	1666	1670	1672	rBV3	735	473	0.02%	0.002%
40	6.445	1679	1681	1683	rBV2	425	172	0.01%	0.001%
41	6.484	1691	1693	1697	rBV4	475	340	0.01%	0.002%
42	6.542	1706	1711	1713	rBV3	1019	670	0.03%	0.004%
43	6.619	1733	1735	1736	rBV	362	193	0.01%	0.001%
44	6.760	1777	1779	1782	rVB2	463	300	0.01%	0.002%
45	6.870	1811	1813	1820	rVB2	682	504	0.02%	0.003%
46	6.902	1820	1823	1825	rBV	516	358	0.01%	0.002%
47	6.937	1833	1834	1837	rBV	307	142	0.01%	0.001%
48	6.989	1838	1850	1874	rBV	312516	566193	22.55%	2.992%
49	7.320	1941	1953	1972	rBV	1183250	2036542	81.11%	10.764%
50	7.625	2038	2048	2071	rBV	222870	389351	15.51%	2.058%
51	7.854	2116	2119	2121	rBV3	859	511	0.02%	0.003%
52	7.979	2137	2158	2176	rBV	365422	622577	24.79%	3.290%
53	8.095	2184	2194	2232	rBV	573259	1046248	41.67%	5.530%
54	8.567	2339	2341	2342	rBV	494	258	0.01%	0.001%
55	8.632	2358	2361	2364	rBV4	1125	744	0.03%	0.004%
56	8.699	2380	2382	2385	rBV2	744	376	0.01%	0.002%
57	8.712	2385	2386	2388	rBV	303	129	0.01%	0.001%
58	8.751	2395	2398	2399	rBV	353	185	0.01%	0.001%
59	8.857	2419	2431	2460	rBV	910215	1470793	58.57%	7.773%
60	9.156	2517	2524	2525	rBV5	1418	1539	0.06%	0.008%
61	9.236	2546	2549	2550	rBV	456	222	0.01%	0.001%
62	9.275	2558	2561	2562	rBV	423	251	0.01%	0.001%
63	9.307	2569	2571	2574	rBV2	497	208	0.01%	0.001%
64	9.352	2583	2585	2588	rBV3	464	214	0.01%	0.001%
65	9.445	2612	2614	2615	rBV	425	193	0.01%	0.001%
66	9.481	2621	2625	2627	rBV2	612	434	0.02%	0.002%
67	9.555	2643	2648	2651	rBV5	1247	1096	0.04%	0.006%
68	9.927	2762	2764	2766	rBV2	392	164	0.01%	0.001%
69	10.085	2810	2813	2814	rBV	601	297	0.01%	0.002%
70	10.223	2843	2856	2873	rBV	804940	1272493	50.68%	6.725%
71	10.481	2934	2936	2940	rBV3	781	681	0.03%	0.004%
72	10.551	2954	2958	2959	rBV4	701	520	0.02%	0.003%
73	10.905	3064	3068	3069	rBV3	1889	1162	0.05%	0.006%
74	11.075	3116	3121	3123	rBV2	576	565	0.02%	0.003%
75	11.146	3137	3143	3145	rBV3	2764	2592	0.10%	0.014%
76	11.194	3155	3158	3160	rBV2	1461	1008	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021077.D
 Acq On : 21 Apr 2021 14:49
 Operator : SY/MD
 Sample : VIBLK24
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	11.255	3165	3177	3197	rBV	878509	1363506	54.30%	7.206%
78	11.542	3264	3266	3267	rBV	559	291	0.01%	0.002%
79	11.632	3281	3294	3314	rBV	1200658	1895321	75.48%	10.017%
80	11.796	3339	3345	3347	rBV5	1762	2205	0.09%	0.012%
81	12.249	3482	3486	3488	rBV2	805	732	0.03%	0.004%
82	12.471	3553	3555	3558	rBV	475	214	0.01%	0.001%
83	12.651	3608	3611	3613	rBV3	730	407	0.02%	0.002%
84	12.943	3700	3702	3705	rBV	819	379	0.02%	0.002%
85	13.509	3875	3878	3880	rBV3	1295	900	0.04%	0.005%




Sum of corrected areas: 18920807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021077.D
Acq On : 21 Apr 2021 14:49
Operator : SY/MD
Sample : VIBLK24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

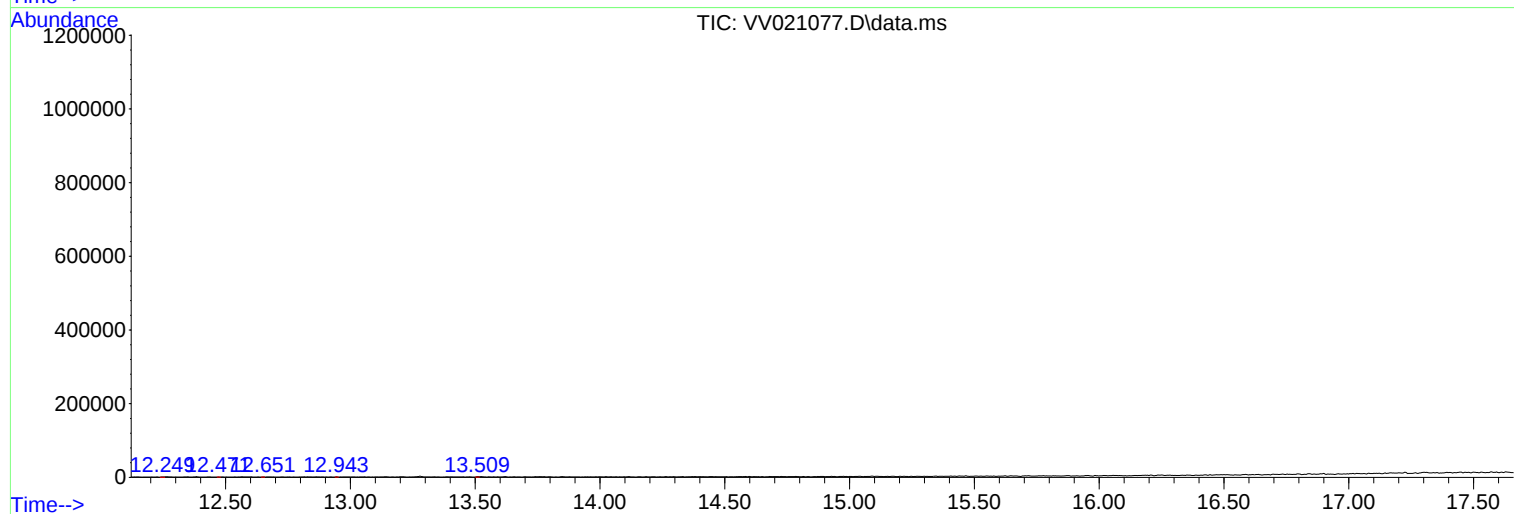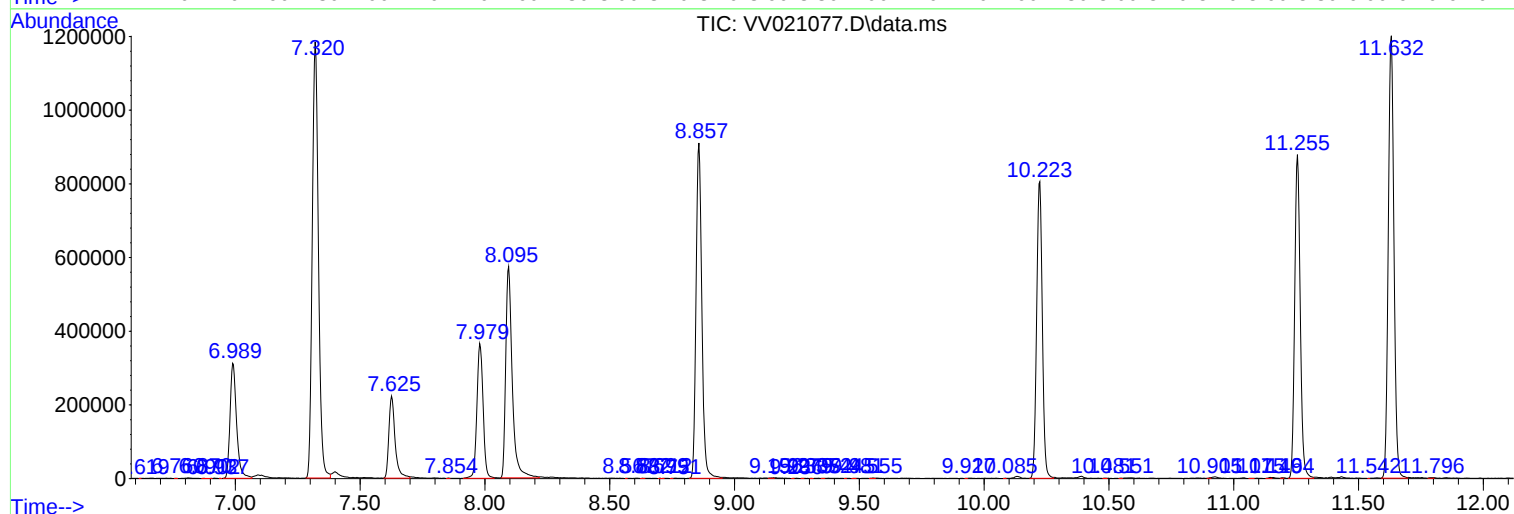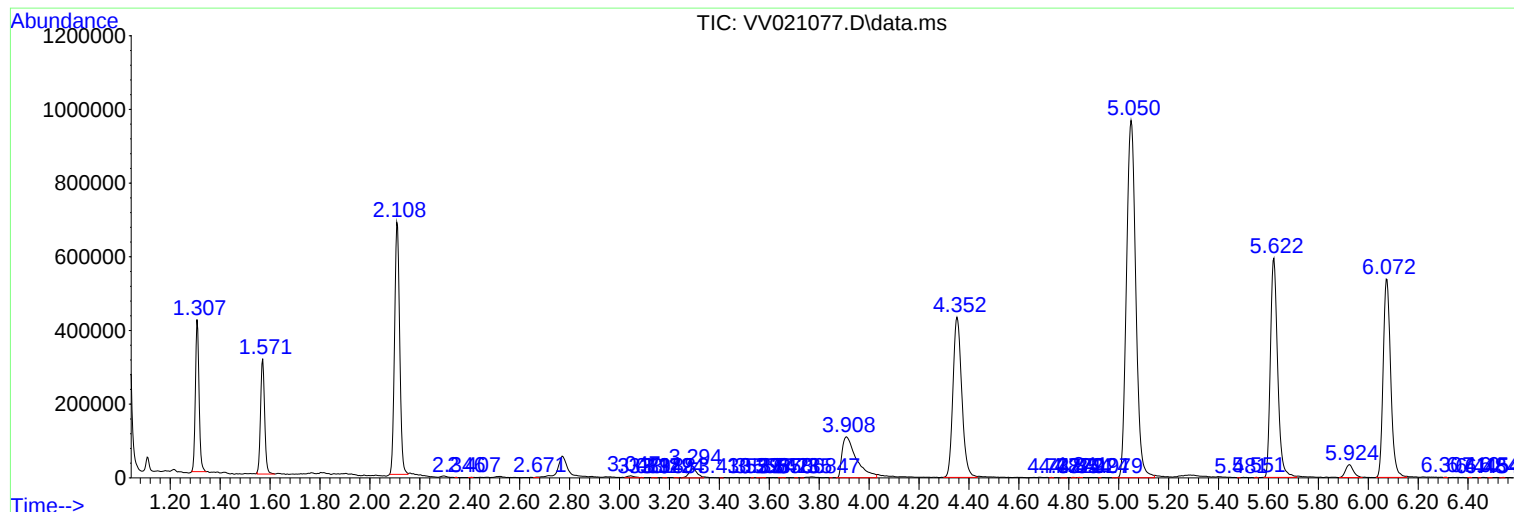

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021077.D
Acq On : 21 Apr 2021 14:49
Operator : SY/MD
Sample : VIBLK24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021077.D
Acq On : 21 Apr 2021 14:49
Operator : SY/MD
Sample : VIBLK24
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------