

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021079.D
 Acq On : 21 Apr 2021 15:36
 Operator : SY/MD
 Sample : M2067-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	374846	389246	16.14%	2.137%
2	1.571	158	165	178	rVB	293307	334150	13.86%	1.834%
3	2.108	322	332	350	rBV	647013	942829	39.10%	5.176%
4	2.368	407	413	414	rBV4	582	625	0.03%	0.003%
5	2.391	418	420	422	rBV	904	480	0.02%	0.003%
6	2.510	449	457	466	rBV5	3839	6583	0.27%	0.036%
7	2.635	493	496	498	rBV	443	272	0.01%	0.001%
8	2.648	498	500	503	rBV2	512	368	0.02%	0.002%
9	2.748	529	531	536	rBV3	640	267	0.01%	0.001%
10	2.870	567	569	571	rBV	478	261	0.01%	0.001%
11	3.060	626	628	630	rBV2	557	249	0.01%	0.001%
12	3.073	630	632	634	rBV2	387	223	0.01%	0.001%
13	3.121	642	647	651	rBV2	483	584	0.02%	0.003%
14	3.201	669	672	675	rBV2	396	223	0.01%	0.001%
15	3.253	684	688	689	rBV2	668	320	0.01%	0.002%
16	3.294	694	701	702	rBV2	601	604	0.03%	0.003%
17	3.391	729	731	735	rVB2	639	335	0.01%	0.002%
18	3.526	768	773	779	rVB3	509	608	0.03%	0.003%
19	3.574	785	788	790	rBV2	643	427	0.02%	0.002%
20	3.651	810	812	814	rBV2	573	261	0.01%	0.001%
21	3.690	821	824	826	rBV2	589	435	0.02%	0.002%
22	3.831	865	868	870	rBV2	387	234	0.01%	0.001%
23	3.857	874	876	878	rBV2	435	224	0.01%	0.001%
24	3.912	881	893	948	rBV	101558	440087	18.25%	2.416%
25	4.352	1014	1030	1053	rBV2	416504	1025592	42.53%	5.630%
26	4.661	1121	1126	1128	rBV2	1106	981	0.04%	0.005%
27	4.989	1225	1228	1230	rBV	788	465	0.02%	0.003%
28	5.050	1230	1247	1290	rVV2	948676	2411300	100.00%	13.237%
29	5.336	1333	1336	1344	rVB6	1336	1177	0.05%	0.006%
30	5.404	1354	1357	1359	rBV2	696	427	0.02%	0.002%
31	5.426	1359	1364	1368	rVB5	1131	1215	0.05%	0.007%
32	5.507	1385	1389	1393	rBV4	1026	761	0.03%	0.004%
33	5.526	1393	1395	1401	rVB3	754	679	0.03%	0.004%
34	5.561	1401	1406	1409	rBV3	878	787	0.03%	0.004%
35	5.622	1412	1425	1458	rBV	690036	1396667	57.92%	7.667%
36	5.915	1507	1516	1528	rBV7	10956	22930	0.95%	0.126%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021079.D
 Acq On : 21 Apr 2021 15:36
 Operator : SY/MD
 Sample : M2067-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.072	1551	1565	1591	rBV	520064	1070687	44.40%	5.878%
38	6.471	1687	1689	1691	rBV2	387	199	0.01%	0.001%
39	6.535	1706	1709	1710	rBV	502	262	0.01%	0.001%
40	6.574	1719	1721	1723	rVB	667	213	0.01%	0.001%
41	6.635	1737	1740	1741	rBV2	410	229	0.01%	0.001%
42	6.645	1741	1743	1747	rBV3	487	384	0.02%	0.002%
43	6.670	1747	1751	1754	rBV2	880	770	0.03%	0.004%
44	6.764	1778	1780	1783	rVB2	670	363	0.02%	0.002%
45	6.780	1783	1785	1787	rBV2	531	301	0.01%	0.002%
46	6.793	1787	1789	1792	rVB	440	195	0.01%	0.001%
47	6.847	1804	1806	1809	rBV2	398	218	0.01%	0.001%
48	6.941	1832	1835	1838	rBV3	510	395	0.02%	0.002%
49	6.989	1840	1850	1879	rVV	296106	543888	22.56%	2.986%
50	7.178	1907	1909	1913	rBV2	843	566	0.02%	0.003%
51	7.240	1926	1928	1934	rBV4	692	781	0.03%	0.004%
52	7.320	1941	1953	1972	rBV	1127336	1955928	81.12%	10.737%
53	7.625	2038	2048	2064	rBV	214099	363436	15.07%	1.995%
54	7.870	2122	2124	2129	rVB3	616	448	0.02%	0.002%
55	7.924	2138	2141	2142	rBV	945	510	0.02%	0.003%
56	7.986	2156	2160	2169	rVB9	2719	3429	0.14%	0.019%
57	8.056	2179	2182	2183	rBV	782	384	0.02%	0.002%
58	8.095	2183	2194	2221	rBV	534575	994560	41.25%	5.460%
59	8.522	2325	2327	2330	rVB2	1088	470	0.02%	0.003%
60	8.555	2335	2337	2340	rVV2	541	233	0.01%	0.001%
61	8.596	2347	2350	2353	rBV3	553	465	0.02%	0.003%
62	8.664	2368	2371	2372	rBV2	732	407	0.02%	0.002%
63	8.748	2394	2397	2403	rBV2	524	575	0.02%	0.003%
64	8.773	2403	2405	2409	rVB2	690	435	0.02%	0.002%
65	8.796	2409	2412	2413	rBV	619	384	0.02%	0.002%
66	8.857	2419	2431	2458	rBV	1053008	1684009	69.84%	9.245%
67	9.239	2547	2550	2553	rBV2	530	387	0.02%	0.002%
68	9.297	2566	2568	2572	rVB	704	384	0.02%	0.002%
69	9.326	2574	2577	2580	rVV2	538	359	0.01%	0.002%
70	9.545	2642	2645	2646	rBV	791	430	0.02%	0.002%
71	9.603	2661	2663	2665	rVB	583	254	0.01%	0.001%
72	9.680	2685	2687	2690	rVB2	675	339	0.01%	0.002%
73	9.767	2710	2714	2716	rBV2	572	410	0.02%	0.002%
74	9.812	2726	2728	2729	rBV	779	344	0.01%	0.002%
75	9.928	2760	2764	2769	rBV4	509	376	0.02%	0.002%
76	9.976	2776	2779	2784	rVB2	897	653	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021079.D
 Acq On : 21 Apr 2021 15:36
 Operator : SY/MD
 Sample : M2067-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.030	2793	2796	2800	rVB2	950	646	0.03%	0.004%
78	10.063	2802	2806	2807	rBV	566	381	0.02%	0.002%
79	10.130	2823	2827	2838	rVB7	5319	6967	0.29%	0.038%
80	10.220	2843	2855	2874	rBV	774148	1207792	50.09%	6.630%
81	10.387	2903	2907	2915	rVB7	2794	3544	0.15%	0.019%
82	10.420	2915	2917	2919	rBV	425	196	0.01%	0.001%
83	10.490	2937	2939	2943	rBB3	467	293	0.01%	0.002%
84	10.545	2952	2956	2958	rBV3	1641	1306	0.05%	0.007%
85	10.828	3040	3044	3047	rBV2	1009	694	0.03%	0.004%
86	10.854	3048	3052	3053	rBV2	1212	800	0.03%	0.004%
87	10.928	3066	3075	3082	rBV7	3927	5969	0.25%	0.033%
88	11.056	3113	3115	3119	rBV4	973	542	0.02%	0.003%
89	11.149	3138	3144	3151	rBV8	2514	3422	0.14%	0.019%
90	11.255	3165	3177	3203	rBV	1001789	1555564	64.51%	8.539%
91	11.632	3280	3294	3315	rBV	1158336	1811725	75.13%	9.946%
92	11.899	3374	3377	3380	rVB3	826	487	0.02%	0.003%
93	12.005	3407	3410	3414	rBV2	925	482	0.02%	0.003%
94	12.082	3432	3434	3436	rBV3	1009	472	0.02%	0.003%
95	12.738	3635	3638	3640	rBV2	762	522	0.02%	0.003%
96	12.786	3650	3653	3655	rBV	746	405	0.02%	0.002%
97	12.921	3693	3695	3697	rBV2	748	379	0.02%	0.002%
98	13.259	3796	3800	3801	rBV	778	528	0.02%	0.003%
99	13.519	3878	3881	3884	rBV3	906	571	0.02%	0.003%
100	13.866	3987	3989	3992	rBV2	1063	596	0.02%	0.003%




Sum of corrected areas: 18216219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021079.D
Acq On : 21 Apr 2021 15:36
Operator : SY/MD
Sample : M2067-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG594

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

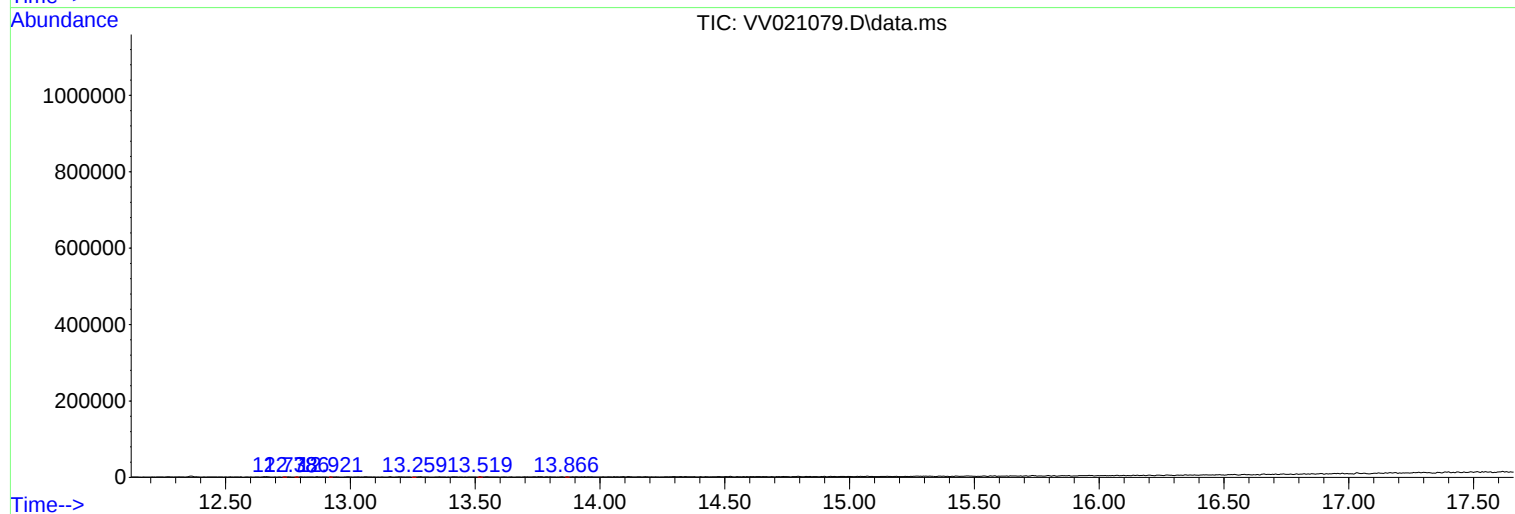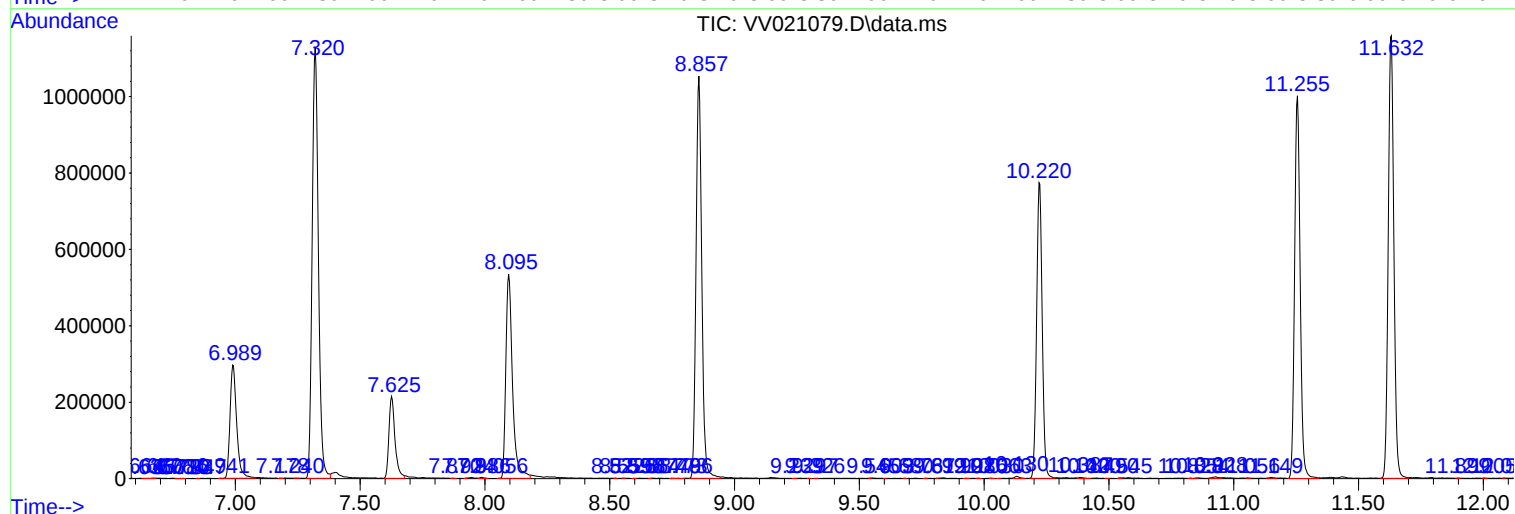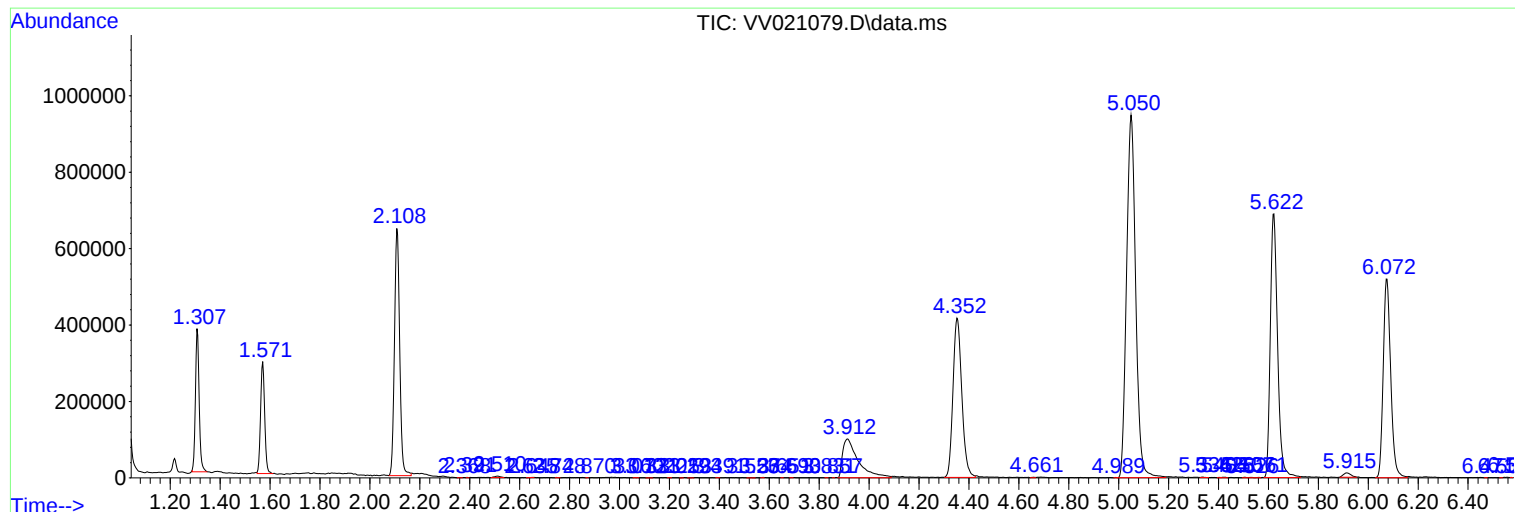

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021079.D
Acq On : 21 Apr 2021 15:36
Operator : SY/MD
Sample : M2067-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG594

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021079.D
Acq On : 21 Apr 2021 15:36
Operator : SY/MD
Sample : M2067-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG594

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------