

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021085.D
 Acq On : 21 Apr 2021 17:57
 Operator : SY/MD
 Sample : M2067-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	32	rVB2	44236	41680	0.04%	0.037%
2	1.307	77	83	101	rVB	381880	402637	0.42%	0.354%
3	1.571	158	165	179	rVB	281764	325929	0.34%	0.287%
4	2.108	323	332	347	rBV	616675	881737	0.92%	0.776%
5	2.635	493	496	498	rBV2	806	525	0.00%	0.000%
6	2.773	521	539	590	rVB2	40969870	95485625	100.00%	83.997%
7	3.465	751	754	761	rVB5	976	1012	0.00%	0.001%
8	3.706	826	829	831	rBV2	608	383	0.00%	0.000%
9	3.912	880	893	927	rBV2	105550	425061	0.45%	0.374%
10	4.352	1014	1030	1054	rBV	404753	1000772	1.05%	0.880%
11	4.529	1083	1085	1088	rBV3	824	627	0.00%	0.001%
12	4.577	1097	1100	1108	rBV5	692	901	0.00%	0.001%
13	4.703	1136	1139	1145	rBV3	642	673	0.00%	0.001%
14	4.828	1176	1178	1182	rBV2	768	567	0.00%	0.000%
15	4.892	1196	1198	1200	rBV	483	339	0.00%	0.000%
16	4.928	1206	1209	1212	rBV2	480	318	0.00%	0.000%
17	4.966	1217	1221	1224	rBV4	490	390	0.00%	0.000%
18	5.050	1228	1247	1273	rBV2	907778	2336293	2.45%	2.055%
19	5.529	1393	1396	1398	rVB2	818	413	0.00%	0.000%
20	5.548	1399	1402	1404	rBV3	633	375	0.00%	0.000%
21	5.622	1412	1425	1449	rBV	696565	1414428	1.48%	1.244%
22	5.918	1508	1517	1528	rVB	6113	11897	0.01%	0.010%
23	6.075	1551	1566	1594	rBV	507383	1035300	1.08%	0.911%
24	6.217	1608	1610	1613	rBV3	1446	1037	0.00%	0.001%
25	6.330	1642	1645	1648	rVB3	539	354	0.00%	0.000%
26	6.397	1664	1666	1671	rVB5	645	557	0.00%	0.000%
27	6.429	1671	1676	1678	rVB4	552	402	0.00%	0.000%
28	6.458	1681	1685	1689	rBV4	707	466	0.00%	0.000%
29	6.516	1700	1703	1706	rBV3	920	564	0.00%	0.000%
30	6.564	1713	1718	1720	rBV5	355	320	0.00%	0.000%
31	6.603	1725	1730	1734	rVB3	903	803	0.00%	0.001%
32	6.645	1740	1743	1747	rVV3	864	594	0.00%	0.001%
33	6.767	1778	1781	1785	rVV5	811	511	0.00%	0.000%
34	6.828	1798	1800	1806	rVB3	774	485	0.00%	0.000%
35	6.989	1838	1850	1872	rBV	288392	530149	0.56%	0.466%
36	7.252	1928	1932	1933	rBV2	872	696	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021085.D
 Acq On : 21 Apr 2021 17:57
 Operator : SY/MD
 Sample : M2067-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	7.320	1941	1953	1970	rBV	1115497	1922308	2.01%	1.691%
38	7.625	2039	2048	2070	rBV2	204437	357564	0.37%	0.315%
39	7.786	2095	2098	2100	rBV2	907	532	0.00%	0.000%
40	7.879	2122	2127	2129	rBV3	1178	1074	0.00%	0.001%
41	7.931	2140	2143	2144	rBV2	831	444	0.00%	0.000%
42	7.982	2155	2159	2162	rBV4	2210	2093	0.00%	0.002%
43	8.095	2183	2194	2234	rVV	565675	1044529	1.09%	0.919%
44	8.471	2308	2311	2314	rBV3	1072	757	0.00%	0.001%
45	8.519	2323	2326	2327	rBV3	836	411	0.00%	0.000%
46	8.551	2334	2336	2343	rVB3	1056	906	0.00%	0.001%
47	8.645	2363	2365	2366	rBV	754	402	0.00%	0.000%
48	8.693	2378	2380	2382	rVB2	720	348	0.00%	0.000%
49	8.857	2419	2431	2458	rBV	1064514	1729378	1.81%	1.521%
50	9.079	2497	2500	2502	rBV4	1384	737	0.00%	0.001%
51	9.117	2508	2512	2514	rBV3	1156	928	0.00%	0.001%
52	9.191	2532	2535	2539	rVB3	888	583	0.00%	0.001%
53	9.249	2551	2553	2558	rVB2	1084	760	0.00%	0.001%
54	9.307	2563	2571	2572	rBV3	686	702	0.00%	0.001%
55	9.397	2595	2599	2606	rBV7	796	839	0.00%	0.001%
56	9.506	2631	2633	2636	rBV2	664	323	0.00%	0.000%
57	9.554	2646	2648	2653	rVB3	753	614	0.00%	0.001%
58	9.654	2676	2679	2682	rBV2	657	524	0.00%	0.000%
59	9.950	2769	2771	2776	rVB2	770	535	0.00%	0.000%
60	10.069	2802	2808	2812	rBV3	521	633	0.00%	0.001%
61	10.133	2819	2828	2835	rBV4	4645	6169	0.01%	0.005%
62	10.172	2835	2840	2843	rBV2	537	585	0.00%	0.001%
63	10.220	2843	2855	2875	rBV	796664	1241139	1.30%	1.092%
64	10.355	2895	2897	2899	rBV2	1062	604	0.00%	0.001%
65	10.458	2927	2929	2932	rBV2	684	512	0.00%	0.000%
66	10.570	2960	2964	2965	rBV2	796	586	0.00%	0.001%
67	10.580	2965	2967	2969	rVV	760	355	0.00%	0.000%
68	10.661	2990	2992	2994	rBV	959	374	0.00%	0.000%
69	10.789	3028	3032	3035	rBV3	830	699	0.00%	0.001%
70	10.834	3040	3046	3048	rBV2	1016	892	0.00%	0.001%
71	10.857	3048	3053	3056	rBV4	1016	961	0.00%	0.001%
72	10.985	3091	3093	3097	rBV2	688	340	0.00%	0.000%
73	11.043	3107	3111	3117	rVB3	1071	1130	0.00%	0.001%
74	11.159	3139	3147	3150	rBV6	2550	3348	0.00%	0.003%
75	11.255	3165	3177	3200	rBV	1066357	1624470	1.70%	1.429%
76	11.468	3241	3243	3247	rBV3	773	638	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
 Data File : VV021085.D
 Acq On : 21 Apr 2021 17:57
 Operator : SY/MD
 Sample : M2067-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	11.558	3263	3271	3278	rBV6	2806	4216	0.00%	0.004%
78	11.632	3282	3294	3313	rVV	1140209	1796874	1.88%	1.581%
79	12.082	3430	3434	3435	rBV2	934	589	0.00%	0.001%
80	12.143	3451	3453	3455	rVB	862	363	0.00%	0.000%
81	12.159	3455	3458	3461	rVB	525	328	0.00%	0.000%
82	12.230	3477	3480	3481	rBV2	648	342	0.00%	0.000%
83	12.239	3481	3483	3487	rVV3	966	623	0.00%	0.001%
84	12.255	3487	3488	3493	rVB4	824	415	0.00%	0.000%
85	12.287	3493	3498	3501	rBV3	759	594	0.00%	0.001%
86	12.358	3513	3520	3531	rBV8	6014	8626	0.01%	0.008%
87	12.477	3555	3557	3559	rBV2	781	422	0.00%	0.000%
88	12.532	3570	3574	3579	rBV3	955	973	0.00%	0.001%
89	12.558	3579	3582	3587	rVB4	834	649	0.00%	0.001%
90	12.580	3587	3589	3592	rBV2	556	327	0.00%	0.000%
91	12.648	3607	3610	3611	rBV	653	364	0.00%	0.000%
92	12.779	3648	3651	3653	rBV	446	322	0.00%	0.000%
93	12.869	3676	3679	3683	rBV2	673	565	0.00%	0.000%
94	13.001	3718	3720	3725	rBV2	680	417	0.00%	0.000%
95	13.059	3734	3738	3741	rBV3	975	912	0.00%	0.001%
96	13.146	3761	3765	3766	rBV2	946	681	0.00%	0.001%
97	13.226	3788	3790	3795	rVB2	749	439	0.00%	0.000%
98	13.561	3890	3894	3896	rBV3	725	662	0.00%	0.001%
99	14.345	4135	4138	4144	rBV4	1227	1298	0.00%	0.001%
100	15.165	4390	4393	4397	rBV3	1530	1327	0.00%	0.001%




Sum of corrected areas: 113677874

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021085.D
Acq On : 21 Apr 2021 17:57
Operator : SY/MD
Sample : M2067-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

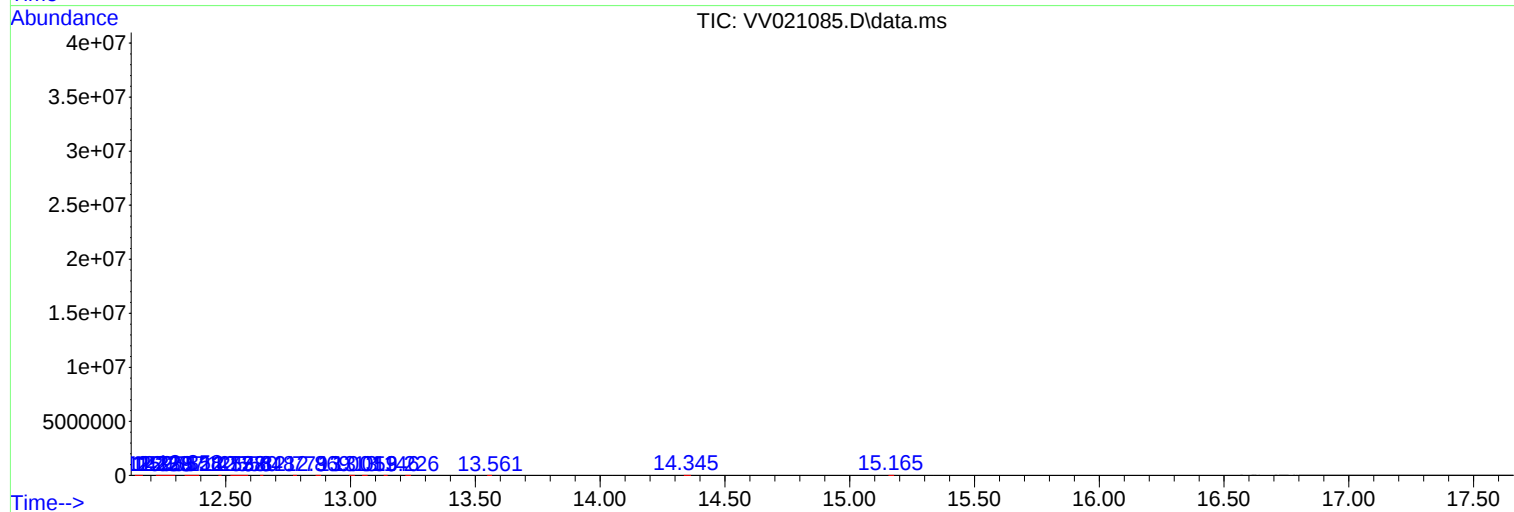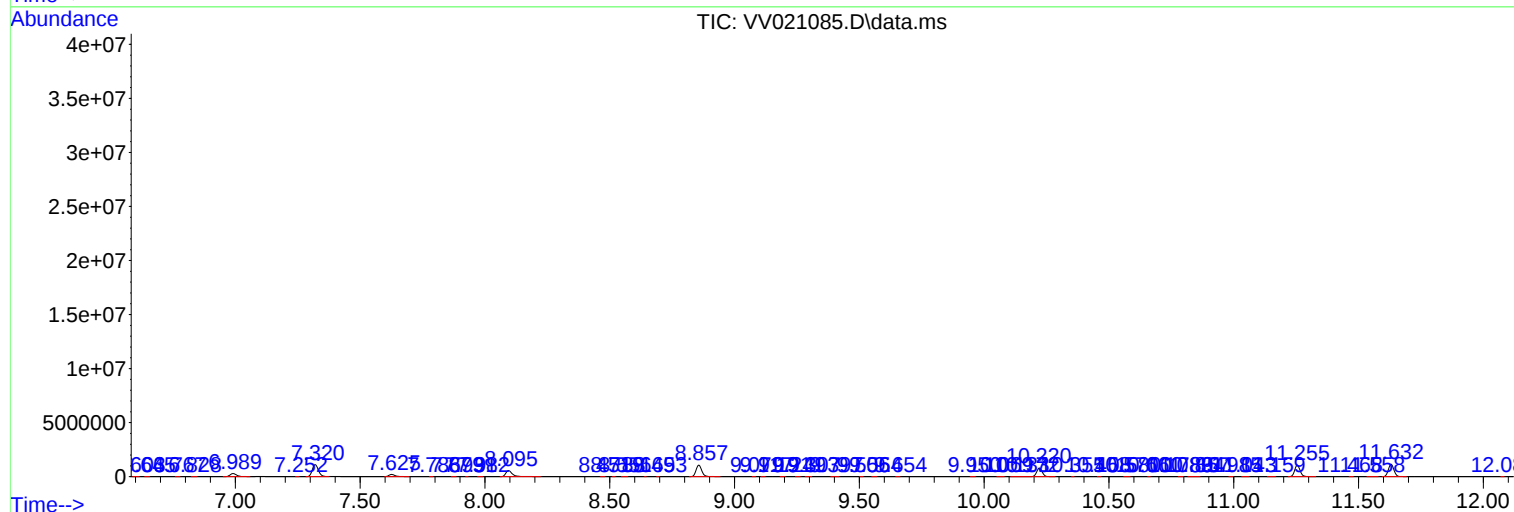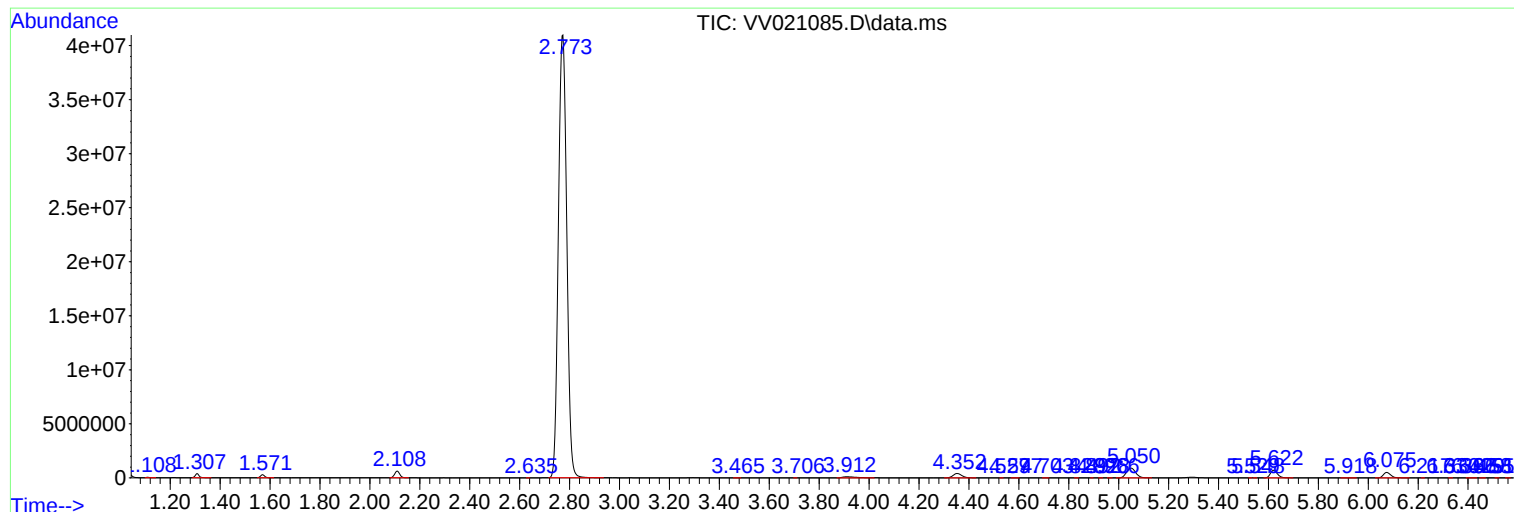

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021085.D
Acq On : 21 Apr 2021 17:57
Operator : SY/MD
Sample : M2067-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021085.D
Acq On : 21 Apr 2021 17:57
Operator : SY/MD
Sample : M2067-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------