
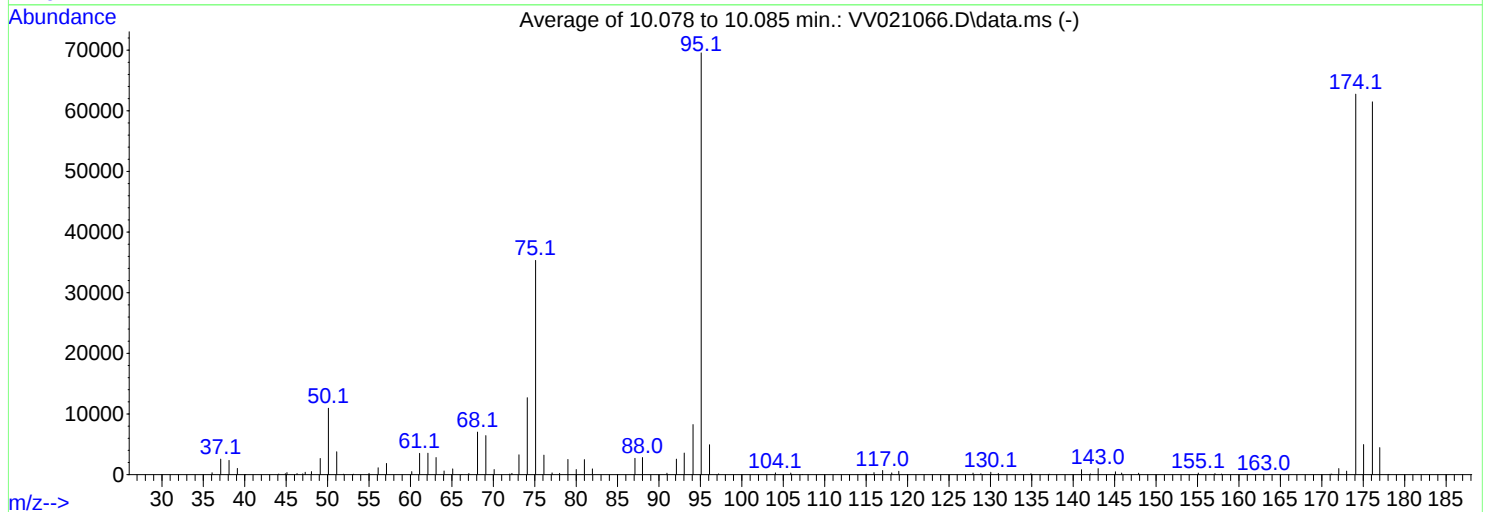


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042121\
Data File : VV021066.D
Acq On : 21 Apr 2021 09:14
Operator : SY/MD
Sample : BFB86
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB186

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Title : VOC Analysis
Last Update : Fri Apr 23 04:33:55 2021

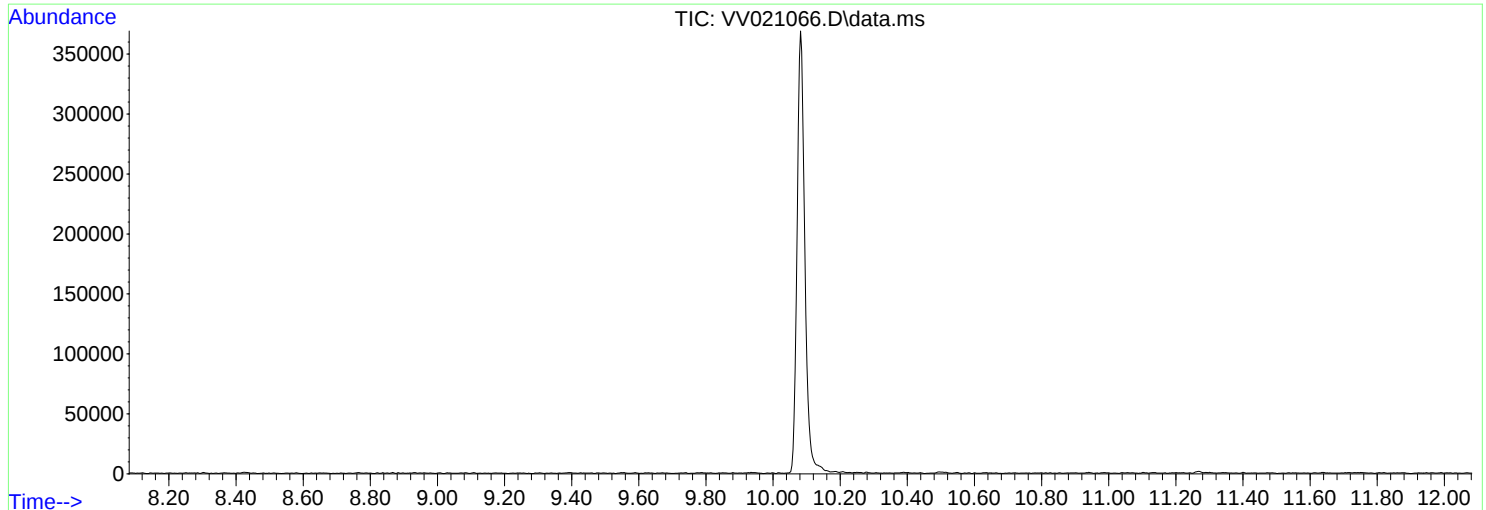

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	10948	PASS
75	95	30	80	50.8	35341	PASS
95	95	100	100	100.0	69555	PASS
96	95	5	9	7.1	4926	PASS
173	174	0.00	2	0.9	572	PASS
174	95	50	120	90.2	62747	PASS
175	174	5	9	7.9	4961	PASS
176	174	95	101	98.0	61488	PASS
177	176	5	9	7.3	4461	PASS

m/z	Abundance
36.10	334.0
37.10	2688.0
38.10	2382.0
39.10	1013.0
40.00	226.0
44.10	669.0
45.10	492.0
46.30	206.0
47.20	427.0
48.10	513.0
49.10	2747.0
50.10	11477.0
51.10	3920.0
53.10	139.0
55.00	244.0
56.10	1244.0
57.10	1883.0
60.20	503.0
61.10	3694.0
62.10	3630.0
63.10	3008.0
64.10	634.0
65.10	979.0
67.00	194.0
68.10	7284.0
69.10	6590.0
70.10	932.0
72.20	296.0
73.10	3325.0
74.10	13173.0
75.10	36728.0
76.10	3344.0
77.10	297.0
78.00	214.0
79.00	2573.0
80.00	904.0
81.00	2550.0
82.00	1006.0
87.10	2788.0
88.00	3008.0
90.90	255.0
92.10	2722.0
93.10	3635.0
94.10	8535.0
95.10	72064.0
96.10	5030.0
97.20	182.0
104.00	296.0
105.90	268.0
115.00	132.0
115.90	341.0
117.00	733.0
118.10	280.0
118.90	575.0
127.90	275.0
128.80	161.0
130.00	388.0
130.90	218.0
134.90	184.0
137.20	105.0
141.00	842.0
142.00	137.0
143.00	975.0
145.10	522.0
145.90	306.0
147.90	256.0
155.10	293.0
157.10	190.0
157.90	133.0
163.00	113.0
171.20	189.0
172.00	1056.0
173.00	888.0
174.10	65168.0
175.10	5096.0
176.10	63808.0
177.00	4608.0

Instrument :
MSVOA_V
ClientSampleId :
BFB186

m/z	Abundance
36.00	311.0
37.10	2516.0
38.10	2528.0
39.10	1042.0
40.00	279.0
44.10	676.0
44.90	459.0
46.30	144.0
47.30	396.0
48.10	421.0
49.10	2785.0
50.10	10864.0
51.10	3628.0
51.90	219.0
53.10	142.0
55.00	187.0
56.10	936.0
57.10	1688.0
60.20	585.0
61.10	3513.0
62.10	3582.0
63.10	2830.0
64.10	611.0
65.10	818.0
67.00	138.0
68.10	7037.0
69.10	6697.0
70.10	695.0
72.30	335.0
73.10	3127.0
74.10	12652.0
75.10	35056.0
76.10	3409.0
77.10	198.0
78.00	135.0
79.00	2238.0
80.00	848.0
81.00	2527.0
82.00	897.0
87.10	2179.0
88.00	2986.0
90.90	259.0
92.10	2420.0
93.00	3690.0
94.10	7930.0
95.10	68648.0
96.10	4694.0
104.00	308.0
105.90	273.0
107.30	107.0
115.00	146.0
115.90	335.0
117.00	649.0
118.10	307.0
119.00	460.0
127.90	240.0
128.80	105.0
130.00	408.0
131.00	202.0
134.90	216.0
141.00	861.0
142.10	119.0
143.00	1107.0
145.10	319.0
145.90	210.0
147.90	136.0
155.10	260.0
157.10	176.0
161.10	113.0
171.00	239.0
172.00	944.0
173.00	829.0
174.10	59608.0
175.00	4727.0
176.10	58272.0
177.00	4423.0

Instrument :
MSVOA_V
ClientSampleId :
BFB186

m/z	Abundance
39.70	116.0
40.10	236.0
44.10	521.0

Instrument :
MSVOA_V
ClientSampleId :
BFB186

m/z	Abundance
36.10	330.0
37.10	2478.0
38.10	2129.0
39.10	1005.0
40.00	207.0
44.10	551.0
45.10	514.0
46.30	192.0
47.00	393.0
47.40	343.0
48.00	546.0
49.10	2485.0
50.10	10503.0
51.10	3784.0
55.00	210.0
56.10	1266.0
57.10	1975.0
60.10	402.0
61.10	3334.0
62.10	3427.0
63.10	2676.0
64.00	560.0
65.10	1043.0
66.20	123.0
67.10	210.0
68.10	6758.0
69.10	6026.0
70.10	935.0
72.00	306.0
73.10	3327.0
74.10	12284.0
75.10	34240.0
76.10	2938.0
77.10	365.0
78.00	269.0
79.00	2717.0
80.00	774.0
81.00	2369.0
81.90	922.0
87.10	3140.0
88.00	2488.0
91.00	236.0
92.10	2541.0
93.10	3373.0
94.10	8332.0
95.10	67952.0
96.10	5053.0
97.20	234.0
104.10	291.0
105.90	277.0
116.00	341.0
117.00	652.0
118.10	264.0
118.90	641.0
127.90	260.0
128.90	186.0
130.10	431.0
130.90	197.0
134.90	112.0
137.00	113.0
141.00	772.0
142.00	180.0
143.00	918.0
145.10	574.0
145.80	278.0
147.90	294.0
155.10	265.0
157.10	166.0
157.90	169.0
171.20	158.0
172.10	1023.0
174.10	63464.0
175.10	5061.0
176.10	62384.0
177.00	4353.0
178.10	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB186