

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030756.D
 Acq On : 21 Apr 2023 11:45
 Operator : SY/MD
 Sample : VV0421WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK330

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	104537	112702	14.11%	1.742%
2	1.539	148	155	170	rVB	98679	119346	14.94%	1.845%
3	2.063	310	318	334	rVB	198960	287000	35.93%	4.437%
4	2.352	406	408	413	rBV5	1168	868	0.11%	0.013%
5	2.388	415	419	421	rBV4	1523	1083	0.14%	0.017%
6	2.420	425	429	433	rBV5	1347	1192	0.15%	0.018%
7	2.449	433	438	439	rBV5	3568	3075	0.38%	0.048%
8	2.609	485	488	490	rBV3	1022	763	0.10%	0.012%
9	2.651	497	501	503	rBV5	1307	1010	0.13%	0.016%
10	2.709	515	519	526	rVB9	1616	1930	0.24%	0.030%
11	2.780	539	541	545	rVB5	1718	826	0.10%	0.013%
12	2.818	549	553	555	rVB5	1278	855	0.11%	0.013%
13	2.844	555	561	562	rBV5	1157	907	0.11%	0.014%
14	3.047	621	624	628	rVB5	1694	1070	0.13%	0.017%
15	3.301	701	703	706	rBV5	1167	691	0.09%	0.011%
16	3.317	706	708	710	rVV3	1709	874	0.11%	0.014%
17	3.416	736	739	742	rBV4	1375	994	0.12%	0.015%
18	3.452	748	750	755	rVB6	1383	1071	0.13%	0.017%
19	3.535	772	776	779	rBV5	1741	1450	0.18%	0.022%
20	3.574	784	788	789	rBV4	1135	723	0.09%	0.011%
21	3.683	819	822	826	rBV6	1098	849	0.11%	0.013%
22	3.738	835	839	842	rVB5	818	653	0.08%	0.010%
23	3.773	847	850	851	rBV3	1524	837	0.10%	0.013%
24	3.809	851	861	887	rBV	44872	142599	17.85%	2.204%
25	4.040	931	933	935	rBV3	1344	645	0.08%	0.010%
26	4.259	985	1001	1019	rBV	128991	330906	41.42%	5.116%
27	4.458	1057	1063	1064	rBV5	1519	1596	0.20%	0.025%
28	4.648	1117	1122	1123	rBV4	1233	970	0.12%	0.015%
29	4.760	1154	1157	1159	rBV4	1501	1027	0.13%	0.016%
30	4.963	1201	1220	1243	rBV3	298985	798838	100.00%	12.350%
31	5.471	1376	1378	1381	rBV3	1340	780	0.10%	0.012%
32	5.542	1387	1400	1423	rBV	287876	600093	75.12%	9.277%
33	5.995	1529	1541	1559	rBV	172373	361846	45.30%	5.594%
34	6.204	1603	1606	1610	rVB5	1803	1015	0.13%	0.016%
35	6.223	1610	1612	1614	rBV2	1458	844	0.11%	0.013%
36	6.403	1664	1668	1670	rBV4	1385	1202	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030756.D
 Acq On : 21 Apr 2023 11:45
 Operator : SY/MD
 Sample : VV0421WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK330

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.416	1670	1672	1677	rVB5	1944	1107	0.14%	0.017%
38	6.921	1817	1829	1847	rBV	93121	179562	22.48%	2.776%
39	7.079	1876	1878	1883	rVB6	1465	1059	0.13%	0.016%
40	7.104	1883	1886	1890	rBV5	2190	1818	0.23%	0.028%
41	7.249	1919	1931	1947	rBV	334301	596821	74.71%	9.227%
42	7.561	2019	2028	2043	rBV2	66008	118898	14.88%	1.838%
43	7.702	2068	2072	2075	rBV5	1290	1143	0.14%	0.018%
44	7.735	2079	2082	2084	rBV4	1112	790	0.10%	0.012%
45	7.992	2157	2162	2164	rBV6	1527	1278	0.16%	0.020%
46	8.034	2166	2175	2191	rBV	149892	291343	36.47%	4.504%
47	8.551	2332	2336	2339	rBV6	1933	1493	0.19%	0.023%
48	8.571	2340	2342	2347	rVB6	1469	1025	0.13%	0.016%
49	8.738	2390	2394	2397	rBV5	1179	1141	0.14%	0.018%
50	8.792	2400	2411	2433	rVV	442003	738952	92.50%	11.424%
51	9.066	2494	2496	2498	rBV3	1315	734	0.09%	0.011%
52	9.198	2534	2537	2539	rBV3	1143	918	0.11%	0.014%
53	9.217	2542	2543	2547	rVV4	976	700	0.09%	0.011%
54	9.252	2551	2554	2556	rBV4	1749	1043	0.13%	0.016%
55	9.548	2643	2646	2648	rVB4	1849	637	0.08%	0.010%
56	9.571	2651	2653	2656	rVB4	1361	652	0.08%	0.010%
57	9.583	2656	2657	2662	rBV5	884	687	0.09%	0.011%
58	9.686	2686	2689	2693	rBV5	1651	1324	0.17%	0.020%
59	9.712	2693	2697	2698	rBV3	1040	666	0.08%	0.010%
60	9.802	2722	2725	2729	rBV5	1054	829	0.10%	0.013%
61	10.008	2784	2789	2791	rBV6	1976	1685	0.21%	0.026%
62	10.159	2821	2836	2854	rBV	238384	383618	48.02%	5.931%
63	10.268	2868	2870	2873	rVB4	1636	825	0.10%	0.013%
64	10.513	2944	2946	2949	rVB4	1107	664	0.08%	0.010%
65	10.535	2949	2953	2955	rBV4	1042	778	0.10%	0.012%
66	10.612	2973	2977	2981	rBV5	1679	1478	0.19%	0.023%
67	10.632	2981	2983	2986	rBV5	1168	786	0.10%	0.012%
68	10.786	3025	3031	3032	rBV5	1809	1612	0.20%	0.025%
69	10.841	3044	3048	3049	rBV3	1145	881	0.11%	0.014%
70	10.902	3064	3067	3070	rBV5	1431	1022	0.13%	0.016%
71	10.979	3088	3091	3097	rVB7	1840	1424	0.18%	0.022%
72	11.030	3103	3107	3110	rBV6	1165	1163	0.15%	0.018%
73	11.053	3112	3114	3117	rVB3	1248	685	0.09%	0.011%
74	11.194	3145	3158	3176	rBV	430548	712492	89.19%	11.015%
75	11.400	3219	3222	3226	rBV6	1422	1435	0.18%	0.022%
76	11.516	3256	3258	3260	rVV3	1895	704	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030756.D
 Acq On : 21 Apr 2023 11:45
 Operator : SY/MD
 Sample : VV0421WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK330

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.567	3262	3274	3292	rVV	362180	594473	74.42%	9.190%
78	11.760	3332	3334	3337	rBV3	971	675	0.08%	0.010%
79	12.140	3449	3452	3456	rVB6	1152	762	0.10%	0.012%
80	12.165	3456	3460	3463	rBV5	1652	1176	0.15%	0.018%
81	12.181	3463	3465	3469	rVB5	882	670	0.08%	0.010%
82	12.320	3505	3508	3510	rBV4	814	732	0.09%	0.011%
83	12.429	3539	3542	3545	rVB3	1452	853	0.11%	0.013%
84	12.451	3546	3549	3550	rBV3	1331	631	0.08%	0.010%
85	12.596	3587	3594	3601	rBV3	3798	5038	0.63%	0.078%
86	12.760	3642	3645	3649	rBV6	1411	1056	0.13%	0.016%
87	12.985	3711	3715	3720	rBV7	1261	1300	0.16%	0.020%
88	13.210	3776	3785	3793	rBV7	7305	11322	1.42%	0.175%
89	13.352	3827	3829	3831	rBV3	1381	758	0.09%	0.012%
90	13.513	3878	3879	3883	rVB4	1707	638	0.08%	0.010%
91	13.564	3893	3895	3897	rBV3	1180	622	0.08%	0.010%
92	13.648	3917	3921	3923	rBV5	1324	1098	0.14%	0.017%
93	13.840	3976	3981	3983	rBV6	1165	998	0.12%	0.015%
94	13.972	4020	4022	4026	rVB4	1621	1061	0.13%	0.016%
95	14.014	4033	4035	4040	rBV6	1433	1210	0.15%	0.019%
96	14.085	4054	4057	4060	rBV5	1446	824	0.10%	0.013%
97	14.101	4060	4062	4065	rBV3	1273	997	0.12%	0.015%
98	14.291	4118	4121	4122	rBV3	1467	717	0.09%	0.011%
99	14.332	4131	4134	4136	rBV3	1925	1139	0.14%	0.018%
100	15.040	4352	4354	4355	rBV2	1824	799	0.10%	0.012%




Sum of corrected areas: 6468551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030756.D
Acq On : 21 Apr 2023 11:45
Operator : SY/MD
Sample : VV0421WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

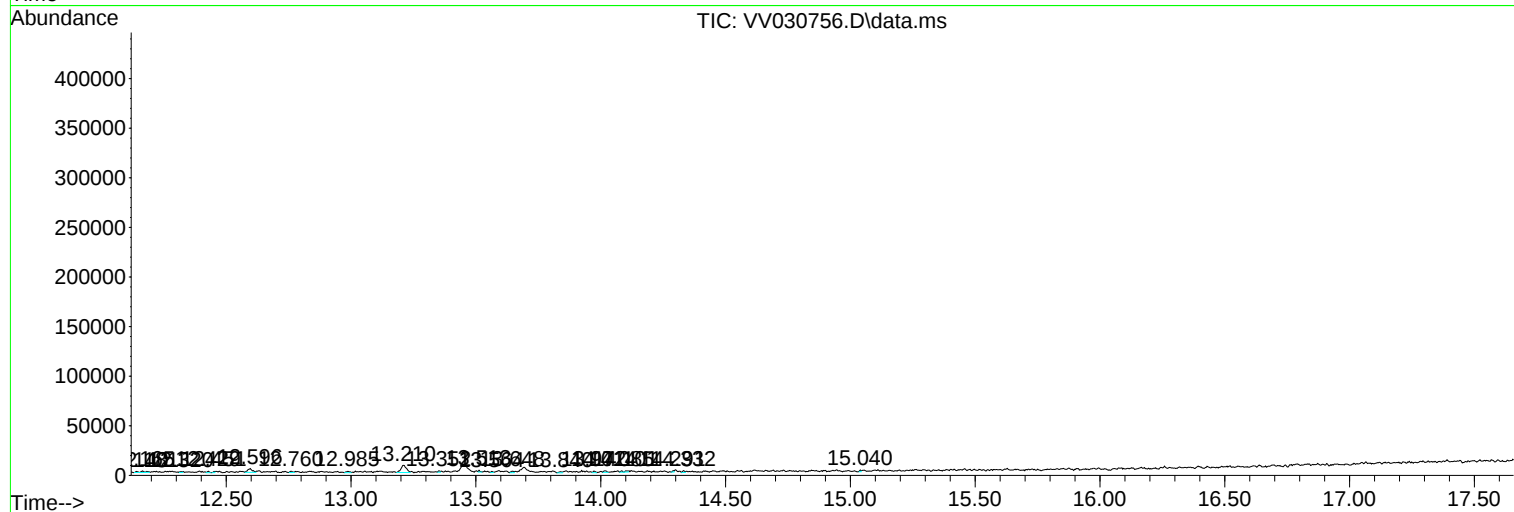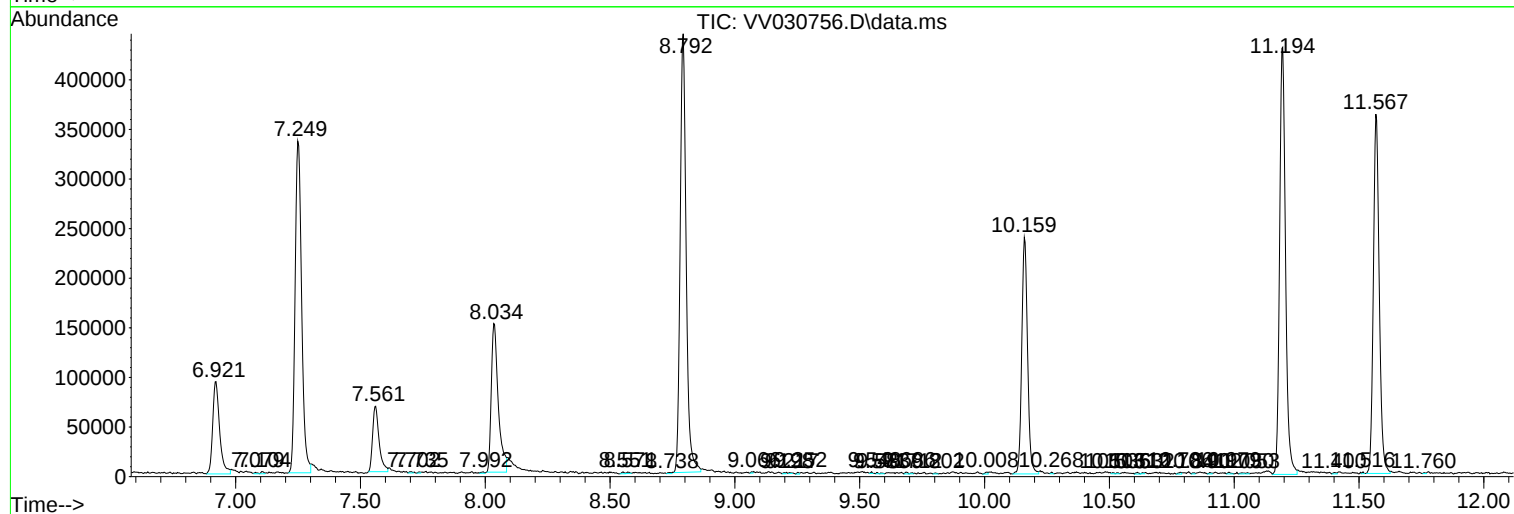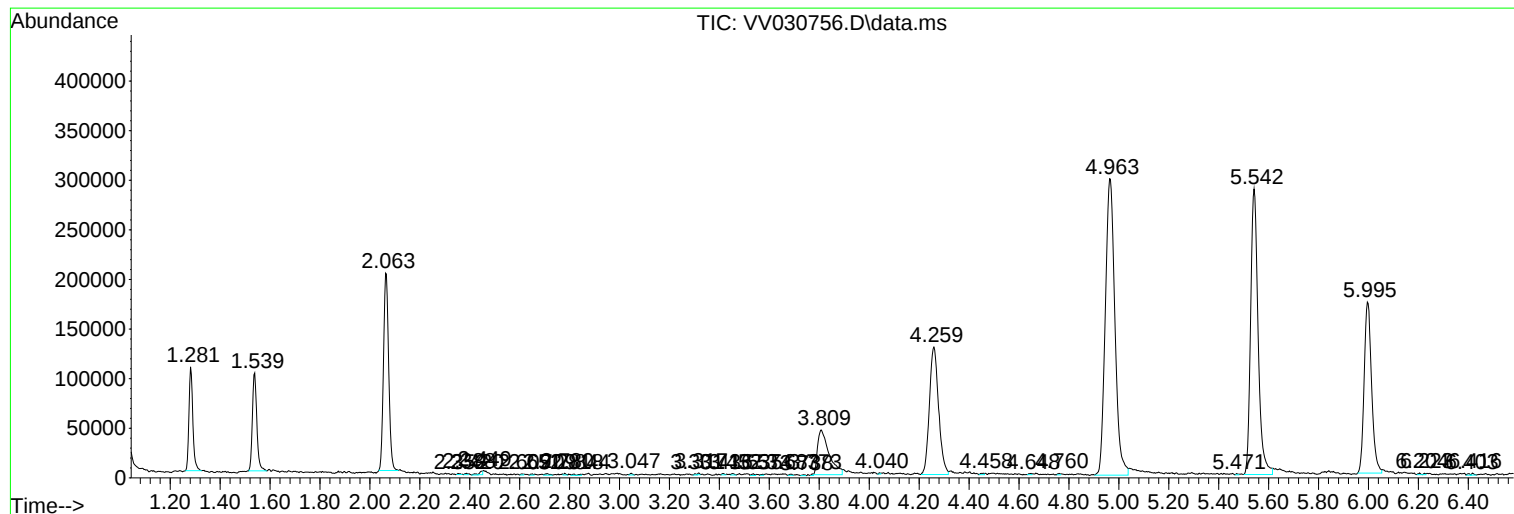

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030756.D
Acq On : 21 Apr 2023 11:45
Operator : SY/MD
Sample : VV0421WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030756.D
Acq On : 21 Apr 2023 11:45
Operator : SY/MD
Sample : VV0421WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK330

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------