

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030759.D
 Acq On : 21 Apr 2023 12:55
 Operator : SY/MD
 Sample : 02398-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	114825	126045	13.94%	1.718%
2	1.539	148	155	166	rBV	115512	132712	14.68%	1.809%
3	2.066	310	319	336	rBV	228316	334854	37.04%	4.564%
4	2.314	393	396	400	rBV5	899	750	0.08%	0.010%
5	2.629	489	494	497	rVB6	1509	1288	0.14%	0.018%
6	2.645	497	499	501	rBV3	961	488	0.05%	0.007%
7	2.892	573	576	583	rBV8	1369	1334	0.15%	0.018%
8	2.989	602	606	607	rBV3	1720	1026	0.11%	0.014%
9	3.085	634	636	640	rVB4	1271	599	0.07%	0.008%
10	3.133	649	651	652	rBV2	1008	511	0.06%	0.007%
11	3.153	655	657	664	rVB7	1450	1193	0.13%	0.016%
12	3.252	686	688	690	rBV3	1355	686	0.08%	0.009%
13	3.365	720	723	725	rBV4	1258	660	0.07%	0.009%
14	3.487	757	761	764	rBV6	1123	1093	0.12%	0.015%
15	3.561	780	784	785	rBV4	1373	830	0.09%	0.011%
16	3.593	791	794	797	rVB5	815	557	0.06%	0.008%
17	3.703	826	828	830	rBV2	1015	532	0.06%	0.007%
18	3.805	848	860	881	rBV2	58580	175459	19.41%	2.392%
19	4.259	988	1001	1025	rVB	147023	366922	40.59%	5.001%
20	4.658	1122	1125	1129	rBV5	1688	1438	0.16%	0.020%
21	4.831	1177	1179	1183	rVB4	1570	1040	0.12%	0.014%
22	4.854	1183	1186	1188	rBV5	1299	770	0.09%	0.010%
23	4.879	1188	1194	1197	rBV7	1343	1385	0.15%	0.019%
24	4.966	1206	1221	1253	rBV2	342903	903988	100.00%	12.322%
25	5.542	1388	1400	1422	rBV	319650	658116	72.80%	8.971%
26	5.767	1467	1470	1471	rBV3	1615	881	0.10%	0.012%
27	5.912	1513	1515	1517	rVB3	1693	511	0.06%	0.007%
28	5.998	1530	1542	1566	rVB	203518	410882	45.45%	5.601%
29	6.227	1610	1613	1614	rBV3	1007	588	0.07%	0.008%
30	6.567	1715	1719	1720	rBV4	1959	1181	0.13%	0.016%
31	6.735	1768	1771	1778	rVB6	1697	1468	0.16%	0.020%
32	6.792	1786	1789	1792	rBV4	1103	868	0.10%	0.012%
33	6.866	1809	1812	1814	rVV3	1517	878	0.10%	0.012%
34	6.921	1817	1829	1844	rBV2	105823	201117	22.25%	2.741%
35	7.117	1887	1890	1892	rBV3	1970	1183	0.13%	0.016%
36	7.165	1902	1905	1910	rVB6	1691	1476	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030759.D
 Acq On : 21 Apr 2023 12:55
 Operator : SY/MD
 Sample : 02398-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.191	1910	1913	1916	rBV5	1206	831	0.09%	0.011%
38	7.252	1920	1932	1952	rBV	393078	690977	76.44%	9.419%
39	7.558	2018	2027	2050	rBV	77640	149137	16.50%	2.033%
40	7.802	2099	2103	2107	rBV7	1405	1415	0.16%	0.019%
41	7.956	2147	2151	2152	rBV3	1381	961	0.11%	0.013%
42	7.966	2152	2154	2158	rVB4	1521	859	0.10%	0.012%
43	8.034	2165	2175	2209	rBV	200280	425388	47.06%	5.798%
44	8.310	2260	2261	2263	rBV2	1439	676	0.07%	0.009%
45	8.493	2316	2318	2319	rBV2	1455	646	0.07%	0.009%
46	8.792	2400	2411	2434	rBV	488432	813907	90.04%	11.094%
47	9.059	2492	2494	2496	rBV3	1470	990	0.11%	0.013%
48	9.111	2508	2510	2513	rBV3	1155	630	0.07%	0.009%
49	9.165	2526	2527	2530	rBV3	1106	598	0.07%	0.008%
50	9.445	2610	2614	2615	rVV2	1007	676	0.07%	0.009%
51	9.561	2648	2650	2652	rBV3	902	534	0.06%	0.007%
52	9.644	2673	2676	2678	rBV4	1718	1152	0.13%	0.016%
53	9.683	2686	2688	2692	rBV5	1099	578	0.06%	0.008%
54	9.728	2699	2702	2703	rBV3	827	525	0.06%	0.007%
55	9.805	2724	2726	2729	rBV3	1761	1034	0.11%	0.014%
56	10.088	2812	2814	2815	rBV2	1474	644	0.07%	0.009%
57	10.159	2825	2836	2855	rBV	281710	448519	49.62%	6.114%
58	10.271	2869	2871	2872	rBV	1679	562	0.06%	0.008%
59	10.320	2885	2886	2889	rVB3	1695	573	0.06%	0.008%
60	10.413	2914	2915	2917	rBV2	930	474	0.05%	0.006%
61	10.522	2947	2949	2951	rBV3	1337	694	0.08%	0.009%
62	10.696	3000	3003	3005	rBV3	1607	1006	0.11%	0.014%
63	10.734	3012	3015	3020	rBV6	1598	1437	0.16%	0.020%
64	11.056	3113	3115	3118	rBV4	1288	889	0.10%	0.012%
65	11.191	3147	3157	3174	rBV	463665	750526	83.02%	10.230%
66	11.461	3239	3241	3242	rBV2	1321	520	0.06%	0.007%
67	11.567	3262	3274	3295	rVV	396764	665722	73.64%	9.074%
68	11.869	3367	3368	3370	rBV2	1570	655	0.07%	0.009%
69	11.972	3398	3400	3402	rVB3	1757	691	0.08%	0.009%
70	12.021	3412	3415	3419	rBV5	1887	1412	0.16%	0.019%
71	12.091	3435	3437	3439	rBV3	1289	566	0.06%	0.008%
72	12.194	3466	3469	3474	rBV7	1375	1214	0.13%	0.017%
73	12.255	3486	3488	3491	rVB4	1701	624	0.07%	0.009%
74	12.355	3517	3519	3521	rBV3	1117	588	0.07%	0.008%
75	12.397	3527	3532	3534	rBV5	1900	1500	0.17%	0.020%
76	12.429	3540	3542	3545	rBV3	1668	950	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030759.D
 Acq On : 21 Apr 2023 12:55
 Operator : SY/MD
 Sample : 02398-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.596	3586	3594	3597	rBV6	2584	3286	0.36%	0.045%
78	12.866	3671	3678	3679	rBV7	2115	1508	0.17%	0.021%
79	12.940	3698	3701	3703	rBV4	774	507	0.06%	0.007%
80	12.956	3703	3706	3709	rBV4	1417	1217	0.13%	0.017%
81	12.998	3717	3719	3720	rBV2	1059	503	0.06%	0.007%
82	13.033	3728	3730	3732	rBV2	1120	626	0.07%	0.009%
83	13.091	3745	3748	3749	rBV4	1176	645	0.07%	0.009%
84	13.127	3756	3759	3761	rBV3	916	680	0.08%	0.009%
85	13.207	3777	3784	3789	rBV9	4003	5966	0.66%	0.081%
86	13.303	3810	3814	3815	rBV3	1266	902	0.10%	0.012%
87	13.339	3823	3825	3828	rVB4	1852	857	0.09%	0.012%
88	13.410	3845	3847	3851	rVB5	1482	737	0.08%	0.010%
89	13.429	3851	3853	3856	rBV4	1103	607	0.07%	0.008%
90	13.451	3856	3860	3861	rBV3	1577	949	0.10%	0.013%
91	13.529	3880	3884	3886	rBV4	1644	1361	0.15%	0.019%
92	13.593	3900	3904	3909	rBV8	2280	2620	0.29%	0.036%
93	13.664	3924	3926	3927	rBV2	1086	569	0.06%	0.008%
94	13.760	3949	3956	3959	rBV8	1960	1901	0.21%	0.026%
95	13.998	4026	4030	4031	rBV4	1201	590	0.07%	0.008%
96	14.265	4110	4113	4115	rBV4	1221	633	0.07%	0.009%
97	14.275	4115	4116	4120	rVV4	1323	689	0.08%	0.009%
98	14.297	4120	4123	4126	rBV5	1741	1141	0.13%	0.016%
99	14.516	4189	4191	4193	rBV3	1402	511	0.06%	0.007%
100	14.586	4210	4213	4214	rBV2	1082	672	0.07%	0.009%




Sum of corrected areas: 7336266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030759.D
Acq On : 21 Apr 2023 12:55
Operator : SY/MD
Sample : 02398-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

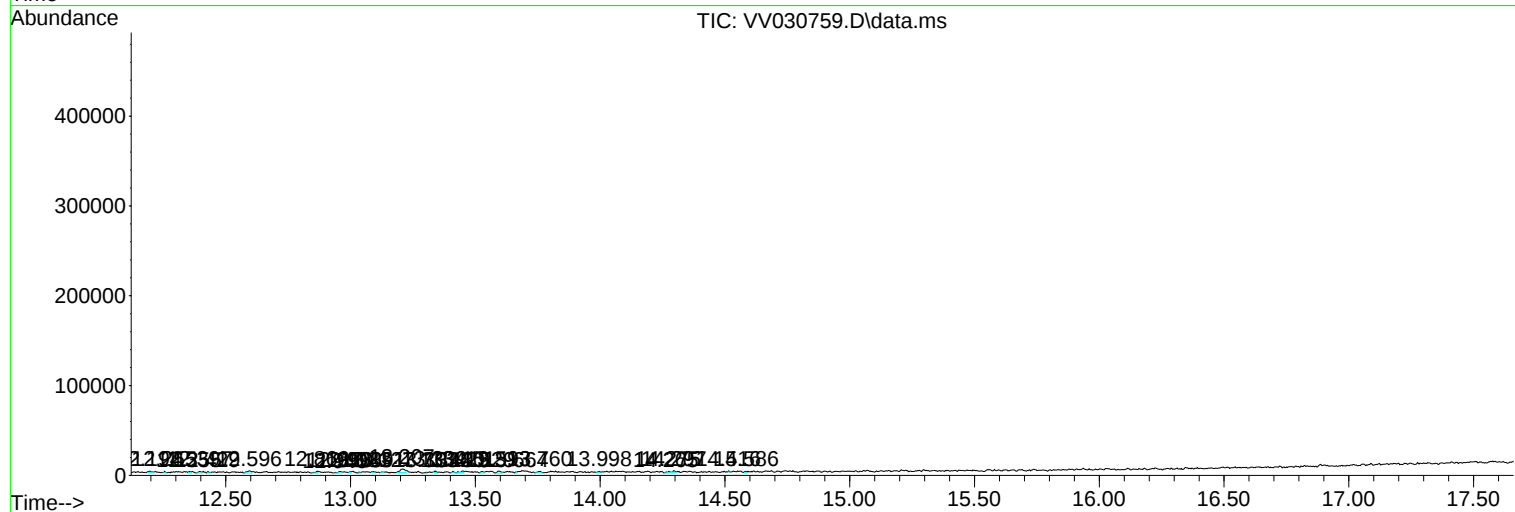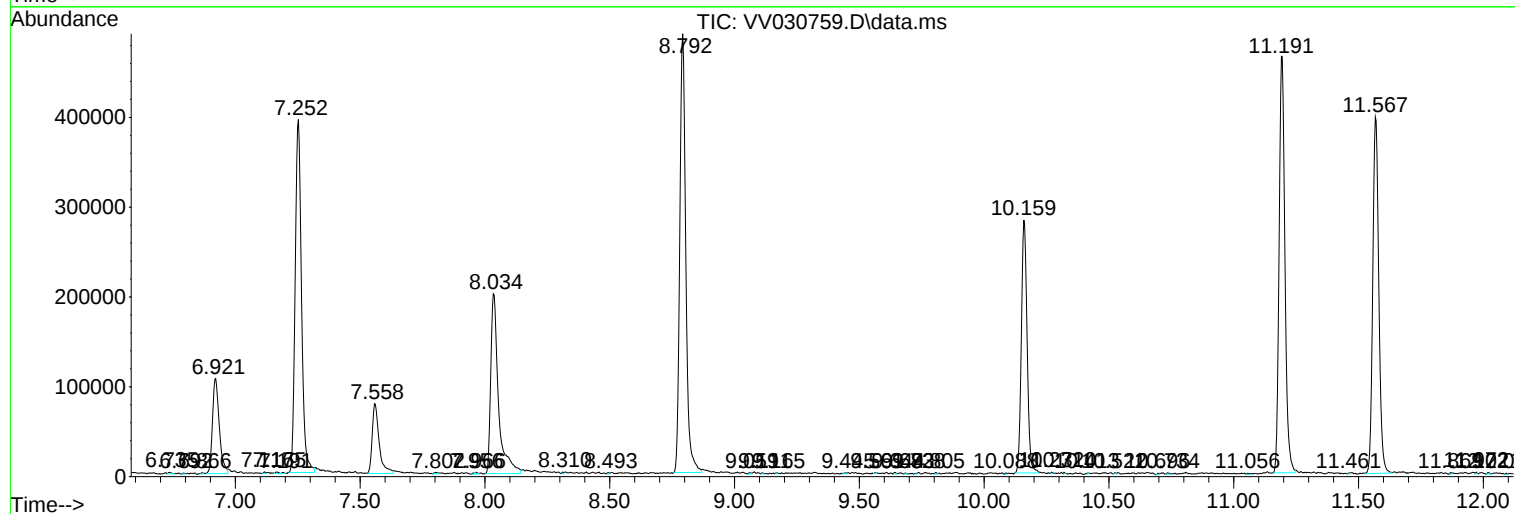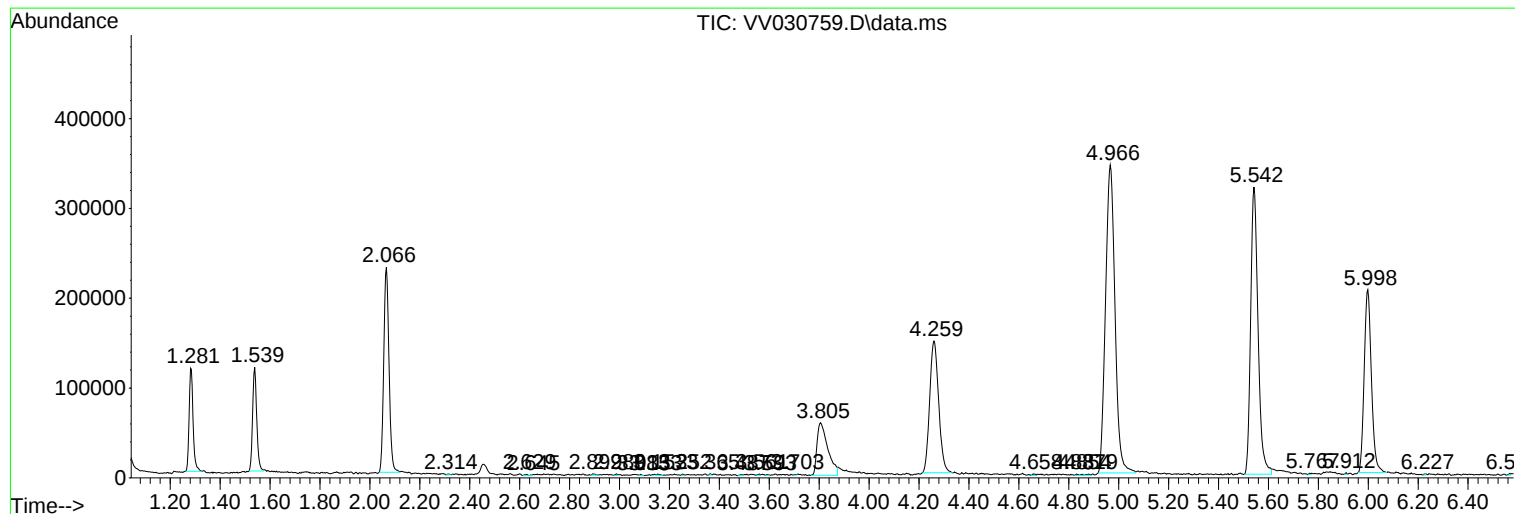

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030759.D
Acq On : 21 Apr 2023 12:55
Operator : SY/MD
Sample : 02398-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030759.D
Acq On : 21 Apr 2023 12:55
Operator : SY/MD
Sample : 02398-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc