

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030761.D
 Acq On : 21 Apr 2023 13:43
 Operator : SY/MD
 Sample : 02398-11DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	107228	119256	1.79%	0.739%
2	1.539	148	155	167	rVB	104696	121825	1.82%	0.755%
3	1.876	257	260	263	rBV4	2049	1412	0.02%	0.009%
4	2.066	309	319	336	rBV	211032	310559	4.65%	1.924%
5	2.317	394	397	398	rBV3	1331	597	0.01%	0.004%
6	2.343	403	405	409	rVB6	1485	990	0.01%	0.006%
7	2.413	423	427	429	rBV5	1532	1174	0.02%	0.007%
8	2.687	509	512	513	rVB3	1026	536	0.01%	0.003%
9	2.706	513	518	519	rBV4	1806	1471	0.02%	0.009%
10	2.880	567	572	578	rVB9	1322	1767	0.03%	0.011%
11	2.909	578	581	583	rBV5	707	585	0.01%	0.004%
12	2.957	592	596	597	rBV3	1074	754	0.01%	0.005%
13	3.018	613	615	618	rVB5	1490	591	0.01%	0.004%
14	3.137	649	652	653	rBV2	1412	700	0.01%	0.004%
15	3.426	739	742	746	rBV5	1958	1469	0.02%	0.009%
16	3.609	794	799	801	rBV6	950	847	0.01%	0.005%
17	3.667	814	817	820	rBV4	1585	1106	0.02%	0.007%
18	3.806	851	860	891	rBV	53108	161364	2.42%	1.000%
19	4.015	923	925	928	rBV4	1368	799	0.01%	0.005%
20	4.053	935	937	939	rBV3	1503	644	0.01%	0.004%
21	4.259	989	1001	1024	rVB	133600	340927	5.11%	2.112%
22	4.497	1072	1075	1076	rBV3	1033	647	0.01%	0.004%
23	4.561	1093	1095	1100	rVB6	1385	795	0.01%	0.005%
24	4.587	1101	1103	1105	rBV3	1952	1000	0.01%	0.006%
25	4.667	1126	1128	1130	rVB3	1221	506	0.01%	0.003%
26	4.709	1138	1141	1146	rBV7	1542	1192	0.02%	0.007%
27	4.902	1199	1201	1204	rBV4	897	653	0.01%	0.004%
28	4.966	1204	1221	1227	rBV2	319789	756087	11.33%	4.684%
29	5.542	1388	1400	1418	rBV	316647	643706	9.64%	3.988%
30	5.998	1530	1542	1565	rBV	182498	377206	5.65%	2.337%
31	6.304	1635	1637	1641	rVB5	1583	1081	0.02%	0.007%
32	6.410	1668	1670	1676	rVB7	1662	1126	0.02%	0.007%
33	6.738	1770	1772	1774	rBV3	917	517	0.01%	0.003%
34	6.767	1779	1781	1784	rBV4	1788	1243	0.02%	0.008%
35	6.834	1798	1802	1803	rBV3	1379	826	0.01%	0.005%
36	6.921	1818	1829	1844	rBV	97519	184886	2.77%	1.145%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030761.D
 Acq On : 21 Apr 2023 13:43
 Operator : SY/MD
 Sample : 02398-11DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1918	1932	1949	rBV	358266	638215	9.56%	3.954%
38	7.561	2019	2028	2048	rBV	68509	125527	1.88%	0.778%
39	7.886	2126	2129	2130	rBV3	1282	711	0.01%	0.004%
40	7.924	2139	2141	2146	rVB5	1289	751	0.01%	0.005%
41	8.034	2166	2175	2204	rBV	185465	370314	5.55%	2.294%
42	8.452	2302	2305	2307	rBV4	1002	619	0.01%	0.004%
43	8.510	2320	2323	2327	rBV6	2090	1751	0.03%	0.011%
44	8.821	2399	2420	2463	rBV2	3681570	6675565	100.00%	41.355%
45	9.153	2521	2523	2524	rBV	1357	581	0.01%	0.004%
46	9.355	2582	2586	2590	rBV6	1447	1411	0.02%	0.009%
47	9.416	2603	2605	2611	rBV6	1275	954	0.01%	0.006%
48	9.590	2657	2659	2663	rBV5	1146	755	0.01%	0.005%
49	9.760	2709	2712	2715	rVV5	1029	606	0.01%	0.004%
50	9.789	2718	2721	2726	rBV7	1135	750	0.01%	0.005%
51	9.937	2765	2767	2769	rBV3	1038	542	0.01%	0.003%
52	9.989	2780	2783	2785	rVB3	1475	833	0.01%	0.005%
53	10.159	2826	2836	2852	rBV	252698	401496	6.01%	2.487%
54	10.252	2861	2865	2867	rBV4	1026	816	0.01%	0.005%
55	10.413	2913	2915	2917	rBV4	1613	849	0.01%	0.005%
56	10.423	2917	2918	2921	rVB3	2107	736	0.01%	0.005%
57	10.493	2936	2940	2943	rBV6	1937	1727	0.03%	0.011%
58	10.564	2960	2962	2965	rBV4	829	575	0.01%	0.004%
59	10.715	3005	3009	3013	rBV6	2142	1667	0.02%	0.010%
60	10.866	3054	3056	3058	rBV3	1056	614	0.01%	0.004%
61	10.995	3092	3096	3098	rBV5	2279	1747	0.03%	0.011%
62	11.018	3101	3103	3105	rVB3	1524	678	0.01%	0.004%
63	11.053	3111	3114	3117	rVB5	999	600	0.01%	0.004%
64	11.127	3127	3137	3146	rBV2	43983	70546	1.06%	0.437%
65	11.217	3147	3165	3182	rVV2	1103773	2394790	35.87%	14.836%
66	11.471	3242	3244	3246	rBV3	1414	705	0.01%	0.004%
67	11.493	3249	3251	3255	rBV4	1257	805	0.01%	0.005%
68	11.583	3262	3279	3295	rBV2	1151678	2302764	34.50%	14.266%
69	11.802	3346	3347	3350	rVB3	2433	967	0.01%	0.006%
70	11.821	3350	3353	3357	rBV5	2181	1904	0.03%	0.012%
71	11.982	3399	3403	3406	rVB5	1715	1386	0.02%	0.009%
72	12.050	3422	3424	3429	rVB6	1418	752	0.01%	0.005%
73	12.085	3433	3435	3438	rBV5	1317	807	0.01%	0.005%
74	12.310	3501	3505	3507	rBV5	1298	1091	0.02%	0.007%
75	12.548	3577	3579	3583	rVB5	1464	841	0.01%	0.005%
76	12.596	3589	3594	3596	rBV6	1652	1363	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030761.D
 Acq On : 21 Apr 2023 13:43
 Operator : SY/MD
 Sample : 02398-11DL 250X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.722	3631	3633	3636	rVB4	1296	514	0.01%	0.003%
78	12.754	3638	3643	3645	rBV5	1136	969	0.01%	0.006%
79	12.805	3656	3659	3662	rVV5	1373	1042	0.02%	0.006%
80	12.825	3662	3665	3668	rVB5	1015	802	0.01%	0.005%
81	12.898	3686	3688	3691	rVB3	1062	569	0.01%	0.004%
82	13.053	3734	3736	3737	rBV2	1327	647	0.01%	0.004%
83	13.098	3744	3750	3751	rBV5	1429	1010	0.02%	0.006%
84	13.165	3769	3771	3773	rVV3	1359	590	0.01%	0.004%
85	13.207	3776	3784	3794	rVB2	34303	55524	0.83%	0.344%
86	13.291	3807	3810	3812	rBV3	1684	834	0.01%	0.005%
87	13.349	3826	3828	3834	rBV7	803	765	0.01%	0.005%
88	13.378	3834	3837	3839	rBV5	1325	750	0.01%	0.005%
89	13.603	3901	3907	3911	rBV8	1509	2087	0.03%	0.013%
90	13.644	3918	3920	3921	rBV2	1623	676	0.01%	0.004%
91	13.689	3929	3934	3944	rVB7	10546	16185	0.24%	0.100%
92	13.963	4017	4019	4021	rBV4	1121	662	0.01%	0.004%
93	14.053	4045	4047	4050	rBV3	1444	860	0.01%	0.005%
94	14.124	4065	4069	4075	rVB9	2127	2166	0.03%	0.013%
95	14.156	4075	4079	4080	rBV4	1090	811	0.01%	0.005%
96	14.342	4135	4137	4138	rBV2	1401	535	0.01%	0.003%
97	14.448	4166	4170	4172	rBV5	1256	935	0.01%	0.006%
98	14.538	4196	4198	4201	rBV4	1646	749	0.01%	0.005%
99	14.654	4231	4234	4235	rBV3	1513	781	0.01%	0.005%
100	14.879	4302	4304	4306	rBV3	1578	597	0.01%	0.004%




Sum of corrected areas: 16142015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030761.D
Acq On : 21 Apr 2023 13:43
Operator : SY/MD
Sample : 02398-11DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

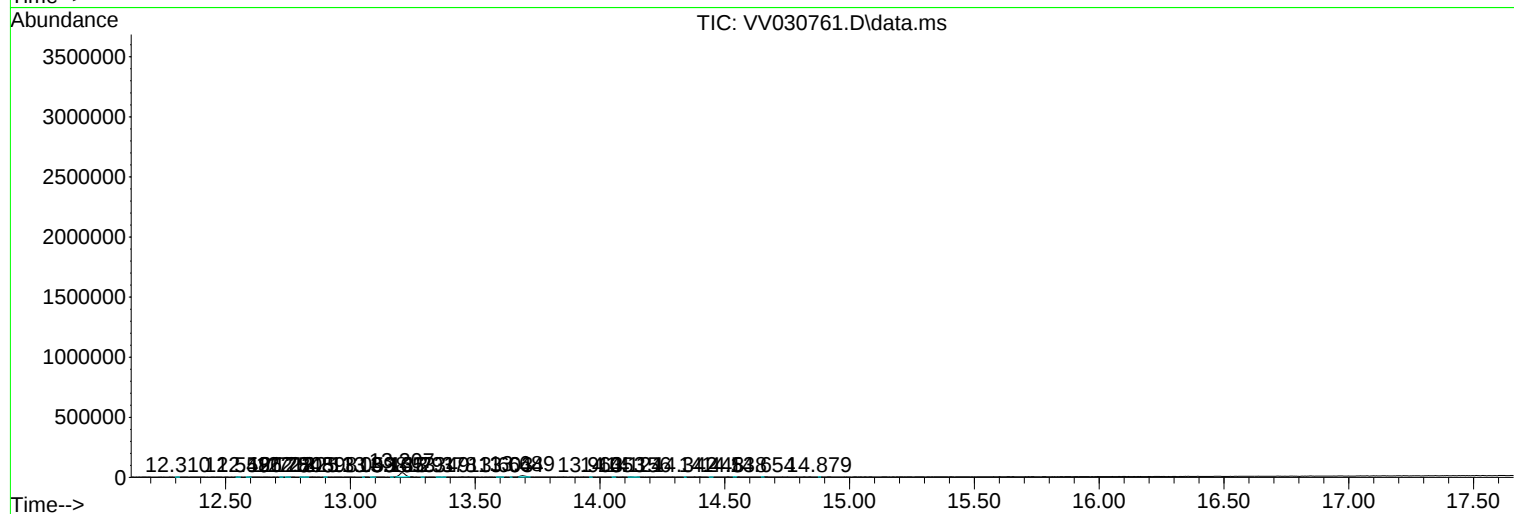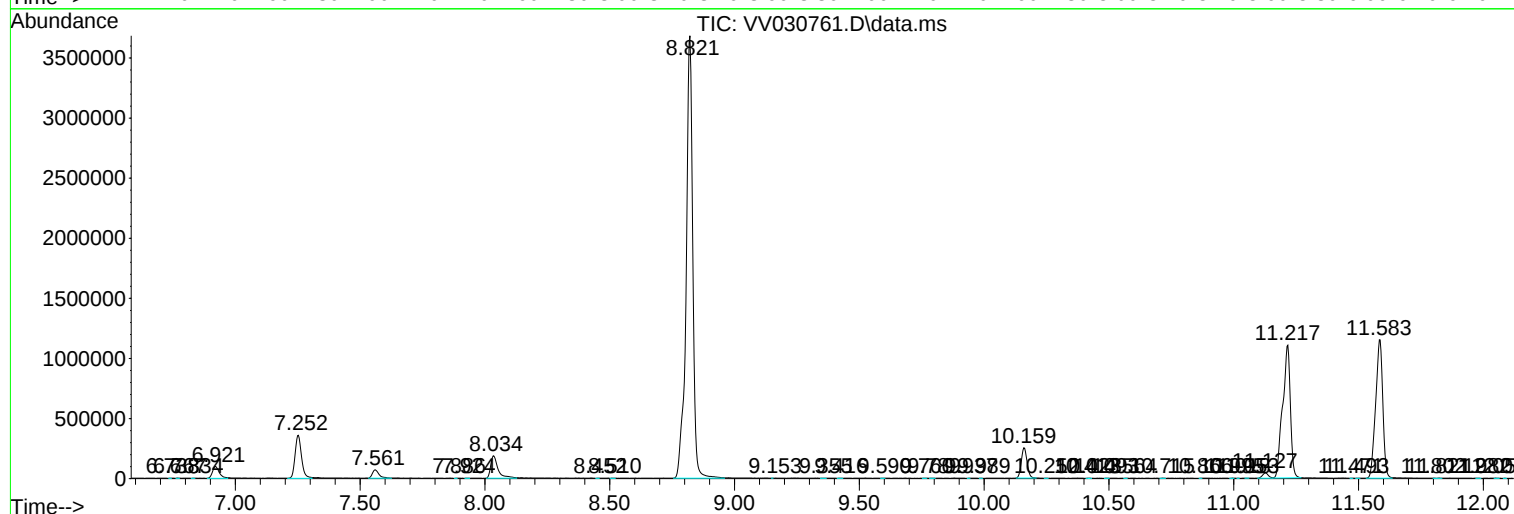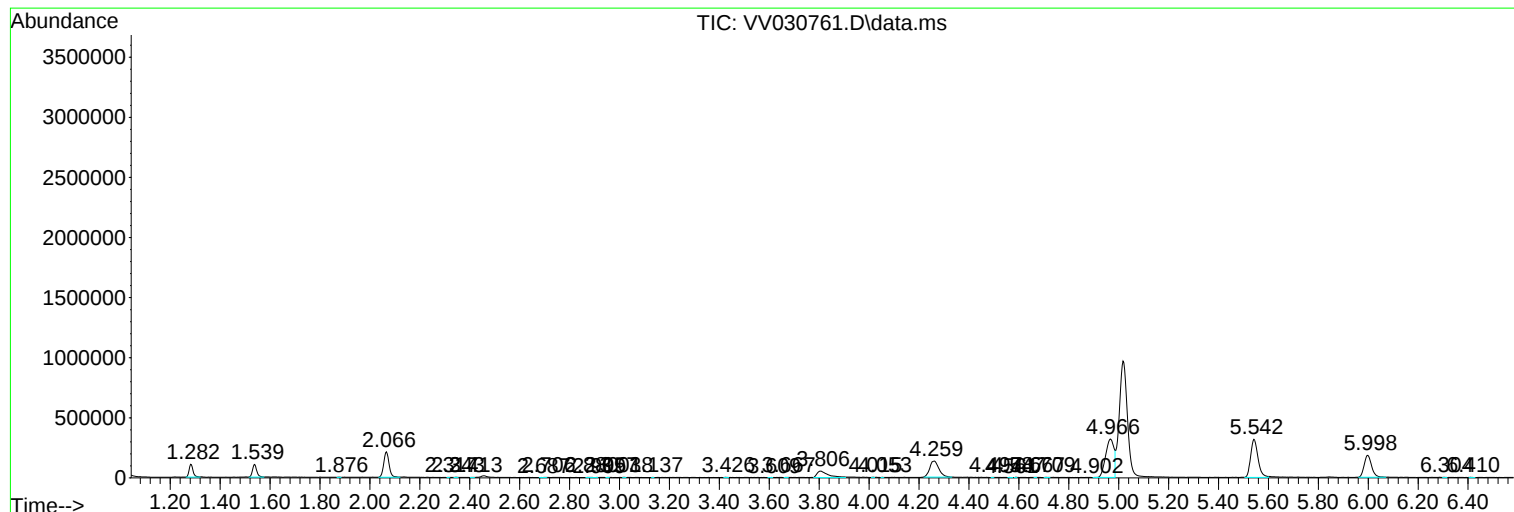

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030761.D
Acq On : 21 Apr 2023 13:43
Operator : SY/MD
Sample : 02398-11DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030761.D
Acq On : 21 Apr 2023 13:43
Operator : SY/MD
Sample : 02398-11DL 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------