

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030763.D
 Acq On : 21 Apr 2023 14:31
 Operator : SY/MD
 Sample : VIBLK205
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK205

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rBV	81355	90610	12.39%	1.561%
2	1.536	148	154	165	rBV	84205	96181	13.15%	1.657%
3	2.066	310	319	334	rVB	158574	227852	31.15%	3.926%
4	2.294	387	390	395	rBV6	1282	1093	0.15%	0.019%
5	2.372	412	414	417	rBV5	1404	829	0.11%	0.014%
6	2.732	523	526	529	rVB4	1781	972	0.13%	0.017%
7	2.748	529	531	534	rBV3	1614	1121	0.15%	0.019%
8	2.825	551	555	556	rBV4	1215	832	0.11%	0.014%
9	2.864	563	567	569	rBV5	1939	1496	0.20%	0.026%
10	2.928	583	587	589	rBV3	1601	1053	0.14%	0.018%
11	3.137	647	652	655	rBV7	1967	2045	0.28%	0.035%
12	3.333	712	713	716	rVB3	1740	746	0.10%	0.013%
13	3.445	742	748	752	rBV8	1513	1869	0.26%	0.032%
14	3.507	764	767	770	rBV5	1822	1388	0.19%	0.024%
15	3.558	781	783	787	rVB5	1224	900	0.12%	0.016%
16	3.593	791	794	798	rBV5	1300	1044	0.14%	0.018%
17	3.806	851	860	879	rBV	50303	137859	18.85%	2.375%
18	4.105	951	953	956	rBV4	1163	787	0.11%	0.014%
19	4.175	972	975	979	rVB5	1989	1605	0.22%	0.028%
20	4.259	985	1001	1026	rBV	114806	297533	40.68%	5.126%
21	4.632	1114	1117	1119	rBV4	1424	967	0.13%	0.017%
22	4.728	1145	1147	1149	rBV2	1204	713	0.10%	0.012%
23	4.783	1162	1164	1166	rVB3	1533	622	0.09%	0.011%
24	4.802	1166	1170	1171	rBV4	1599	1001	0.14%	0.017%
25	4.835	1176	1180	1182	rBV5	1025	724	0.10%	0.012%
26	4.966	1201	1221	1250	rBV2	264332	731356	100.00%	12.601%
27	5.410	1357	1359	1360	rBV2	1498	630	0.09%	0.011%
28	5.542	1388	1400	1423	rBV	241031	504762	69.02%	8.697%
29	5.998	1530	1542	1558	rBV2	158219	325084	44.45%	5.601%
30	6.593	1725	1727	1733	rVB5	2577	1767	0.24%	0.030%
31	6.622	1734	1736	1739	rBV5	1221	872	0.12%	0.015%
32	6.712	1760	1764	1770	rBV7	1501	1745	0.24%	0.030%
33	6.921	1818	1829	1849	rBV	83845	163582	22.37%	2.818%
34	7.252	1921	1932	1954	rBV	280899	510117	69.75%	8.789%
35	7.468	1996	1999	2002	rBV4	1722	1274	0.17%	0.022%
36	7.561	2019	2028	2049	rBV	59669	111371	15.23%	1.919%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030763.D
 Acq On : 21 Apr 2023 14:31
 Operator : SY/MD
 Sample : VIBLK205
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK205

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.715	2074	2076	2081	rVB6	1909	1311	0.18%	0.023%
38	7.786	2096	2098	2102	rVB4	1656	771	0.11%	0.013%
39	7.944	2145	2147	2149	rVB2	1721	584	0.08%	0.010%
40	8.034	2166	2175	2205	rBV	167612	345941	47.30%	5.960%
41	8.297	2255	2257	2258	rBV	1365	549	0.08%	0.009%
42	8.693	2378	2380	2381	rBV3	1535	710	0.10%	0.012%
43	8.793	2400	2411	2437	rBV	375454	665366	90.98%	11.464%
44	9.011	2476	2479	2482	rBV5	1764	1226	0.17%	0.021%
45	9.124	2512	2514	2515	rBV2	1147	590	0.08%	0.010%
46	9.153	2521	2523	2525	rBV3	1444	1025	0.14%	0.018%
47	9.233	2545	2548	2551	rBV3	2045	1555	0.21%	0.027%
48	9.375	2589	2592	2597	rVB7	1563	1262	0.17%	0.022%
49	9.403	2597	2601	2603	rBV5	1606	1263	0.17%	0.022%
50	9.793	2720	2722	2725	rBV4	817	603	0.08%	0.010%
51	9.911	2757	2759	2763	rVB5	1569	904	0.12%	0.016%
52	10.018	2783	2792	2796	rBV9	2412	2891	0.40%	0.050%
53	10.159	2825	2836	2855	rVB	235071	375385	51.33%	6.468%
54	10.301	2878	2880	2887	rVB8	2068	2088	0.29%	0.036%
55	10.333	2887	2890	2895	rBV6	2497	2293	0.31%	0.040%
56	10.410	2911	2914	2916	rBV4	1240	705	0.10%	0.012%
57	10.503	2941	2943	2945	rVB4	1567	556	0.08%	0.010%
58	10.526	2945	2950	2952	rBV5	1736	1301	0.18%	0.022%
59	10.558	2957	2960	2963	rBV4	1383	982	0.13%	0.017%
60	10.606	2973	2975	2980	rBV6	1399	1303	0.18%	0.022%
61	10.680	2996	2998	3000	rVB3	1297	618	0.08%	0.011%
62	10.702	3003	3005	3010	rVB5	1327	712	0.10%	0.012%
63	10.850	3049	3051	3054	rBV3	1109	592	0.08%	0.010%
64	10.889	3060	3063	3067	rBV4	1016	646	0.09%	0.011%
65	10.915	3069	3071	3076	rBV5	892	748	0.10%	0.013%
66	11.014	3096	3102	3107	rBV8	1697	2214	0.30%	0.038%
67	11.130	3130	3138	3145	rBV8	3660	6527	0.89%	0.112%
68	11.194	3147	3158	3178	rVV	351671	598736	81.87%	10.316%
69	11.493	3249	3251	3254	rVB4	1649	874	0.12%	0.015%
70	11.509	3254	3256	3258	rBV2	1028	609	0.08%	0.010%
71	11.571	3260	3275	3294	rBV	301492	523283	71.55%	9.016%
72	11.908	3377	3380	3383	rBV4	1568	1124	0.15%	0.019%
73	11.924	3383	3385	3389	rVV5	1111	750	0.10%	0.013%
74	11.956	3392	3395	3399	rVV6	1352	1065	0.15%	0.018%
75	12.046	3421	3423	3427	rVB4	1352	928	0.13%	0.016%
76	12.217	3474	3476	3479	rBV4	1537	940	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030763.D
 Acq On : 21 Apr 2023 14:31
 Operator : SY/MD
 Sample : VIBLK205
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK205

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.255	3483	3488	3491	rBV7	1030	1147	0.16%	0.020%
78	12.320	3505	3508	3511	rVB4	2109	1355	0.19%	0.023%
79	12.339	3511	3514	3516	rBV3	1353	774	0.11%	0.013%
80	12.426	3538	3541	3542	rBV3	990	613	0.08%	0.011%
81	12.452	3545	3549	3551	rBV5	1151	971	0.13%	0.017%
82	12.503	3558	3565	3570	rBV9	1805	1918	0.26%	0.033%
83	12.635	3605	3606	3609	rBV3	1126	562	0.08%	0.010%
84	12.670	3614	3617	3622	rBV6	1853	2197	0.30%	0.038%
85	12.744	3638	3640	3642	rBV3	1495	736	0.10%	0.013%
86	12.776	3648	3650	3652	rBV3	899	576	0.08%	0.010%
87	12.796	3652	3656	3661	rVB6	1635	1789	0.24%	0.031%
88	12.940	3697	3701	3704	rBV6	915	1009	0.14%	0.017%
89	13.056	3735	3737	3742	rVB6	1394	830	0.11%	0.014%
90	13.368	3831	3834	3839	rVB7	2085	1611	0.22%	0.028%
91	13.390	3839	3841	3844	rBV3	1355	770	0.11%	0.013%
92	13.423	3847	3851	3853	rBV5	1503	1342	0.18%	0.023%
93	13.763	3955	3957	3959	rBV3	1302	700	0.10%	0.012%
94	14.156	4077	4079	4085	rVB6	1797	1241	0.17%	0.021%
95	14.233	4101	4103	4106	rBV3	1086	739	0.10%	0.013%
96	14.316	4125	4129	4131	rBV4	1304	960	0.13%	0.017%
97	14.381	4146	4149	4151	rBV3	1639	1257	0.17%	0.022%
98	14.474	4172	4178	4183	rBV9	1792	2347	0.32%	0.040%
99	14.535	4195	4197	4201	rBV5	1322	991	0.14%	0.017%
100	14.895	4306	4309	4314	rBV6	1966	1693	0.23%	0.029%




Sum of corrected areas: 5804060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030763.D
Acq On : 21 Apr 2023 14:31
Operator : SY/MD
Sample : VIBLK205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

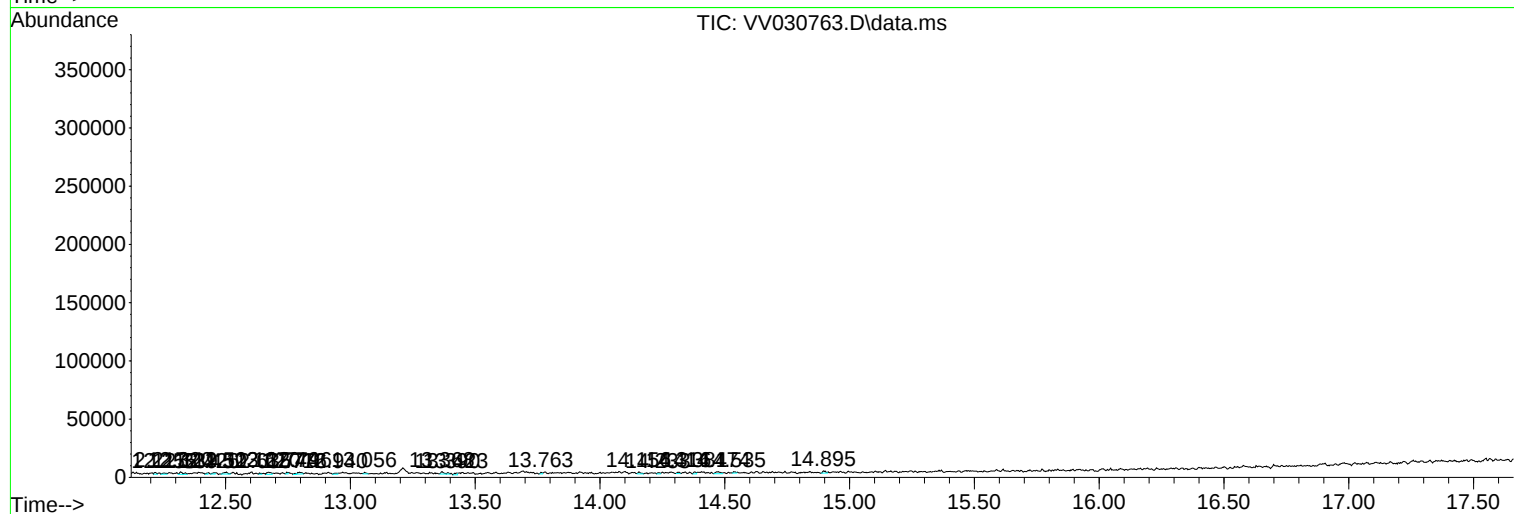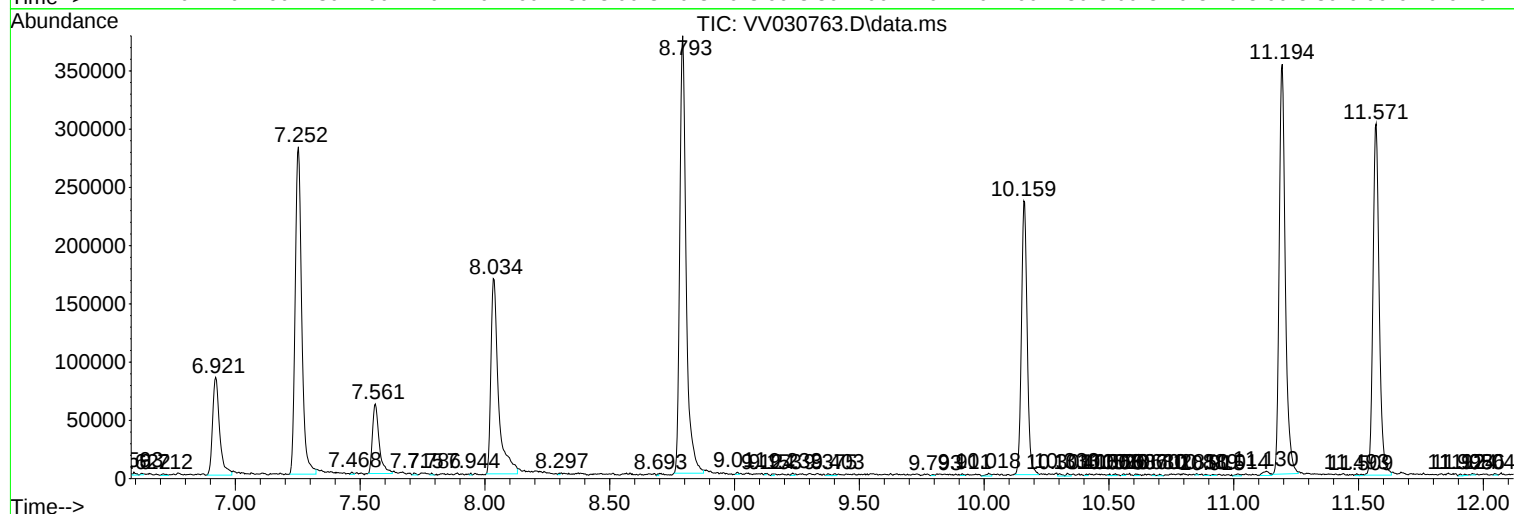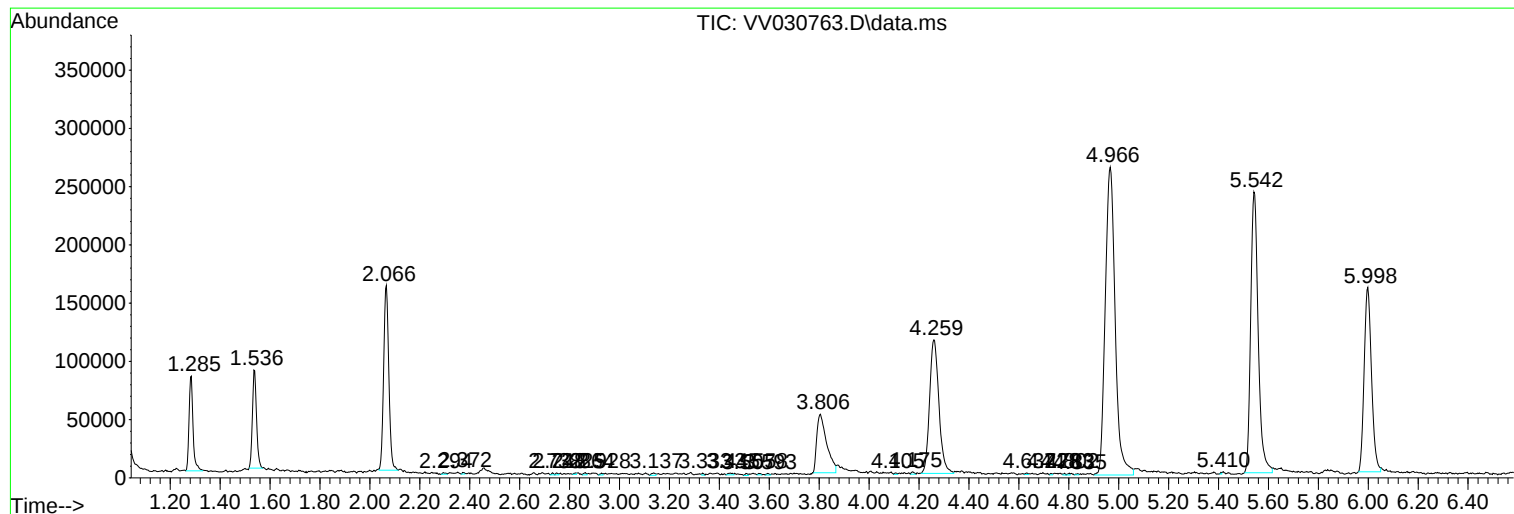

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030763.D
Acq On : 21 Apr 2023 14:31
Operator : SY/MD
Sample : VIBLK205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030763.D
Acq On : 21 Apr 2023 14:31
Operator : SY/MD
Sample : VIBLK205
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc