

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030764.D
 Acq On : 21 Apr 2023 14:57
 Operator : SY/MD
 Sample : 02398-06DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	98150	104524	8.67%	1.423%
2	1.536	148	154	170	rVB	98638	118910	9.87%	1.618%
3	2.066	310	319	338	rVB	194418	285550	23.69%	3.886%
4	2.359	407	410	413	rBV5	1217	944	0.08%	0.013%
5	2.397	416	422	424	rBV7	1931	2101	0.17%	0.029%
6	2.455	427	440	454	rBV2	30525	55941	4.64%	0.761%
7	2.626	491	493	496	rBV3	1376	790	0.07%	0.011%
8	2.812	546	551	552	rBV5	1073	782	0.06%	0.011%
9	3.156	654	658	662	rBV6	1535	1543	0.13%	0.021%
10	3.188	665	668	671	rBV3	1425	868	0.07%	0.012%
11	3.336	709	714	717	rBV8	1217	1337	0.11%	0.018%
12	3.452	748	750	753	rBV3	1096	718	0.06%	0.010%
13	3.503	762	766	770	rVB6	1169	936	0.08%	0.013%
14	3.716	828	832	833	rBV4	1232	879	0.07%	0.012%
15	3.735	836	838	841	rVB4	1664	846	0.07%	0.012%
16	3.754	841	844	848	rBV5	835	659	0.05%	0.009%
17	3.806	849	860	886	rBV	49923	151131	12.54%	2.057%
18	4.259	983	1001	1021	rVV	125887	329151	27.31%	4.480%
19	4.622	1112	1114	1117	rBV4	1267	658	0.05%	0.009%
20	4.674	1127	1130	1132	rBV5	1198	893	0.07%	0.012%
21	4.777	1158	1162	1166	rBV6	1334	1342	0.11%	0.018%
22	4.857	1185	1187	1189	rBV3	1221	650	0.05%	0.009%
23	4.905	1200	1202	1204	rBV3	1691	842	0.07%	0.011%
24	4.966	1204	1221	1249	rVV2	287789	777989	64.55%	10.588%
25	5.179	1283	1287	1290	rBV6	1374	1139	0.09%	0.016%
26	5.542	1386	1400	1419	rBV	280566	586123	48.63%	7.977%
27	5.995	1531	1541	1561	rVB	172872	346089	28.71%	4.710%
28	6.259	1620	1623	1630	rVB7	2048	2305	0.19%	0.031%
29	6.288	1630	1632	1634	rBV3	1019	621	0.05%	0.008%
30	6.298	1634	1635	1639	rVB4	1221	646	0.05%	0.009%
31	6.622	1733	1736	1740	rBV6	1219	1146	0.10%	0.016%
32	6.728	1764	1769	1770	rBV5	1118	752	0.06%	0.010%
33	6.854	1806	1808	1813	rVB5	1470	869	0.07%	0.012%
34	6.921	1819	1829	1844	rBV	87386	163772	13.59%	2.229%
35	7.092	1879	1882	1885	rBV5	1598	1405	0.12%	0.019%
36	7.249	1920	1931	1951	rBV	328135	574984	47.70%	7.825%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030764.D
 Acq On : 21 Apr 2023 14:57
 Operator : SY/MD
 Sample : 02398-06DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.561	2020	2028	2044	rVB	62537	106039	8.80%	1.443%
38	7.809	2101	2105	2110	rBV8	2095	1796	0.15%	0.024%
39	7.892	2128	2131	2132	rBV3	1274	644	0.05%	0.009%
40	8.034	2166	2175	2190	rBV	163878	310391	25.75%	4.224%
41	8.272	2244	2249	2251	rBV5	1905	1943	0.16%	0.026%
42	8.751	2395	2398	2399	rBV3	1469	834	0.07%	0.011%
43	8.793	2400	2411	2436	rVV2	431884	902584	74.88%	12.284%
44	9.047	2486	2490	2493	rBV6	1690	1810	0.15%	0.025%
45	9.156	2519	2524	2525	rBV4	1543	1185	0.10%	0.016%
46	9.220	2542	2544	2548	rVB4	1903	1171	0.10%	0.016%
47	9.336	2576	2580	2581	rBV3	1457	838	0.07%	0.011%
48	9.368	2586	2590	2592	rBV5	1277	742	0.06%	0.010%
49	9.410	2599	2603	2605	rBV5	1775	1250	0.10%	0.017%
50	9.461	2617	2619	2622	rBV4	1491	1076	0.09%	0.015%
51	9.577	2652	2655	2660	rVB6	2371	1633	0.14%	0.022%
52	9.674	2681	2685	2688	rVV5	1263	1015	0.08%	0.014%
53	9.764	2709	2713	2719	rBV7	1952	1834	0.15%	0.025%
54	9.789	2719	2721	2725	rVV5	1194	651	0.05%	0.009%
55	9.879	2742	2749	2751	rBV6	1551	1752	0.15%	0.024%
56	10.005	2785	2788	2790	rBV4	1516	947	0.08%	0.013%
57	10.098	2812	2817	2819	rBV4	931	991	0.08%	0.013%
58	10.159	2826	2836	2849	rBV	240680	380100	31.53%	5.173%
59	10.410	2911	2914	2916	rBV4	1648	1063	0.09%	0.014%
60	10.503	2941	2943	2946	rBV4	1412	643	0.05%	0.009%
61	10.564	2960	2962	2965	rBV3	1103	857	0.07%	0.012%
62	10.657	2989	2991	2995	rVB3	1349	672	0.06%	0.009%
63	10.686	2996	3000	3006	rVB6	1954	1762	0.15%	0.024%
64	10.728	3011	3013	3015	rBV3	1164	713	0.06%	0.010%
65	10.934	3076	3077	3082	rVB4	1998	1309	0.11%	0.018%
66	10.982	3088	3092	3096	rBV6	1578	1376	0.11%	0.019%
67	11.018	3102	3103	3108	rVB4	1383	839	0.07%	0.011%
68	11.047	3108	3112	3113	rBV4	1061	791	0.07%	0.011%
69	11.088	3120	3125	3126	rBV5	1336	855	0.07%	0.012%
70	11.127	3132	3137	3145	rVB2	10326	12846	1.07%	0.175%
71	11.194	3147	3158	3181	rVV	430879	744598	61.78%	10.134%
72	11.384	3215	3217	3220	rBV3	1460	926	0.08%	0.013%
73	11.416	3224	3227	3228	rBV3	1397	770	0.06%	0.010%
74	11.580	3262	3278	3296	rBV2	505868	1205328	100.00%	16.404%
75	11.764	3332	3335	3338	rBV5	1156	997	0.08%	0.014%
76	12.050	3422	3424	3427	rBV4	1034	599	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030764.D
 Acq On : 21 Apr 2023 14:57
 Operator : SY/MD
 Sample : 02398-06DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.111	3439	3443	3447	rBV5	1809	1702	0.14%	0.023%
78	12.175	3459	3463	3464	rBV4	1088	598	0.05%	0.008%
79	12.201	3468	3471	3474	rBV5	1024	715	0.06%	0.010%
80	12.275	3492	3494	3497	rVB4	1222	841	0.07%	0.011%
81	12.300	3497	3502	3506	rBV7	1242	1262	0.10%	0.017%
82	12.342	3511	3515	3516	rBV4	1385	795	0.07%	0.011%
83	12.516	3567	3569	3570	rBV2	1262	585	0.05%	0.008%
84	12.657	3610	3613	3616	rBV5	1110	741	0.06%	0.010%
85	12.735	3629	3637	3642	rVB10	1399	1808	0.15%	0.025%
86	12.776	3647	3650	3652	rBV3	964	707	0.06%	0.010%
87	12.950	3700	3704	3709	rBV7	681	638	0.05%	0.009%
88	13.014	3720	3724	3727	rBV4	1644	1699	0.14%	0.023%
89	13.207	3776	3784	3797	rVB	59535	91735	7.61%	1.249%
90	13.320	3817	3819	3822	rBV3	1317	804	0.07%	0.011%
91	13.336	3822	3824	3826	rVV3	1249	639	0.05%	0.009%
92	13.526	3880	3883	3887	rBV5	1137	637	0.05%	0.009%
93	13.583	3898	3901	3903	rBV3	1341	741	0.06%	0.010%
94	13.689	3926	3934	3945	rBV7	10289	17474	1.45%	0.238%
95	13.918	4001	4005	4006	rBV4	1325	1027	0.09%	0.014%
96	14.342	4134	4137	4138	rBV2	1731	856	0.07%	0.012%
97	14.635	4224	4228	4230	rBV5	1023	824	0.07%	0.011%
98	14.693	4243	4246	4247	rBV4	1308	703	0.06%	0.010%
99	15.040	4350	4354	4356	rBV4	1567	1288	0.11%	0.018%
100	15.101	4371	4373	4376	rBV3	1294	769	0.06%	0.010%


Sum of corrected areas: 7347593

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030764.D
Acq On : 21 Apr 2023 14:57
Operator : SY/MD
Sample : 02398-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

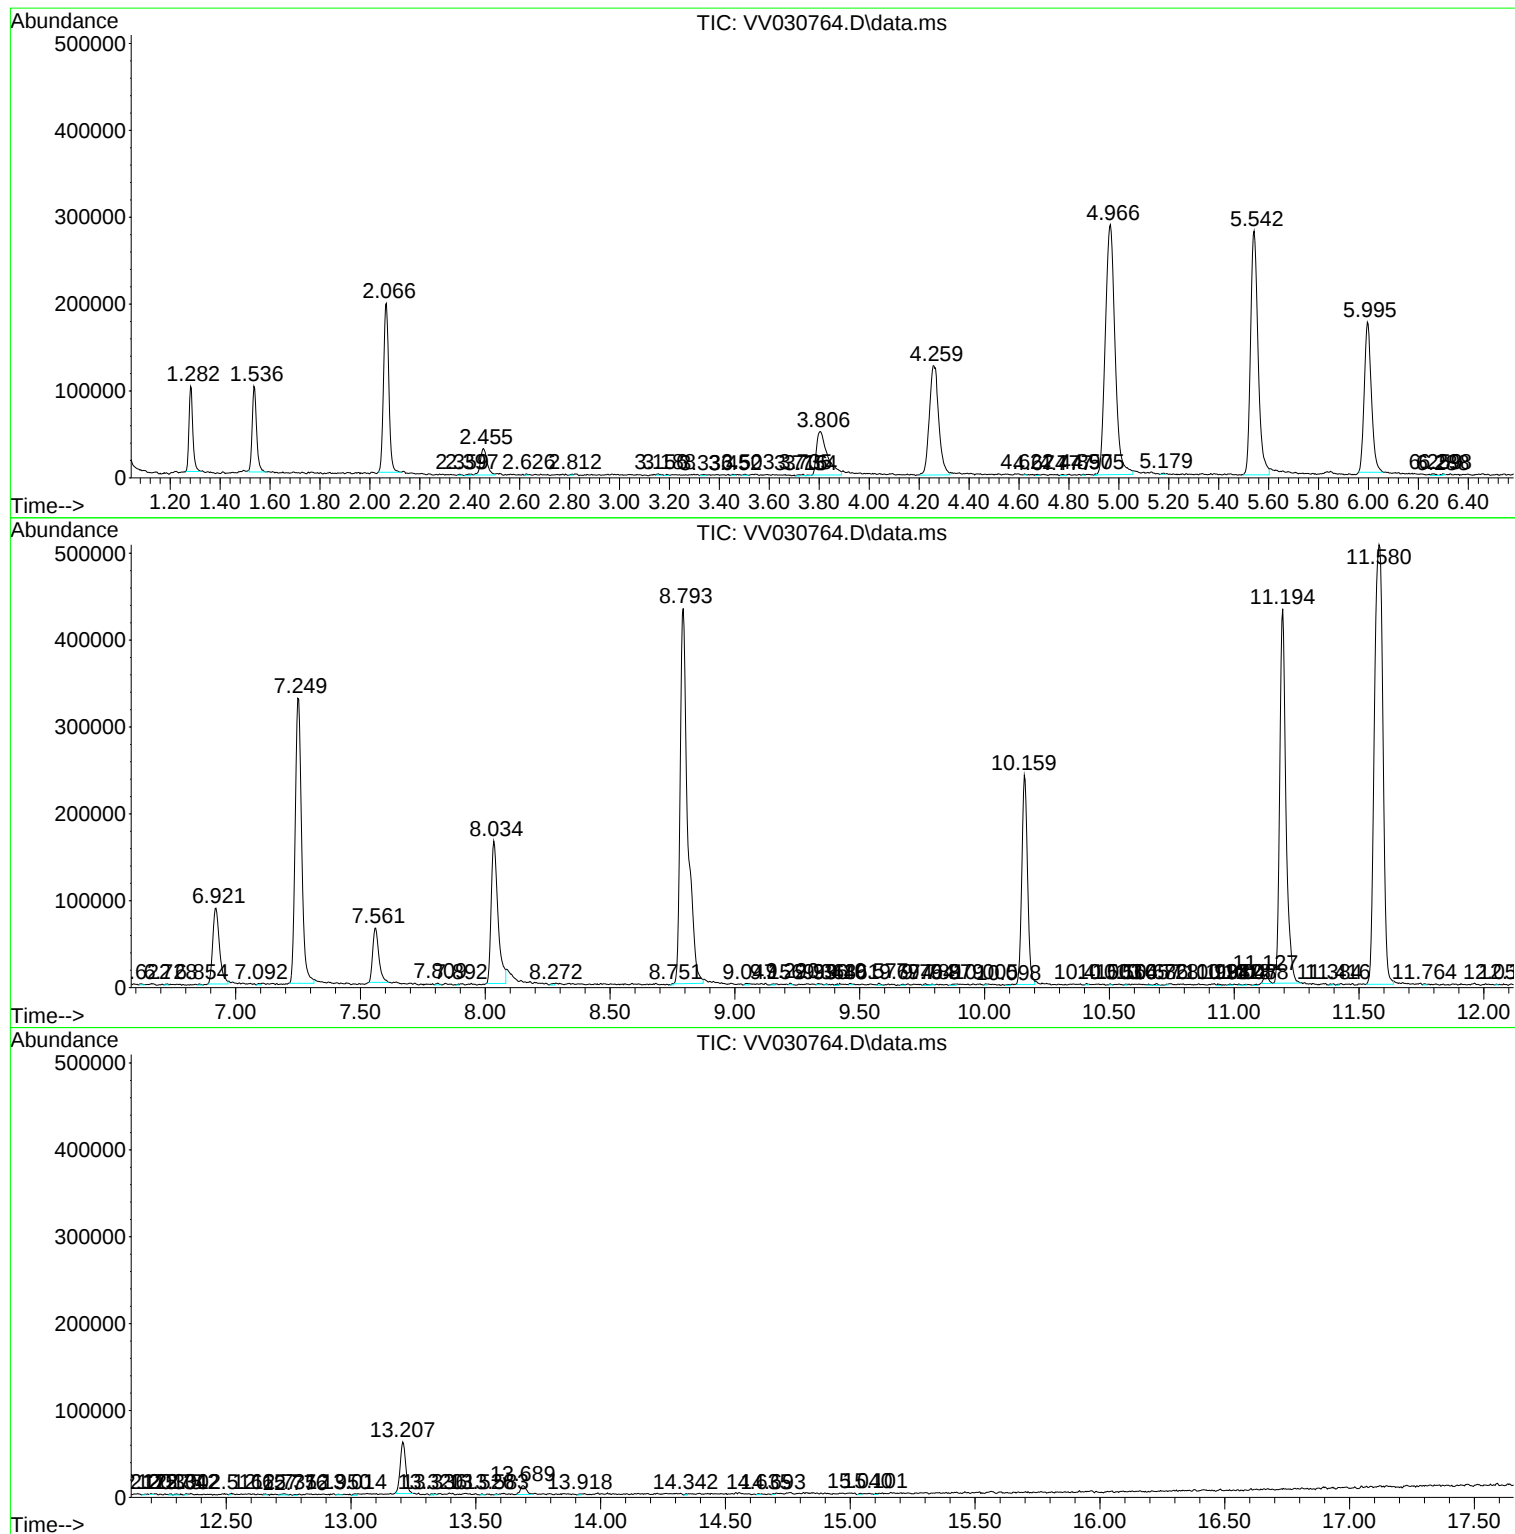

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030764.D
Acq On : 21 Apr 2023 14:57
Operator : SY/MD
Sample : 02398-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030764.D
Acq On : 21 Apr 2023 14:57
Operator : SY/MD
Sample : 02398-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------