

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030765.D
 Acq On : 21 Apr 2023 15:21
 Operator : SY/MD
 Sample : 02398-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	103075	113420	9.40%	1.482%
2	1.535	148	154	167	rVB	99966	119030	9.87%	1.556%
3	2.066	310	319	339	rVB	201514	296568	24.58%	3.876%
4	2.240	371	373	377	rBV4	1845	1402	0.12%	0.018%
5	2.384	415	418	423	rBV5	1098	1067	0.09%	0.014%
6	2.455	433	440	456	rVB2	30635	53718	4.45%	0.702%
7	2.555	469	471	475	rVB5	1806	1031	0.09%	0.013%
8	2.757	532	534	537	rBV3	883	608	0.05%	0.008%
9	2.793	543	545	548	rVB3	1444	752	0.06%	0.010%
10	2.966	597	599	601	rBV3	1038	515	0.04%	0.007%
11	3.079	632	634	639	rVV4	1298	1124	0.09%	0.015%
12	3.143	652	654	657	rVB4	1079	518	0.04%	0.007%
13	3.185	663	667	668	rBV4	1302	1068	0.09%	0.014%
14	3.214	673	676	679	rVB4	1059	744	0.06%	0.010%
15	3.397	730	733	735	rBV5	841	537	0.04%	0.007%
16	3.442	745	747	750	rVB4	1801	1155	0.10%	0.015%
17	3.500	762	765	769	rBV4	1430	1030	0.09%	0.013%
18	3.593	790	794	797	rBV5	2426	1976	0.16%	0.026%
19	3.613	797	800	801	rVV3	1268	644	0.05%	0.008%
20	3.805	850	860	887	rBV	50062	143553	11.90%	1.876%
21	4.124	957	959	961	rBV2	1407	777	0.06%	0.010%
22	4.204	979	984	985	rBV4	2004	1467	0.12%	0.019%
23	4.259	988	1001	1019	rVV2	127092	317416	26.31%	4.149%
24	4.876	1190	1193	1194	rBV3	952	551	0.05%	0.007%
25	4.966	1205	1221	1233	rBV2	295038	783330	64.93%	10.238%
26	5.259	1310	1312	1315	rBV3	1326	789	0.07%	0.010%
27	5.542	1388	1400	1422	rBV	285814	590506	48.95%	7.718%
28	5.831	1484	1490	1492	rBV6	2698	3247	0.27%	0.042%
29	5.998	1530	1542	1561	rBV	173870	352531	29.22%	4.608%
30	6.207	1606	1607	1611	rVB4	1616	838	0.07%	0.011%
31	6.371	1656	1658	1661	rBV4	1363	1019	0.08%	0.013%
32	6.481	1689	1692	1694	rBV3	1738	951	0.08%	0.012%
33	6.516	1701	1703	1707	rBV4	1518	934	0.08%	0.012%
34	6.574	1719	1721	1722	rBV2	1380	599	0.05%	0.008%
35	6.741	1770	1773	1775	rBV4	1377	869	0.07%	0.011%
36	6.754	1775	1777	1782	rVB6	1200	853	0.07%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030765.D
 Acq On : 21 Apr 2023 15:21
 Operator : SY/MD
 Sample : 02398-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.780	1782	1785	1787	rBV4	1163	598	0.05%	0.008%
38	6.921	1819	1829	1843	rBV2	88605	165902	13.75%	2.168%
39	7.252	1920	1932	1953	rBV	337941	597989	49.57%	7.816%
40	7.561	2019	2028	2054	rBV	64644	119050	9.87%	1.556%
41	7.950	2147	2149	2153	rBV5	1077	813	0.07%	0.011%
42	8.034	2164	2175	2201	rBV	171038	353061	29.26%	4.615%
43	8.397	2286	2288	2290	rVB3	1492	635	0.05%	0.008%
44	8.458	2305	2307	2310	rBV4	1351	634	0.05%	0.008%
45	8.635	2360	2362	2363	rBV2	1412	526	0.04%	0.007%
46	8.792	2399	2411	2417	rBV	449944	767863	63.65%	10.036%
47	9.172	2527	2529	2530	rBV	1491	559	0.05%	0.007%
48	9.291	2564	2566	2570	rVB4	1570	772	0.06%	0.010%
49	9.429	2606	2609	2612	rBV4	1592	1105	0.09%	0.014%
50	9.551	2645	2647	2652	rVV5	1353	1165	0.10%	0.015%
51	9.680	2684	2687	2691	rBV6	1729	1383	0.11%	0.018%
52	9.734	2700	2704	2708	rBV6	1059	1105	0.09%	0.014%
53	9.834	2733	2735	2737	rVB3	1362	607	0.05%	0.008%
54	9.857	2737	2742	2744	rBV6	1495	1189	0.10%	0.016%
55	9.892	2749	2753	2756	rBV6	2071	1683	0.14%	0.022%
56	9.911	2757	2759	2765	rVV7	1944	1291	0.11%	0.017%
57	10.014	2787	2791	2793	rBV6	1709	1139	0.09%	0.015%
58	10.159	2822	2836	2855	rBV	250890	392239	32.51%	5.127%
59	10.268	2867	2870	2871	rBV3	1086	592	0.05%	0.008%
60	10.358	2896	2898	2901	rVB3	1150	568	0.05%	0.007%
61	10.432	2918	2921	2922	rBV3	1842	1005	0.08%	0.013%
62	10.493	2936	2940	2944	rBV7	1408	1556	0.13%	0.020%
63	10.513	2944	2946	2947	rBV2	1328	646	0.05%	0.008%
64	10.538	2952	2954	2960	rVB7	1193	782	0.06%	0.010%
65	10.564	2960	2962	2965	rBV4	1182	883	0.07%	0.012%
66	10.783	3028	3030	3032	rBV3	1315	692	0.06%	0.009%
67	10.934	3075	3077	3079	rVB3	1487	534	0.04%	0.007%
68	10.985	3090	3093	3096	rBV4	1011	691	0.06%	0.009%
69	11.127	3127	3137	3146	rBV2	27761	45605	3.78%	0.596%
70	11.194	3147	3158	3183	rVB2	465430	1075525	89.15%	14.058%
71	11.426	3228	3230	3233	rBV3	1525	1041	0.09%	0.014%
72	11.580	3262	3278	3297	rBV2	505685	1206443	100.00%	15.769%
73	11.821	3352	3353	3355	rBV2	1126	523	0.04%	0.007%
74	11.988	3403	3405	3408	rBV4	1081	742	0.06%	0.010%
75	12.014	3411	3413	3417	rVB5	1829	1233	0.10%	0.016%
76	12.165	3458	3460	3466	rVB6	1385	1330	0.11%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030765.D
 Acq On : 21 Apr 2023 15:21
 Operator : SY/MD
 Sample : 02398-03DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.201	3466	3471	3473	rBV6	1429	1265	0.10%	0.017%
78	12.268	3489	3492	3496	rVB5	1900	1218	0.10%	0.016%
79	12.313	3504	3506	3508	rBV3	1622	722	0.06%	0.009%
80	12.374	3521	3525	3529	rBV5	1097	1096	0.09%	0.014%
81	12.467	3549	3554	3558	rVB7	1772	1794	0.15%	0.023%
82	12.487	3558	3560	3562	rVB2	1366	578	0.05%	0.008%
83	12.503	3562	3565	3566	rBV2	1418	745	0.06%	0.010%
84	12.705	3625	3628	3632	rVB5	2097	1413	0.12%	0.018%
85	12.840	3668	3670	3673	rBV4	963	593	0.05%	0.008%
86	12.879	3677	3682	3686	rBV8	2291	2047	0.17%	0.027%
87	12.959	3704	3707	3708	rBV2	1881	1061	0.09%	0.014%
88	13.014	3719	3724	3728	rVB5	1359	1150	0.10%	0.015%
89	13.075	3742	3743	3745	rBV2	1204	667	0.06%	0.009%
90	13.156	3765	3768	3770	rBV4	1986	1287	0.11%	0.017%
91	13.168	3770	3772	3773	rVV2	1617	700	0.06%	0.009%
92	13.207	3776	3784	3798	rVB2	36850	59425	4.93%	0.777%
93	13.287	3807	3809	3813	rVB4	1592	789	0.07%	0.010%
94	13.390	3838	3841	3843	rVB4	1311	643	0.05%	0.008%
95	13.426	3849	3852	3855	rBV4	1345	888	0.07%	0.012%
96	13.451	3855	3860	3864	rBV7	1569	2101	0.17%	0.027%
97	13.599	3904	3906	3908	rBV3	1224	784	0.06%	0.010%
98	13.625	3912	3914	3917	rBV4	1845	1120	0.09%	0.015%
99	13.689	3927	3934	3945	rVB4	11676	19256	1.60%	0.252%
100	14.528	4193	4195	4197	rBV3	1110	676	0.06%	0.009%




Sum of corrected areas: 7650854

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030765.D
Acq On : 21 Apr 2023 15:21
Operator : SY/MD
Sample : 02398-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

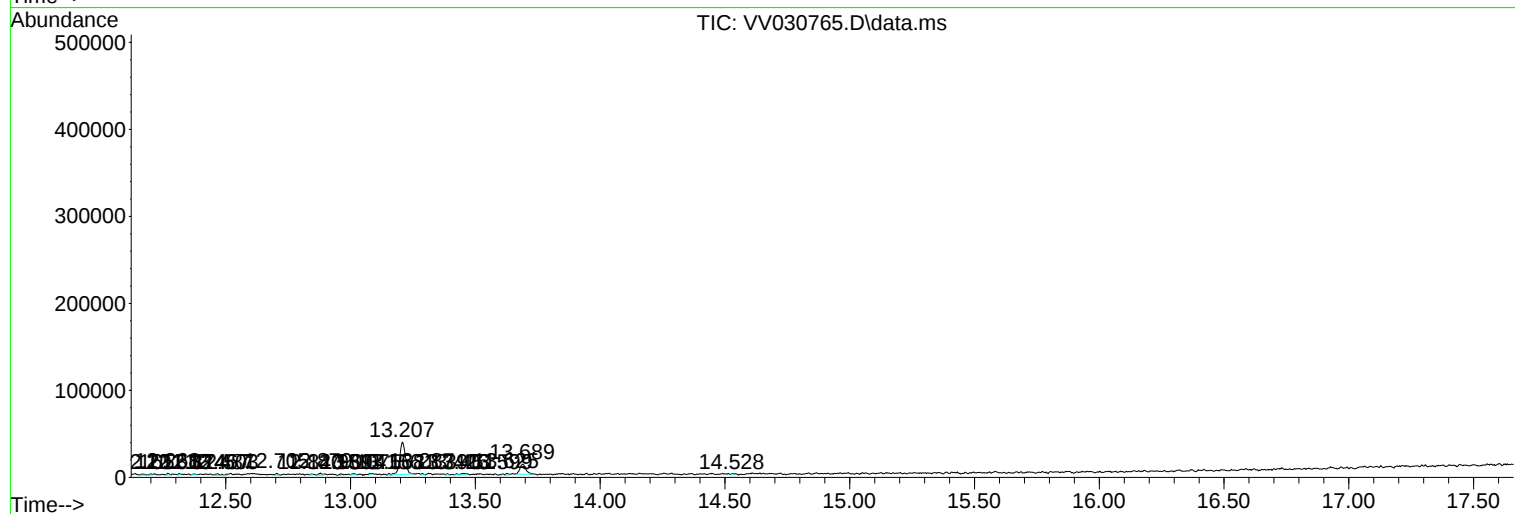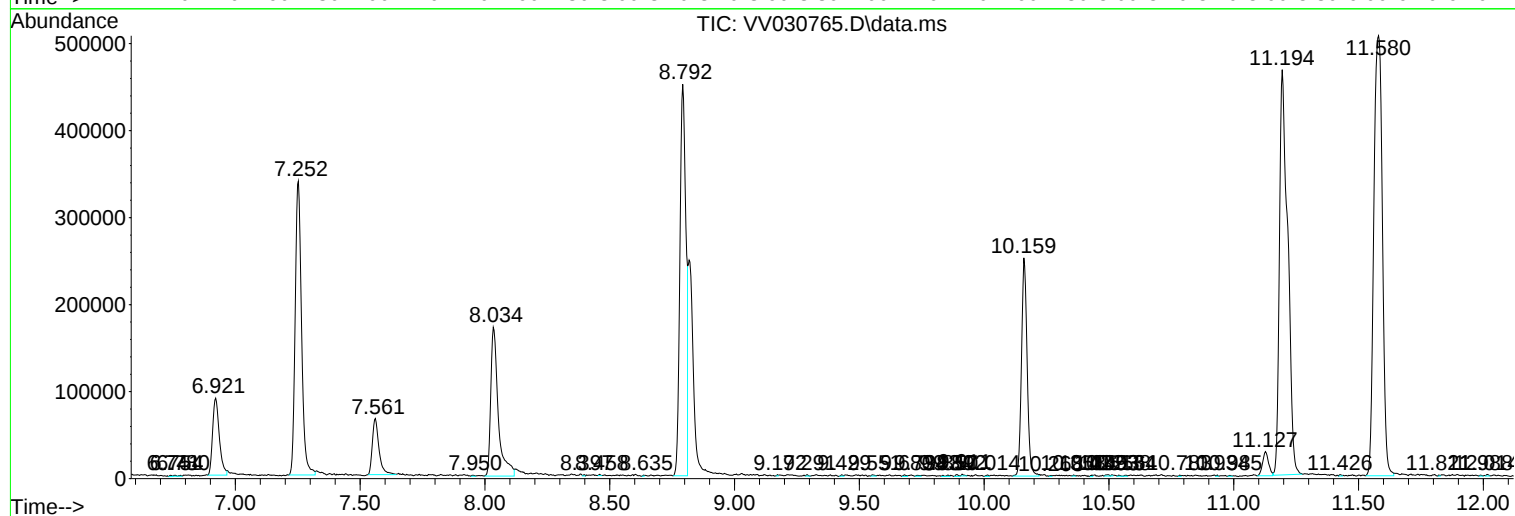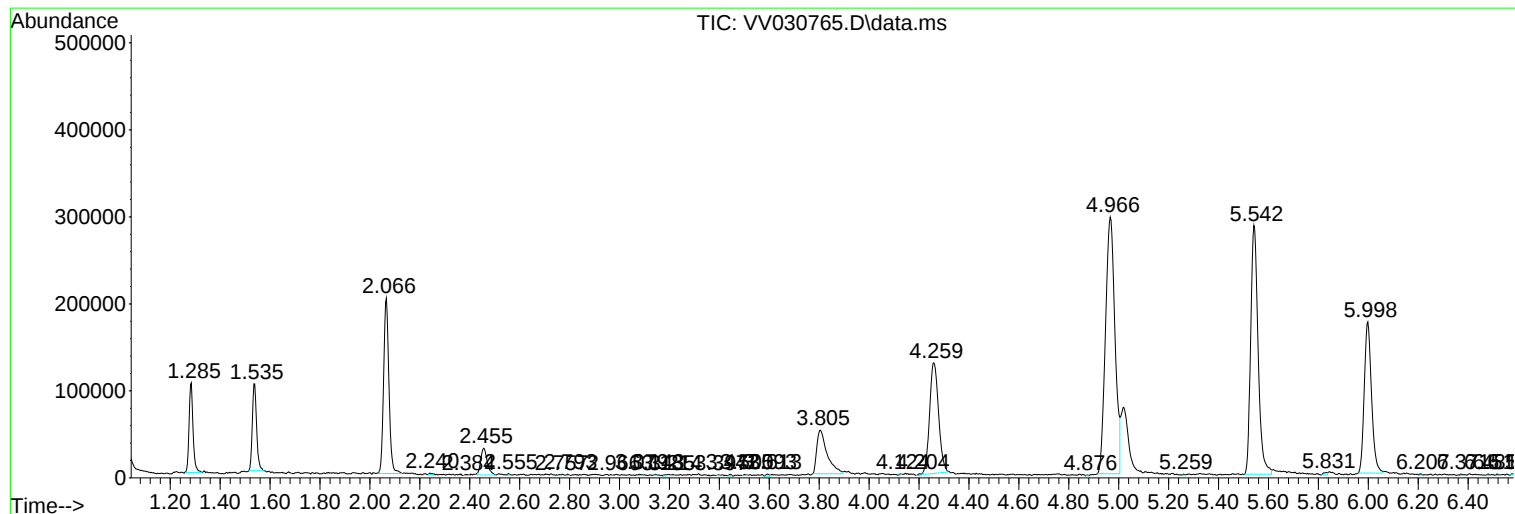

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030765.D
Acq On : 21 Apr 2023 15:21
Operator : SY/MD
Sample : 02398-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030765.D
Acq On : 21 Apr 2023 15:21
Operator : SY/MD
Sample : 02398-03DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------