

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030767.D
 Acq On : 21 Apr 2023 16:09
 Operator : SY/MD
 Sample : 02398-08 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	98570	105624	3.92%	0.978%
2	1.539	148	155	167	rVB	98993	116093	4.31%	1.075%
3	2.066	310	319	335	rVB	191949	279732	10.38%	2.591%
4	2.224	366	368	372	rBV4	1196	828	0.03%	0.008%
5	2.323	396	399	400	rBV3	912	418	0.02%	0.004%
6	2.407	420	425	428	rBV7	1724	1610	0.06%	0.015%
7	2.760	533	535	537	rBV	1357	691	0.03%	0.006%
8	2.770	537	538	540	rVB3	948	295	0.01%	0.003%
9	2.812	548	551	552	rBV2	1031	612	0.02%	0.006%
10	2.931	586	588	589	rBV2	1025	531	0.02%	0.005%
11	2.963	597	598	601	rVB3	1298	503	0.02%	0.005%
12	2.979	601	603	606	rBV4	840	526	0.02%	0.005%
13	2.995	606	608	610	rVV3	1348	692	0.03%	0.006%
14	3.024	613	617	619	rVB5	1374	1112	0.04%	0.010%
15	3.043	619	623	626	rBV5	1603	1797	0.07%	0.017%
16	3.121	642	647	650	rBV6	1655	1214	0.05%	0.011%
17	3.133	650	651	654	rBV3	888	399	0.01%	0.004%
18	3.285	693	698	700	rBV5	1302	1054	0.04%	0.010%
19	3.310	704	706	708	rBV4	983	597	0.02%	0.006%
20	3.387	726	730	734	rBV5	1170	1305	0.05%	0.012%
21	3.404	734	735	737	rBV2	1026	315	0.01%	0.003%
22	3.490	757	762	768	rVB9	1803	1754	0.07%	0.016%
23	3.523	768	772	774	rBV4	2147	1314	0.05%	0.012%
24	3.558	781	783	786	rBV4	1051	785	0.03%	0.007%
25	3.603	794	797	798	rBV3	1358	669	0.02%	0.006%
26	3.805	850	860	882	rBV	52999	156702	5.81%	1.451%
27	4.259	986	1001	1022	rBV	130135	336289	12.48%	3.114%
28	4.522	1081	1083	1087	rBV5	1684	955	0.04%	0.009%
29	4.641	1118	1120	1123	rBV4	1140	767	0.03%	0.007%
30	4.805	1168	1171	1173	rVB3	1344	717	0.03%	0.007%
31	4.966	1204	1221	1231	rBV2	293891	762506	28.30%	7.062%
32	5.487	1377	1383	1385	rBV7	1712	1540	0.06%	0.014%
33	5.542	1388	1400	1426	rVV	290925	596073	22.12%	5.520%
34	5.998	1530	1542	1565	rBV	172139	352522	13.08%	3.265%
35	6.301	1634	1636	1640	rVB5	2442	1509	0.06%	0.014%
36	6.320	1640	1642	1646	rBV5	880	598	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030767.D
 Acq On : 21 Apr 2023 16:09
 Operator : SY/MD
 Sample : 02398-08 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.346	1646	1650	1651	rBV4	1519	1071	0.04%	0.010%
38	6.420	1672	1673	1676	rBV2	1044	637	0.02%	0.006%
39	6.484	1691	1693	1696	rBV3	596	266	0.01%	0.002%
40	6.558	1714	1716	1718	rBV3	1742	1043	0.04%	0.010%
41	6.690	1754	1757	1758	rBV2	1487	807	0.03%	0.007%
42	6.744	1773	1774	1776	rBV2	1186	392	0.01%	0.004%
43	6.821	1791	1798	1800	rBV7	1919	1795	0.07%	0.017%
44	6.921	1819	1829	1846	rBV	89257	168616	6.26%	1.562%
45	7.149	1896	1900	1903	rBV5	1892	1607	0.06%	0.015%
46	7.252	1921	1932	1953	rBV	325862	573443	21.28%	5.311%
47	7.561	2019	2028	2045	rBV	64730	114331	4.24%	1.059%
48	7.972	2152	2156	2159	rBV6	1414	1427	0.05%	0.013%
49	8.034	2165	2175	2194	rBV	174684	340757	12.64%	3.156%
50	8.352	2272	2274	2276	rBV3	1662	976	0.04%	0.009%
51	8.567	2335	2341	2342	rBV5	2286	1951	0.07%	0.018%
52	8.712	2384	2386	2387	rBV2	1064	434	0.02%	0.004%
53	8.728	2387	2391	2392	rVV3	1387	846	0.03%	0.008%
54	8.796	2400	2412	2413	rBV	483542	585567	21.73%	5.423%
55	9.304	2568	2570	2573	rBV4	1127	604	0.02%	0.006%
56	9.477	2621	2624	2626	rBV5	1341	868	0.03%	0.008%
57	9.606	2661	2664	2667	rBV5	1222	765	0.03%	0.007%
58	9.638	2672	2674	2677	rVB4	1129	406	0.02%	0.004%
59	9.696	2690	2692	2697	rVB6	1646	1298	0.05%	0.012%
60	9.715	2697	2698	2706	rVB7	1815	1665	0.06%	0.015%
61	9.757	2709	2711	2712	rBV2	841	273	0.01%	0.003%
62	9.850	2738	2740	2743	rBV3	1390	812	0.03%	0.008%
63	9.934	2764	2766	2768	rBV3	1247	767	0.03%	0.007%
64	9.988	2780	2783	2787	rBV4	1169	979	0.04%	0.009%
65	10.091	2813	2815	2817	rBV3	862	370	0.01%	0.003%
66	10.159	2824	2836	2853	rBV	239004	390146	14.48%	3.613%
67	10.233	2857	2859	2862	rVV4	1275	743	0.03%	0.007%
68	10.265	2866	2869	2874	rVB5	2002	1340	0.05%	0.012%
69	10.291	2874	2877	2878	rBV3	1333	858	0.03%	0.008%
70	10.349	2894	2895	2899	rVB4	1348	794	0.03%	0.007%
71	10.432	2918	2921	2926	rBV6	1176	1094	0.04%	0.010%
72	10.542	2953	2955	2956	rBV3	774	337	0.01%	0.003%
73	10.577	2961	2966	2969	rBV6	1956	1952	0.07%	0.018%
74	10.667	2989	2994	2995	rBV4	1350	1024	0.04%	0.009%
75	10.738	3012	3016	3018	rBV5	1668	1270	0.05%	0.012%
76	10.824	3041	3043	3048	rVB5	1217	980	0.04%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030767.D
 Acq On : 21 Apr 2023 16:09
 Operator : SY/MD
 Sample : 02398-08 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	10.985	3090	3093	3094	rBV2	1099	702	0.03%	0.007%
78	11.033	3103	3108	3111	rVB6	1255	937	0.03%	0.009%
79	11.053	3112	3114	3118	rBV4	977	806	0.03%	0.007%
80	11.123	3124	3136	3147	rBV	228101	356287	13.22%	3.300%
81	11.217	3148	3165	3181	rVB2	1063923	2310360	85.73%	21.396%
82	11.586	3262	3280	3299	rBV2	1433775	2694832	100.00%	24.957%
83	11.911	3378	3381	3388	rBV9	1864	2454	0.09%	0.023%
84	12.172	3460	3462	3464	rBV3	1343	776	0.03%	0.007%
85	12.185	3464	3466	3469	rVV3	1129	680	0.03%	0.006%
86	12.271	3491	3493	3494	rBV2	945	338	0.01%	0.003%
87	12.583	3586	3590	3592	rBV5	2158	1661	0.06%	0.015%
88	12.738	3632	3638	3641	rBV8	2104	1904	0.07%	0.018%
89	12.850	3668	3673	3676	rBV6	1908	1796	0.07%	0.017%
90	12.943	3700	3702	3705	rBV4	1169	405	0.02%	0.004%
91	13.091	3746	3748	3749	rVB2	1057	273	0.01%	0.003%
92	13.130	3758	3760	3762	rBV3	1509	881	0.03%	0.008%
93	13.207	3772	3784	3798	rBV	227063	347312	12.89%	3.216%
94	13.348	3825	3828	3831	rBV5	1245	865	0.03%	0.008%
95	13.512	3878	3879	3883	rVB3	1740	749	0.03%	0.007%
96	13.689	3924	3934	3946	rBV	83793	134140	4.98%	1.242%
97	13.831	3976	3978	3980	rBV2	1179	664	0.02%	0.006%
98	13.908	4000	4002	4004	rBV3	1233	400	0.01%	0.004%
99	14.570	4206	4208	4211	rBV4	1620	1138	0.04%	0.011%
100	14.631	4224	4227	4229	rBV4	2195	1594	0.06%	0.015%




Sum of corrected areas: 10797913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030767.D
Acq On : 21 Apr 2023 16:09
Operator : SY/MD
Sample : 02398-08 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

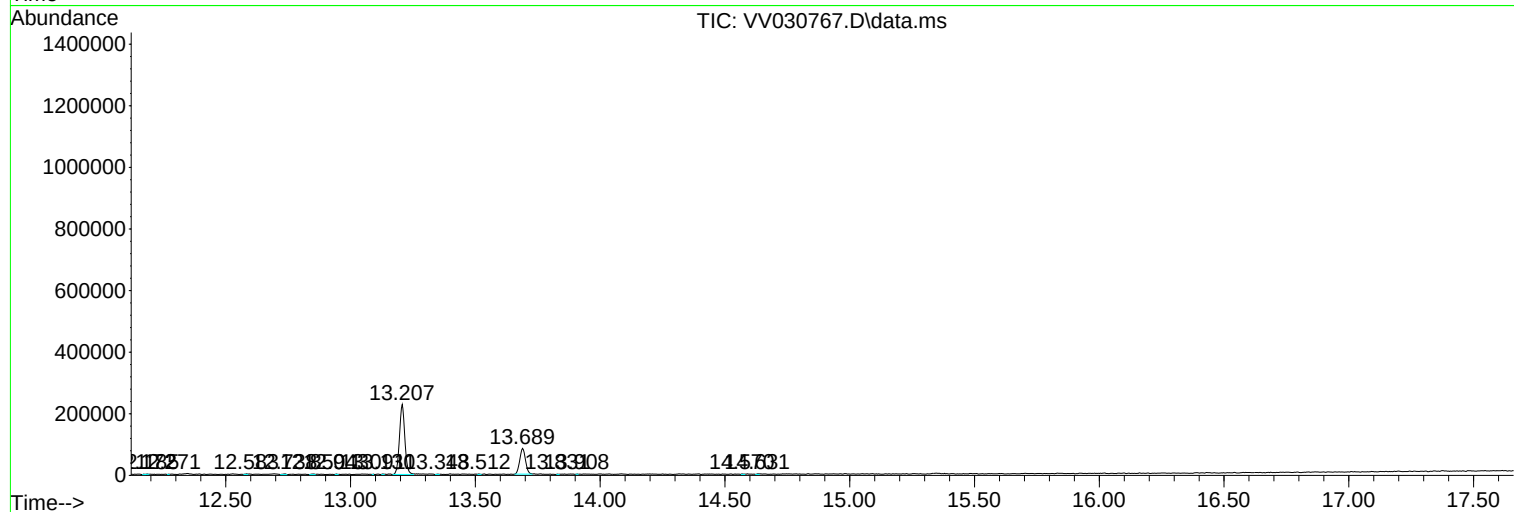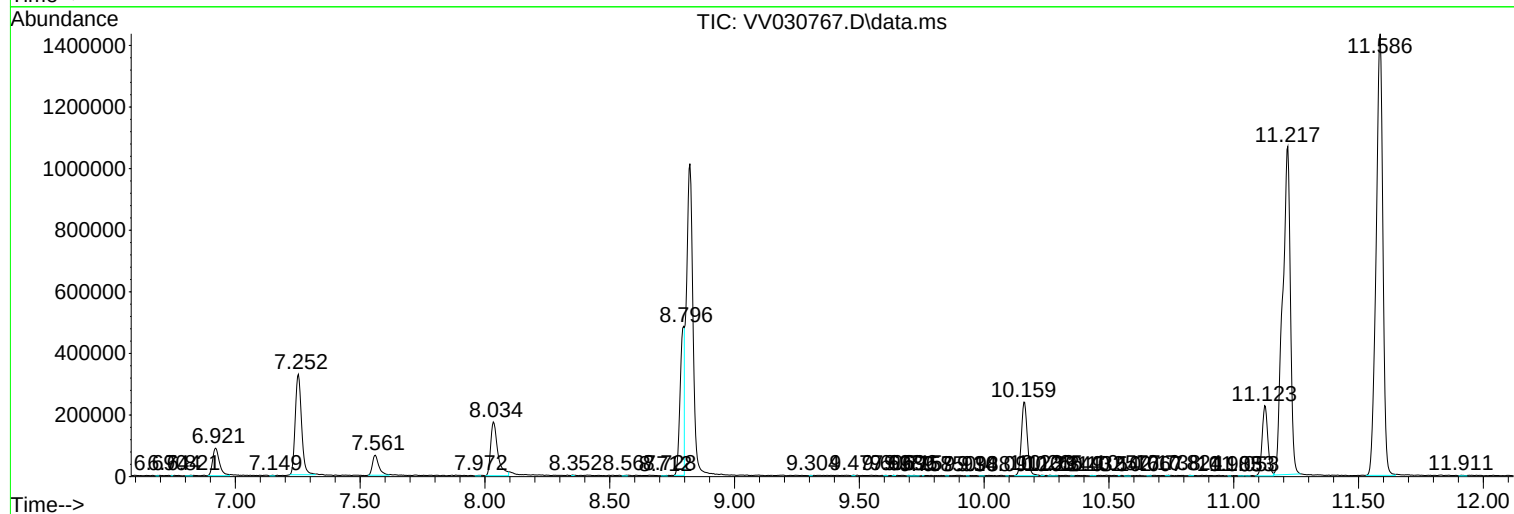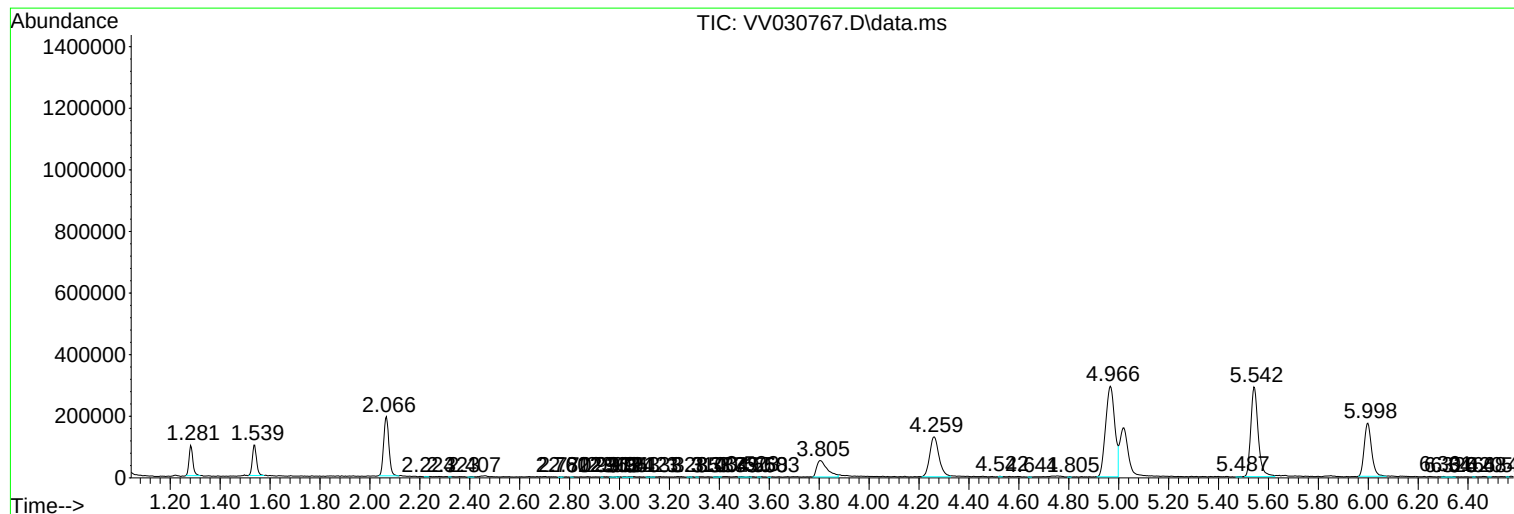

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030767.D
Acq On : 21 Apr 2023 16:09
Operator : SY/MD
Sample : 02398-08 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030767.D
Acq On : 21 Apr 2023 16:09
Operator : SY/MD
Sample : 02398-08 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------