

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030768.D
 Acq On : 21 Apr 2023 16:32
 Operator : SY/MD
 Sample : 02398-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	99616	111369	4.13%	1.005%
2	1.535	148	154	169	rVB	102987	126434	4.69%	1.141%
3	2.066	310	319	333	rVB	196793	285953	10.62%	2.582%
4	2.175	352	353	356	rVB3	2253	673	0.02%	0.006%
5	2.294	386	390	392	rBV4	2034	1428	0.05%	0.013%
6	2.336	401	403	408	rBV6	1301	839	0.03%	0.008%
7	2.584	477	480	482	rBV2	1433	890	0.03%	0.008%
8	2.658	499	503	505	rBV4	1247	719	0.03%	0.006%
9	2.677	505	509	511	rBV4	1463	928	0.03%	0.008%
10	2.889	571	575	578	rBV5	1922	1501	0.06%	0.014%
11	2.960	595	597	602	rVB6	1913	1426	0.05%	0.013%
12	3.018	613	615	620	rVB5	2014	1547	0.06%	0.014%
13	3.114	643	645	647	rVB3	1658	711	0.03%	0.006%
14	3.140	651	653	654	rBV2	1476	699	0.03%	0.006%
15	3.291	698	700	703	rVB4	2150	1136	0.04%	0.010%
16	3.310	703	706	709	rBV4	1289	1007	0.04%	0.009%
17	3.323	709	710	715	rVB4	1521	1107	0.04%	0.010%
18	3.384	724	729	733	rVB7	1779	1654	0.06%	0.015%
19	3.410	733	737	738	rBV4	1106	758	0.03%	0.007%
20	3.458	750	752	756	rBV5	1113	876	0.03%	0.008%
21	3.551	778	781	785	rBV6	1012	928	0.03%	0.008%
22	3.613	796	800	804	rBV6	1713	1316	0.05%	0.012%
23	3.651	810	812	817	rBV6	995	848	0.03%	0.008%
24	3.683	818	822	828	rVB8	2051	2054	0.08%	0.019%
25	3.802	850	859	895	rVV	54557	173520	6.44%	1.567%
26	4.259	985	1001	1026	rVV	132044	340619	12.64%	3.075%
27	4.458	1061	1063	1065	rBV3	1577	746	0.03%	0.007%
28	4.661	1123	1126	1130	rVB4	1472	971	0.04%	0.009%
29	4.789	1164	1166	1170	rBV6	1487	1169	0.04%	0.011%
30	4.879	1192	1194	1197	rBV4	1165	675	0.03%	0.006%
31	4.966	1204	1221	1230	rBV2	303482	787913	29.25%	7.113%
32	5.301	1322	1325	1327	rBV4	1614	1058	0.04%	0.010%
33	5.542	1388	1400	1421	rBV	289800	599602	22.26%	5.413%
34	5.815	1482	1485	1486	rBV3	1616	992	0.04%	0.009%
35	5.998	1527	1542	1562	rBV	178089	375008	13.92%	3.386%
36	6.571	1716	1720	1723	rBV6	2060	2171	0.08%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030768.D
 Acq On : 21 Apr 2023 16:32
 Operator : SY/MD
 Sample : 02398-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.625	1732	1737	1738	rBV5	1527	1111	0.04%	0.010%
38	6.747	1772	1775	1777	rBV4	1434	1016	0.04%	0.009%
39	6.921	1818	1829	1844	rBV	91916	177335	6.58%	1.601%
40	7.088	1879	1881	1884	rBV3	1381	729	0.03%	0.007%
41	7.252	1921	1932	1959	rBV	338918	599728	22.26%	5.414%
42	7.561	2019	2028	2042	rBV2	65629	116504	4.32%	1.052%
43	8.034	2166	2175	2192	rBV2	183706	350655	13.02%	3.166%
44	8.349	2271	2273	2279	rBV5	1834	1896	0.07%	0.017%
45	8.423	2294	2296	2300	rBV5	1595	1043	0.04%	0.009%
46	8.677	2372	2375	2379	rBV6	1317	1076	0.04%	0.010%
47	8.696	2379	2381	2386	rVB4	1001	670	0.02%	0.006%
48	8.821	2399	2420	2444	rBV2	1212405	2693792	100.00%	24.320%
49	9.249	2551	2553	2557	rBV5	1825	1165	0.04%	0.011%
50	9.345	2580	2583	2585	rBV4	1835	1103	0.04%	0.010%
51	9.452	2613	2616	2617	rBV3	1448	911	0.03%	0.008%
52	9.525	2634	2639	2641	rBV5	1923	1864	0.07%	0.017%
53	9.583	2655	2657	2662	rVB5	1494	1192	0.04%	0.011%
54	9.805	2723	2726	2728	rBV3	1591	1175	0.04%	0.011%
55	9.844	2736	2738	2741	rVB3	2162	1271	0.05%	0.011%
56	9.860	2741	2743	2745	rBV3	1147	752	0.03%	0.007%
57	9.947	2765	2770	2772	rBV5	1960	1412	0.05%	0.013%
58	10.037	2794	2798	2799	rBV4	1283	1013	0.04%	0.009%
59	10.095	2814	2816	2821	rBV6	1279	1280	0.05%	0.012%
60	10.117	2821	2823	2826	rVV4	1938	1412	0.05%	0.013%
61	10.159	2826	2836	2859	rVB	249525	401267	14.90%	3.623%
62	10.268	2867	2870	2871	rBV3	1368	675	0.03%	0.006%
63	10.316	2883	2885	2892	rVV7	1231	1286	0.05%	0.012%
64	10.358	2896	2898	2903	rVB6	1662	842	0.03%	0.008%
65	10.413	2913	2915	2922	rVB6	1996	1665	0.06%	0.015%
66	10.538	2950	2954	2958	rVB7	1224	915	0.03%	0.008%
67	10.725	3007	3012	3013	rBV5	1412	1216	0.05%	0.011%
68	10.751	3018	3020	3024	rVB5	1449	1061	0.04%	0.010%
69	10.789	3028	3032	3036	rVV7	1498	1424	0.05%	0.013%
70	10.876	3057	3059	3063	rBV5	1360	1053	0.04%	0.010%
71	10.898	3063	3066	3069	rVB4	2026	1170	0.04%	0.011%
72	10.918	3069	3072	3077	rBV7	1649	1617	0.06%	0.015%
73	10.943	3077	3080	3083	rBV5	1060	868	0.03%	0.008%
74	11.011	3098	3101	3105	rVB5	1258	1094	0.04%	0.010%
75	11.066	3116	3118	3121	rBV4	1367	912	0.03%	0.008%
76	11.127	3127	3137	3147	rBV	51824	83992	3.12%	0.758%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030768.D
 Acq On : 21 Apr 2023 16:32
 Operator : SY/MD
 Sample : 02398-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.217	3148	3165	3188	rVB2	687927	1711618	63.54%	15.453%
78	11.583	3263	3279	3297	rBV2	674525	1486946	55.20%	13.424%
79	12.046	3416	3423	3425	rBV7	1489	1874	0.07%	0.017%
80	12.078	3430	3433	3437	rBV5	1563	1712	0.06%	0.015%
81	12.223	3476	3478	3481	rBV3	1138	792	0.03%	0.007%
82	12.275	3492	3494	3499	rBV5	897	710	0.03%	0.006%
83	12.300	3500	3502	3505	rVV4	1144	724	0.03%	0.007%
84	12.345	3509	3516	3522	rBV4	3134	4927	0.18%	0.044%
85	12.403	3531	3534	3536	rBV4	1218	910	0.03%	0.008%
86	12.464	3551	3553	3557	rVB6	1344	765	0.03%	0.007%
87	12.487	3557	3560	3563	rBV4	1625	1393	0.05%	0.013%
88	12.580	3587	3589	3593	rBV5	1170	681	0.03%	0.006%
89	12.776	3648	3650	3653	rVB4	1389	821	0.03%	0.007%
90	12.815	3660	3662	3666	rBV5	1316	965	0.04%	0.009%
91	13.075	3741	3743	3745	rBV3	1203	706	0.03%	0.006%
92	13.207	3768	3784	3798	rBV	274351	435337	16.16%	3.930%
93	13.384	3836	3839	3841	rBV4	1244	911	0.03%	0.008%
94	13.586	3900	3902	3904	rBV3	1906	968	0.04%	0.009%
95	13.654	3921	3923	3924	rBV2	1524	701	0.03%	0.006%
96	13.689	3924	3934	3947	rVB	78643	124798	4.63%	1.127%
97	13.799	3966	3968	3971	rBV4	1423	954	0.04%	0.009%
98	13.914	4001	4004	4005	rBV4	1300	914	0.03%	0.008%
99	14.262	4108	4112	4118	rBV8	2078	2083	0.08%	0.019%
100	14.647	4229	4232	4235	rBV5	1979	1823	0.07%	0.016%



Sum of corrected areas: 11076440

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030768.D
Acq On : 21 Apr 2023 16:32
Operator : SY/MD
Sample : 02398-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

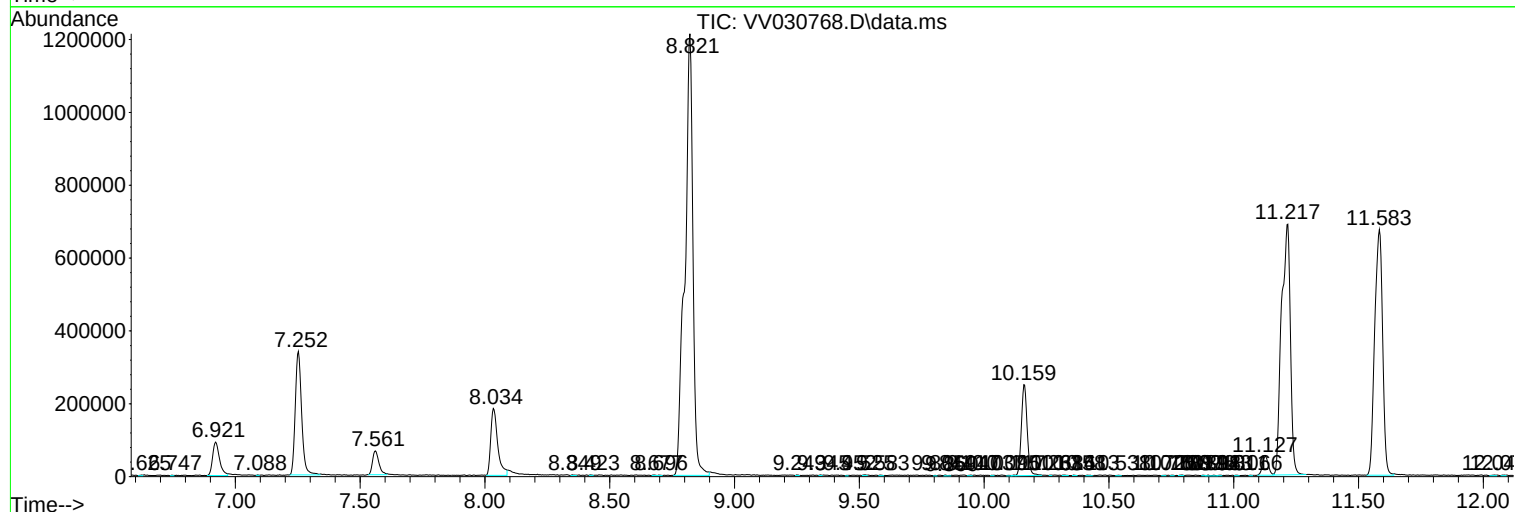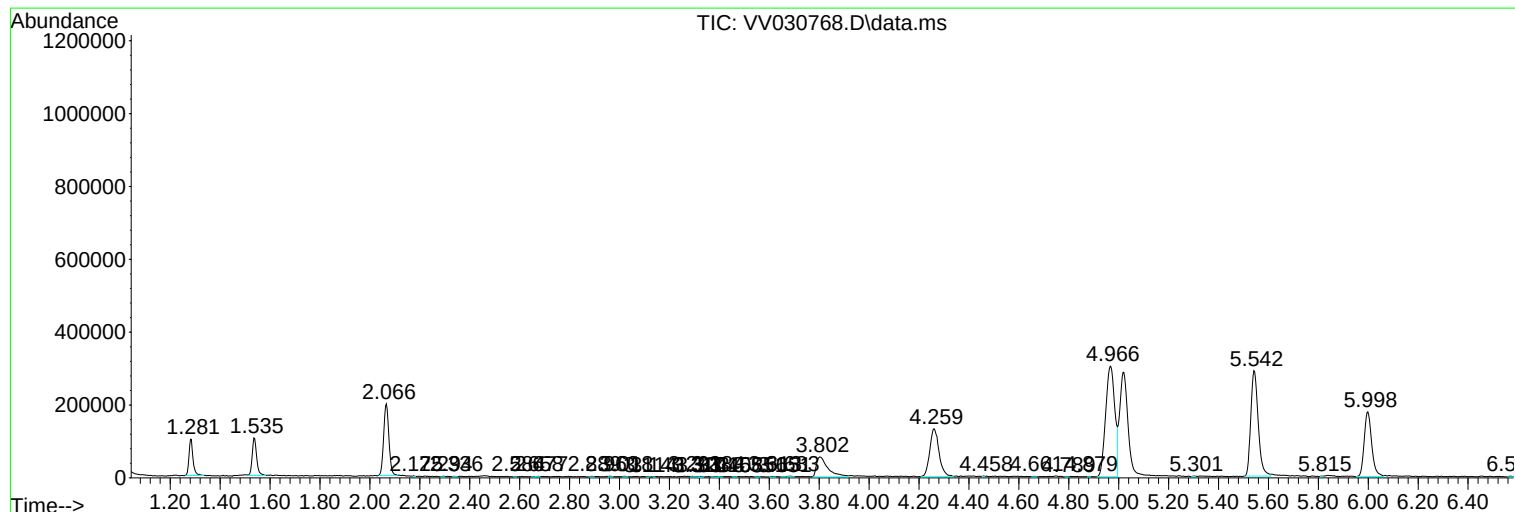

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030768.D
Acq On : 21 Apr 2023 16:32
Operator : SY/MD
Sample : 02398-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030768.D
Acq On : 21 Apr 2023 16:32
Operator : SY/MD
Sample : 02398-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------