

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030770.D
 Acq On : 21 Apr 2023 17:19
 Operator : SY/MD
 Sample : 02398-12DL2 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	105951	115958	10.90%	1.649%
2	1.535	148	154	165	rVB	104823	120786	11.35%	1.718%
3	2.066	310	319	333	rVB	197637	288492	27.11%	4.103%
4	2.294	388	390	394	rBV3	1508	1106	0.10%	0.016%
5	2.436	428	434	436	rBV7	1629	1553	0.15%	0.022%
6	2.532	463	464	466	rBV2	933	423	0.04%	0.006%
7	2.641	494	498	499	rBV4	1197	819	0.08%	0.012%
8	2.677	507	509	511	rBV3	1297	598	0.06%	0.009%
9	2.699	514	516	519	rVB4	1696	657	0.06%	0.009%
10	2.793	542	545	547	rBV3	1415	963	0.09%	0.014%
11	2.841	557	560	561	rBV3	890	372	0.03%	0.005%
12	2.873	568	570	573	rBV4	1176	773	0.07%	0.011%
13	2.963	596	598	601	rBV3	1121	828	0.08%	0.012%
14	2.979	601	603	606	rVV4	907	507	0.05%	0.007%
15	3.050	623	625	628	rBV5	1494	944	0.09%	0.013%
16	3.104	639	642	645	rBV4	1865	1205	0.11%	0.017%
17	3.137	648	652	654	rBV5	1284	1112	0.10%	0.016%
18	3.166	659	661	662	rVB2	1468	423	0.04%	0.006%
19	3.182	662	666	668	rBV4	1263	894	0.08%	0.013%
20	3.281	694	697	699	rBV4	1418	1167	0.11%	0.017%
21	3.339	710	715	718	rBV5	1279	1168	0.11%	0.017%
22	3.391	727	731	733	rBV4	1287	872	0.08%	0.012%
23	3.458	749	752	754	rBV3	1685	1082	0.10%	0.015%
24	3.571	785	787	788	rVB2	1222	372	0.03%	0.005%
25	3.725	830	835	837	rBV5	1954	1749	0.16%	0.025%
26	3.802	850	859	880	rBV	50476	141287	13.28%	2.009%
27	4.149	964	967	969	rVB4	1377	772	0.07%	0.011%
28	4.172	970	974	978	rBV5	1418	1458	0.14%	0.021%
29	4.259	989	1001	1024	rVB	124530	310263	29.16%	4.412%
30	4.815	1172	1174	1177	rBV3	916	727	0.07%	0.010%
31	4.876	1190	1193	1195	rBV3	1089	677	0.06%	0.010%
32	4.892	1195	1198	1203	rVB6	1184	1014	0.10%	0.014%
33	4.966	1203	1221	1230	rBV2	292231	754524	70.91%	10.730%
34	5.439	1366	1368	1372	rVB5	946	590	0.06%	0.008%
35	5.542	1388	1400	1428	rBV	287198	600728	56.45%	8.543%
36	5.998	1531	1542	1561	rBV	167893	339382	31.89%	4.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030770.D
 Acq On : 21 Apr 2023 17:19
 Operator : SY/MD
 Sample : 02398-12DL2 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.339	1645	1648	1650	rBV4	1219	905	0.09%	0.013%
38	6.548	1709	1713	1715	rBV5	1901	1424	0.13%	0.020%
39	6.715	1761	1765	1769	rBV6	1479	1449	0.14%	0.021%
40	6.754	1773	1777	1780	rBV7	1210	786	0.07%	0.011%

41	6.870	1812	1813	1815	rVB3	1326	442	0.04%	0.006%
42	6.921	1816	1829	1852	rVV	87760	173817	16.33%	2.472%
43	7.252	1921	1932	1955	rBV	318690	572032	53.76%	8.135%
44	7.561	2018	2028	2042	rBV	64380	117155	11.01%	1.666%
45	8.034	2166	2175	2192	rBV	164056	321082	30.17%	4.566%

46	8.297	2255	2257	2260	rBV4	1399	720	0.07%	0.010%
47	8.554	2334	2337	2339	rBV3	1083	782	0.07%	0.011%
48	8.603	2350	2352	2355	rBV4	1403	994	0.09%	0.014%
49	8.641	2362	2364	2366	rVB2	1415	635	0.06%	0.009%
50	8.654	2366	2368	2371	rVB4	1949	1075	0.10%	0.015%

51	8.696	2378	2381	2384	rBV4	1335	745	0.07%	0.011%
52	8.741	2391	2395	2397	rBV5	1302	1164	0.11%	0.017%
53	8.792	2401	2411	2414	rBV	472816	653766	61.44%	9.297%
54	9.226	2545	2546	2548	rBV2	1253	617	0.06%	0.009%
55	9.275	2558	2561	2562	rBV3	1433	851	0.08%	0.012%

56	9.313	2570	2573	2577	rBV5	1375	1503	0.14%	0.021%
57	9.413	2602	2604	2608	rBV4	1398	1000	0.09%	0.014%
58	9.561	2646	2650	2652	rBV5	1287	886	0.08%	0.013%
59	9.821	2727	2731	2734	rVB4	1349	910	0.09%	0.013%
60	9.979	2778	2780	2781	rBV2	1755	737	0.07%	0.010%

61	10.162	2826	2837	2858	rVB	237039	382611	35.96%	5.441%
62	10.307	2879	2882	2884	rVB4	1182	583	0.05%	0.008%
63	10.339	2889	2892	2894	rBV3	1233	978	0.09%	0.014%
64	10.381	2903	2905	2909	rBV4	1420	1122	0.11%	0.016%
65	10.442	2922	2924	2925	rBV2	1340	418	0.04%	0.006%

66	10.493	2937	2940	2942	rBV4	1875	1124	0.11%	0.016%
67	10.564	2960	2962	2963	rBV2	1199	457	0.04%	0.006%
68	10.603	2973	2974	2979	rVB5	1567	904	0.08%	0.013%
69	10.628	2979	2982	2984	rBV4	1394	741	0.07%	0.011%
70	10.693	3000	3002	3004	rVV3	1116	576	0.05%	0.008%

71	10.747	3018	3019	3020	rBV	1281	431	0.04%	0.006%
72	10.773	3025	3027	3032	rBV6	1272	1047	0.10%	0.015%
73	10.834	3045	3046	3049	rBV3	1409	634	0.06%	0.009%
74	10.924	3072	3074	3080	rBV5	1486	1129	0.11%	0.016%
75	11.011	3099	3101	3102	rBV2	1211	472	0.04%	0.007%

76	11.059	3113	3116	3117	rBV3	978	546	0.05%	0.008%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030770.D
 Acq On : 21 Apr 2023 17:19
 Operator : SY/MD
 Sample : 02398-12DL2 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP3DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.127	3127	3137	3147	rBV5	12389	23523	2.21%	0.335%
78	11.194	3147	3158	3179	rVV2	451389	1064126	100.00%	15.132%
79	11.493	3246	3251	3255	rBV6	1895	1840	0.17%	0.026%
80	11.516	3255	3258	3260	rVB4	836	553	0.05%	0.008%
81	11.574	3262	3276	3293	rBV2	413556	964818	90.67%	13.720%
82	11.795	3343	3345	3348	rBV4	1664	849	0.08%	0.012%
83	11.866	3365	3367	3369	rBV3	1160	448	0.04%	0.006%
84	11.895	3374	3376	3377	rBV2	841	373	0.04%	0.005%
85	11.975	3399	3401	3403	rBV3	939	636	0.06%	0.009%
86	12.246	3483	3485	3487	rBV3	1473	865	0.08%	0.012%
87	12.365	3520	3522	3526	rVB5	1065	577	0.05%	0.008%
88	12.381	3526	3527	3531	rBV4	1065	682	0.06%	0.010%
89	12.484	3557	3559	3561	rBV3	1720	827	0.08%	0.012%
90	12.738	3635	3638	3640	rBV4	863	389	0.04%	0.006%
91	12.834	3664	3668	3669	rBV3	1608	1132	0.11%	0.016%
92	12.882	3681	3683	3684	rBV2	772	401	0.04%	0.006%
93	13.165	3769	3771	3774	rVB5	1196	619	0.06%	0.009%
94	13.210	3778	3785	3795	rVB4	12474	19626	1.84%	0.279%
95	13.342	3824	3826	3828	rBV3	938	519	0.05%	0.007%
96	13.615	3906	3911	3912	rBV5	1483	1196	0.11%	0.017%
97	13.657	3921	3924	3927	rVB5	1724	1047	0.10%	0.015%
98	13.863	3985	3988	3989	rBV3	1324	724	0.07%	0.010%
99	13.969	4019	4021	4022	rBV2	901	428	0.04%	0.006%
100	14.056	4047	4048	4049	rBV	1321	405	0.04%	0.006%




Sum of corrected areas: 7032098

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030770.D
Acq On : 21 Apr 2023 17:19
Operator : SY/MD
Sample : 02398-12DL2 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

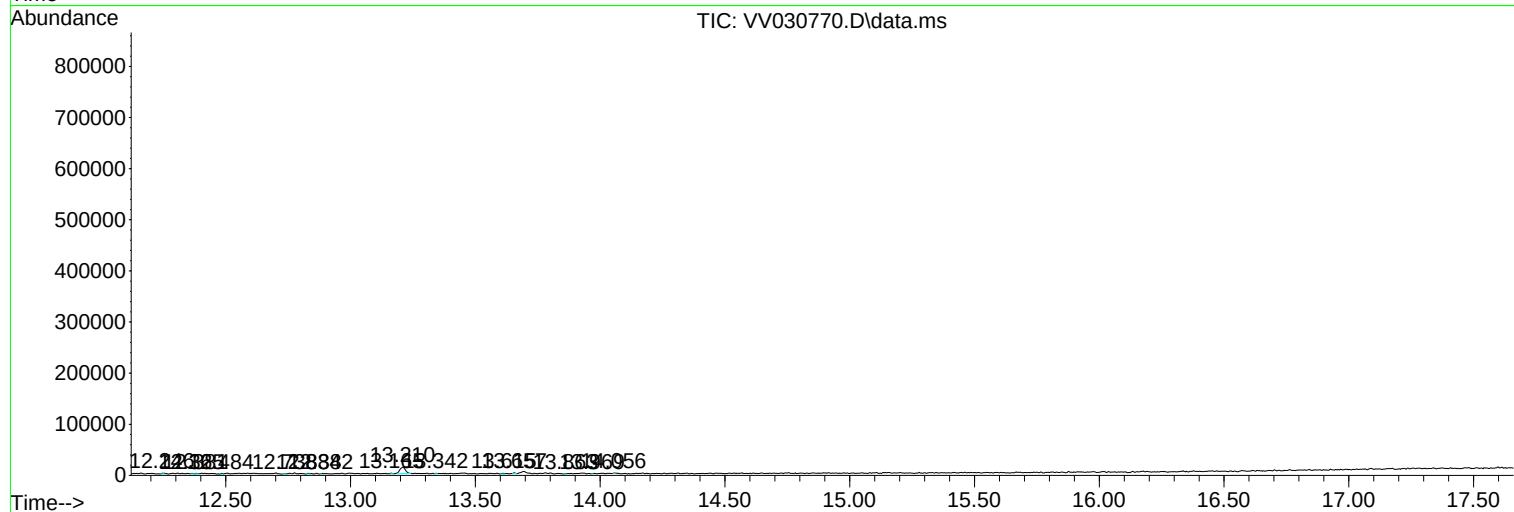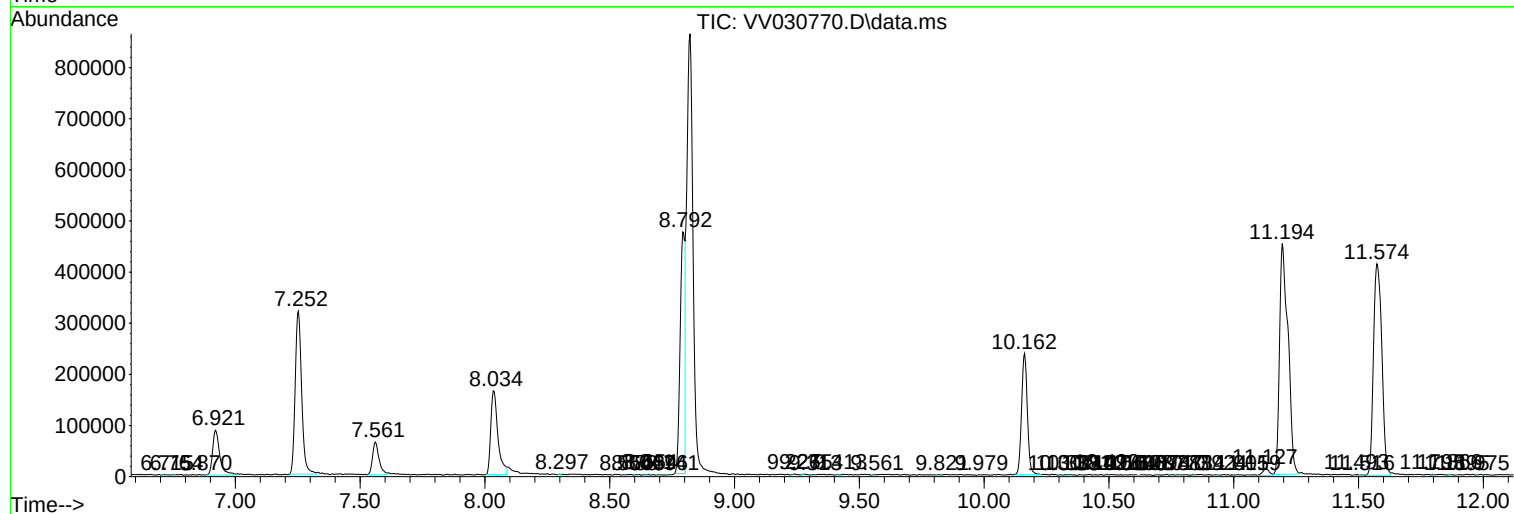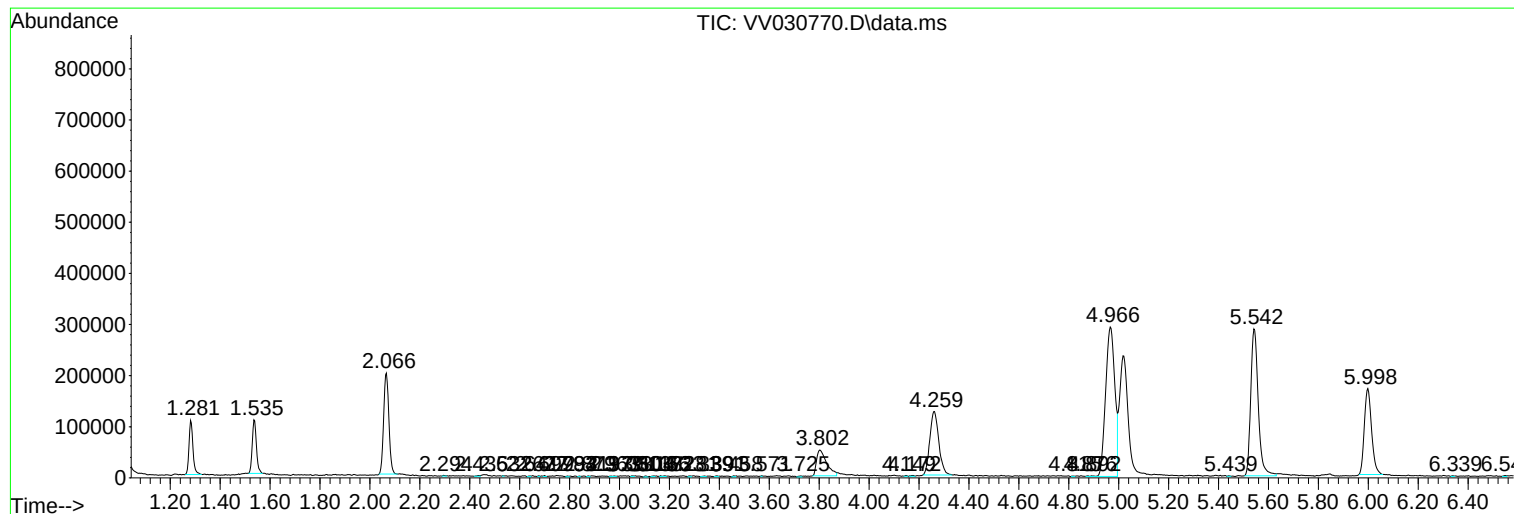

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030770.D
Acq On : 21 Apr 2023 17:19
Operator : SY/MD
Sample : 02398-12DL2 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030770.D
Acq On : 21 Apr 2023 17:19
Operator : SY/MD
Sample : 02398-12DL2 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP3DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------