

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030771.D
 Acq On : 21 Apr 2023 17:43
 Operator : SY/MD
 Sample : 02440-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rBV	99276	107465	13.19%	1.772%
2	1.536	148	154	170	rVB	95749	114193	14.02%	1.883%
3	2.066	309	319	332	rBV	190026	282204	34.64%	4.653%
4	2.597	479	484	486	rBV5	1255	1007	0.12%	0.017%
5	2.696	513	515	521	rVB6	1751	1442	0.18%	0.024%
6	2.725	521	524	525	rBV2	1458	780	0.10%	0.013%
7	2.806	548	549	553	rBV4	967	522	0.06%	0.009%
8	2.854	561	564	567	rBV5	764	575	0.07%	0.009%
9	2.896	573	577	580	rBV5	1695	1370	0.17%	0.023%
10	2.963	595	598	600	rBV4	1285	905	0.11%	0.015%
11	3.188	666	668	671	rBV4	1117	530	0.07%	0.009%
12	3.227	678	680	684	rVB5	1852	1182	0.15%	0.019%
13	3.298	697	702	704	rBV7	1416	1540	0.19%	0.025%
14	3.439	743	746	749	rBV5	1180	983	0.12%	0.016%
15	3.484	755	760	763	rBV7	1407	1211	0.15%	0.020%
16	3.526	769	773	775	rBV5	1055	735	0.09%	0.012%
17	3.632	803	806	808	rBV4	1152	910	0.11%	0.015%
18	3.802	850	859	884	rBV2	43785	128879	15.82%	2.125%
19	4.085	945	947	951	rVB4	1870	994	0.12%	0.016%
20	4.259	982	1001	1025	rBV	120398	315539	38.73%	5.203%
21	4.510	1076	1079	1081	rBV3	1359	889	0.11%	0.015%
22	4.542	1087	1089	1092	rVB4	1486	763	0.09%	0.013%
23	4.564	1092	1096	1097	rBV4	1693	1096	0.13%	0.018%
24	4.674	1126	1130	1132	rBV5	1738	1255	0.15%	0.021%
25	4.703	1137	1139	1143	rBV3	1106	842	0.10%	0.014%
26	4.966	1203	1221	1257	rBV2	273945	814739	100.00%	13.434%
27	5.352	1339	1341	1345	rBV5	1369	988	0.12%	0.016%
28	5.542	1386	1400	1420	rBV	233582	491661	60.35%	8.107%
29	5.998	1530	1542	1560	rBV	160294	324659	39.85%	5.353%
30	6.388	1658	1663	1665	rBV6	1240	1033	0.13%	0.017%
31	6.455	1682	1684	1690	rVB6	1798	1469	0.18%	0.024%
32	6.590	1720	1726	1732	rBV10	2233	2769	0.34%	0.046%
33	6.857	1802	1809	1810	rBV7	1550	1429	0.18%	0.024%
34	6.921	1819	1829	1845	rBV	81051	151306	18.57%	2.495%
35	7.252	1919	1932	1953	rBV	303042	547208	67.16%	9.023%
36	7.561	2019	2028	2040	rBV	60176	103381	12.69%	1.705%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030771.D
 Acq On : 21 Apr 2023 17:43
 Operator : SY/MD
 Sample : 02440-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.760	2087	2090	2092	rBV4	1594	1038	0.13%	0.017%
38	8.034	2166	2175	2212	rBV	146353	307816	37.78%	5.076%
39	8.423	2293	2296	2299	rBV5	1361	910	0.11%	0.015%
40	8.596	2345	2350	2352	rBV6	1403	1206	0.15%	0.020%
41	8.661	2367	2370	2373	rBV5	1151	946	0.12%	0.016%
42	8.699	2381	2382	2385	rVB3	1312	653	0.08%	0.011%
43	8.719	2385	2388	2393	rVB5	752	585	0.07%	0.010%
44	8.741	2393	2395	2397	rBV2	1502	736	0.09%	0.012%
45	8.796	2400	2412	2413	rBV	391922	478783	58.77%	7.895%
46	9.294	2565	2567	2570	rBV4	936	608	0.07%	0.010%
47	9.355	2583	2586	2589	rBV4	1942	1433	0.18%	0.024%
48	9.384	2591	2595	2596	rBV4	1024	689	0.08%	0.011%
49	9.619	2664	2668	2670	rBV4	1745	1316	0.16%	0.022%
50	9.751	2706	2709	2712	rVB5	1209	813	0.10%	0.013%
51	9.770	2712	2715	2721	rBV8	1820	1822	0.22%	0.030%
52	9.831	2732	2734	2739	rVB7	1322	760	0.09%	0.013%
53	9.899	2753	2755	2758	rVV4	918	533	0.07%	0.009%
54	9.924	2758	2763	2765	rVV6	1341	1060	0.13%	0.017%
55	10.002	2784	2787	2790	rBV5	752	591	0.07%	0.010%
56	10.159	2826	2836	2851	rBV	222254	357112	43.83%	5.888%
57	10.455	2926	2928	2930	rVB3	1886	788	0.10%	0.013%
58	10.603	2971	2974	2975	rBV3	987	559	0.07%	0.009%
59	10.651	2987	2989	2991	rBV3	876	532	0.07%	0.009%
60	10.728	3011	3013	3016	rBV4	1381	879	0.11%	0.014%
61	10.879	3056	3060	3062	rBV5	1766	1353	0.17%	0.022%
62	11.127	3126	3137	3147	rBV	89488	142371	17.47%	2.348%
63	11.194	3148	3158	3161	rBV	395275	557572	68.44%	9.194%
64	11.432	3229	3232	3233	rBV3	1222	762	0.09%	0.013%
65	11.571	3264	3275	3297	rVB2	354862	674669	82.81%	11.124%
66	11.699	3313	3315	3318	rBV5	1175	656	0.08%	0.011%
67	11.780	3338	3340	3344	rBV4	1552	1187	0.15%	0.020%
68	11.931	3385	3387	3388	rBV2	1586	583	0.07%	0.010%
69	11.940	3388	3390	3394	rVB5	1473	653	0.08%	0.011%
70	11.995	3404	3407	3411	rBV6	1253	744	0.09%	0.012%
71	12.053	3421	3425	3428	rBV5	960	948	0.12%	0.016%
72	12.124	3445	3447	3449	rBV3	1204	626	0.08%	0.010%
73	12.169	3456	3461	3464	rBV7	1558	1565	0.19%	0.026%
74	12.294	3498	3500	3503	rBV3	1254	1015	0.12%	0.017%
75	12.503	3562	3565	3567	rBV4	1358	907	0.11%	0.015%
76	12.583	3587	3590	3592	rBV4	1165	746	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030771.D
 Acq On : 21 Apr 2023 17:43
 Operator : SY/MD
 Sample : 02440-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.638	3605	3607	3611	rVB4	1327	732	0.09%	0.012%
78	12.664	3611	3615	3618	rBV6	1332	1059	0.13%	0.017%
79	12.760	3643	3645	3646	rBV2	1157	522	0.06%	0.009%
80	12.789	3651	3654	3660	rVB8	1608	1808	0.22%	0.030%
81	12.866	3676	3678	3679	rBV2	1825	778	0.10%	0.013%
82	12.989	3714	3716	3718	rBV2	1070	564	0.07%	0.009%
83	13.056	3734	3737	3738	rBV2	1225	658	0.08%	0.011%
84	13.133	3757	3761	3762	rVV4	1116	671	0.08%	0.011%
85	13.207	3775	3784	3800	rVB	47353	78679	9.66%	1.297%
86	13.272	3800	3804	3805	rBV4	956	684	0.08%	0.011%
87	13.345	3824	3827	3830	rBV3	1228	796	0.10%	0.013%
88	13.371	3832	3835	3839	rBV6	1670	1144	0.14%	0.019%
89	13.445	3856	3858	3860	rBV2	1328	711	0.09%	0.012%
90	13.497	3870	3874	3877	rBV6	1271	1033	0.13%	0.017%
91	13.516	3879	3880	3885	rVB5	1069	602	0.07%	0.010%
92	13.644	3916	3920	3921	rBV3	1307	983	0.12%	0.016%
93	13.689	3929	3934	3943	rVB8	7594	10294	1.26%	0.170%
94	13.799	3966	3968	3972	rBV5	1225	860	0.11%	0.014%
95	13.870	3989	3990	3993	rVB3	1559	671	0.08%	0.011%
96	13.886	3993	3995	3997	rBV2	1160	618	0.08%	0.010%
97	14.220	4097	4099	4104	rVB5	1661	1376	0.17%	0.023%
98	14.246	4104	4107	4108	rBV3	1541	817	0.10%	0.013%
99	14.670	4237	4239	4242	rBV3	1220	726	0.09%	0.012%
100	15.204	4402	4405	4407	rBV4	1452	952	0.12%	0.016%




Sum of corrected areas: 6064716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030771.D
Acq On : 21 Apr 2023 17:43
Operator : SY/MD
Sample : 02440-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

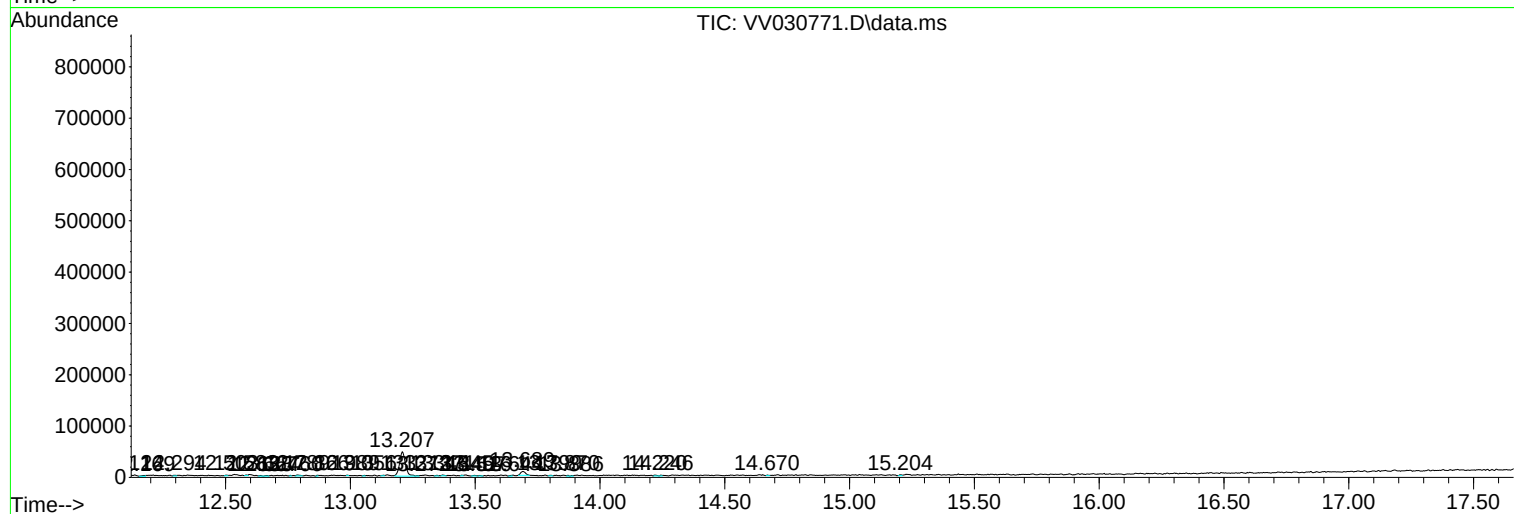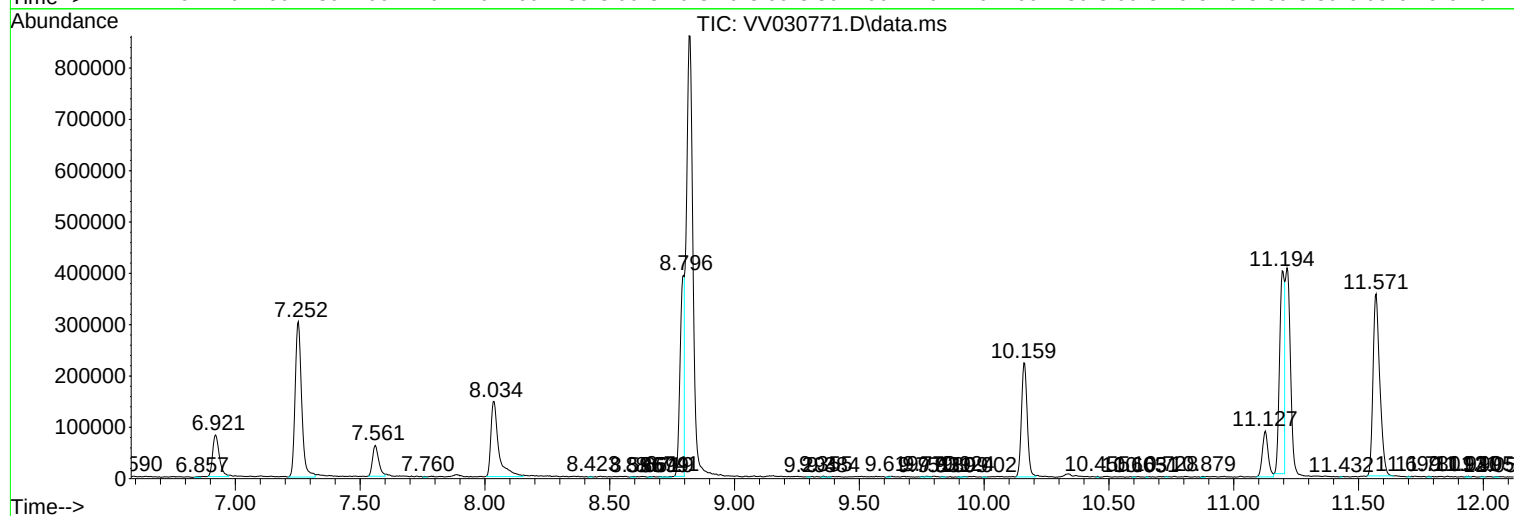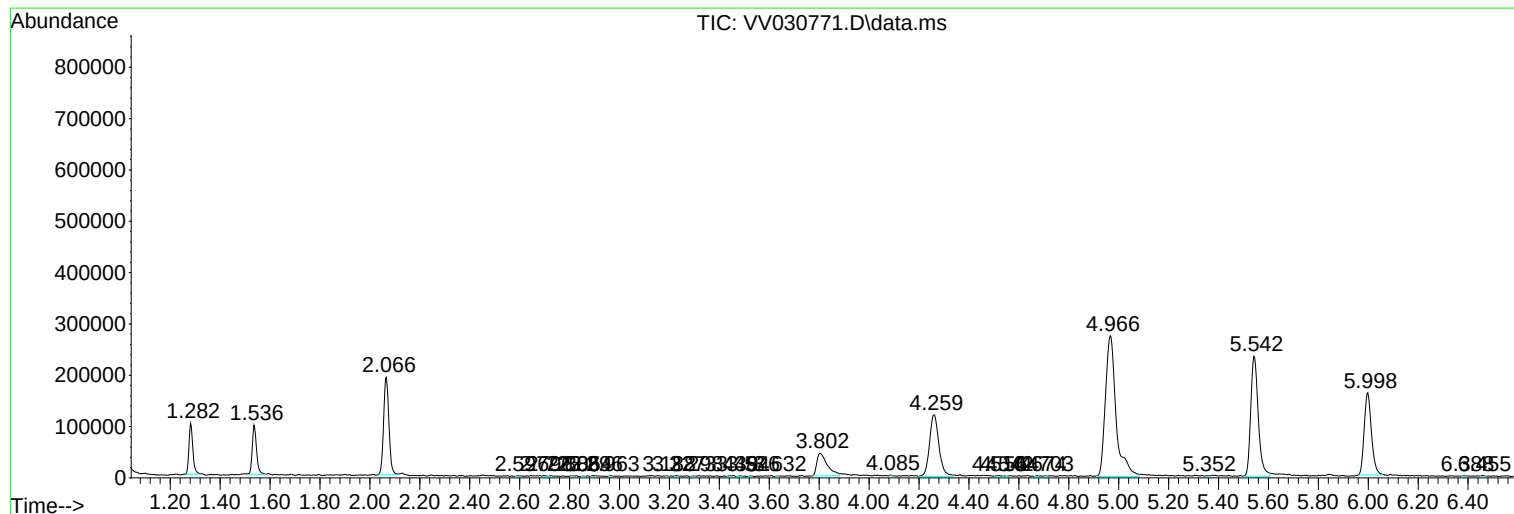

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030771.D
Acq On : 21 Apr 2023 17:43
Operator : SY/MD
Sample : 02440-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030771.D
Acq On : 21 Apr 2023 17:43
Operator : SY/MD
Sample : 02440-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------