

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030773.D
 Acq On : 21 Apr 2023 18:31
 Operator : SY/MD
 Sample : 02440-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rVB	98424	105833	13.83%	1.672%
2	1.535	148	154	167	rVB	101300	118721	15.51%	1.875%
3	2.066	309	319	335	rBV	193259	288185	37.66%	4.552%
4	2.317	393	397	401	rBV6	2100	2185	0.29%	0.035%
5	2.342	404	405	410	rVV5	2125	1201	0.16%	0.019%
6	2.375	410	415	421	rVB8	1769	1980	0.26%	0.031%
7	2.407	421	425	431	rBV9	2085	2249	0.29%	0.036%
8	2.452	436	439	441	rBV3	2101	1185	0.15%	0.019%
9	2.481	446	448	453	rVB5	1522	1183	0.15%	0.019%
10	2.564	470	474	478	rVB6	1326	896	0.12%	0.014%
11	2.786	540	543	546	rBV4	1775	1188	0.16%	0.019%
12	2.857	562	565	568	rBV4	1319	928	0.12%	0.015%
13	2.899	575	578	579	rVB4	1799	815	0.11%	0.013%
14	2.982	600	604	605	rBV4	1154	815	0.11%	0.013%
15	3.014	610	614	616	rBV4	1318	856	0.11%	0.014%
16	3.178	662	665	668	rBV4	983	684	0.09%	0.011%
17	3.201	668	672	675	rBV5	854	633	0.08%	0.010%
18	3.307	702	705	708	rBB5	1201	822	0.11%	0.013%
19	3.423	739	741	745	rVB5	1928	1246	0.16%	0.020%
20	3.442	745	747	749	rBV3	1168	707	0.09%	0.011%
21	3.690	820	824	828	rVB6	1430	1300	0.17%	0.021%
22	3.725	828	835	838	rBV6	1530	2236	0.29%	0.035%
23	3.802	850	859	884	rBV	50574	143293	18.72%	2.263%
24	4.259	988	1001	1019	rBV	123053	306462	40.05%	4.841%
25	4.461	1060	1064	1071	rVB8	1482	1634	0.21%	0.026%
26	4.494	1071	1074	1077	rBV5	1356	935	0.12%	0.015%
27	4.561	1092	1095	1097	rBV4	1393	1073	0.14%	0.017%
28	4.677	1128	1131	1132	rBV2	1143	638	0.08%	0.010%
29	4.844	1179	1183	1186	rBV6	1142	1011	0.13%	0.016%
30	4.966	1204	1221	1246	rBV3	288630	765289	100.00%	12.088%
31	5.227	1301	1302	1307	rBV5	1643	794	0.10%	0.013%
32	5.542	1388	1400	1429	rBV	283065	602061	78.67%	9.510%
33	5.895	1508	1510	1513	rBV4	1595	1104	0.14%	0.017%
34	5.998	1530	1542	1566	rBV	172433	351770	45.97%	5.556%
35	6.236	1614	1616	1620	rBV5	1081	613	0.08%	0.010%
36	6.497	1693	1697	1700	rBV6	1436	1227	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030773.D
 Acq On : 21 Apr 2023 18:31
 Operator : SY/MD
 Sample : 02440-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.677	1750	1753	1756	rVB4	1319	775	0.10%	0.012%
38	6.696	1756	1759	1761	rBV4	1356	950	0.12%	0.015%
39	6.921	1819	1829	1847	rBV	84116	160131	20.92%	2.529%
40	7.072	1874	1876	1880	rBV4	1574	892	0.12%	0.014%
41	7.098	1880	1884	1886	rBV4	1435	942	0.12%	0.015%
42	7.252	1920	1932	1954	rBV	325713	575328	75.18%	9.088%
43	7.561	2019	2028	2045	rBV	61746	110372	14.42%	1.743%
44	7.812	2103	2106	2109	rBV4	1578	908	0.12%	0.014%
45	8.034	2166	2175	2207	rBV	162657	343611	44.90%	5.428%
46	8.452	2303	2305	2308	rBV4	1055	614	0.08%	0.010%
47	8.519	2323	2326	2329	rBV5	1479	1383	0.18%	0.022%
48	8.699	2378	2382	2384	rBV5	1469	1262	0.16%	0.020%
49	8.792	2400	2411	2431	rBV	439500	727389	95.05%	11.490%
50	9.152	2520	2523	2527	rBV5	1442	1247	0.16%	0.020%
51	9.246	2548	2552	2554	rBV5	1694	916	0.12%	0.014%
52	9.368	2588	2590	2593	rBV4	1389	1042	0.14%	0.016%
53	9.384	2593	2595	2600	rVB4	1319	854	0.11%	0.013%
54	9.603	2661	2663	2666	rBV3	983	663	0.09%	0.010%
55	9.638	2672	2674	2679	rBV6	1348	1328	0.17%	0.021%
56	9.918	2758	2761	2763	rBV3	1665	907	0.12%	0.014%
57	10.072	2807	2809	2811	rBV3	1462	845	0.11%	0.013%
58	10.162	2826	2837	2854	rBV	235483	374926	48.99%	5.922%
59	10.307	2878	2882	2884	rBV4	1439	1223	0.16%	0.019%
60	10.390	2904	2908	2910	rBV5	1343	856	0.11%	0.014%
61	10.439	2919	2923	2924	rBV4	1436	833	0.11%	0.013%
62	10.535	2946	2953	2955	rBV7	1769	1759	0.23%	0.028%
63	10.644	2982	2987	2990	rBV5	1994	1674	0.22%	0.026%
64	10.686	2998	3000	3005	rVB5	1377	922	0.12%	0.015%
65	10.799	3033	3035	3041	rVB5	1598	1319	0.17%	0.021%
66	10.834	3041	3046	3047	rBV4	1236	1033	0.13%	0.016%
67	10.918	3067	3072	3077	rBV6	1324	1408	0.18%	0.022%
68	11.101	3125	3129	3130	rBV3	1517	949	0.12%	0.015%
69	11.194	3147	3158	3176	rBV	421257	665970	87.02%	10.519%
70	11.567	3264	3274	3289	rBV	331370	542437	70.88%	8.568%
71	11.863	3363	3366	3368	rBV2	1889	1181	0.15%	0.019%
72	12.008	3409	3411	3414	rVB3	1935	885	0.12%	0.014%
73	12.030	3414	3418	3422	rBV7	1014	943	0.12%	0.015%
74	12.123	3444	3447	3450	rBV4	1835	1089	0.14%	0.017%
75	12.213	3471	3475	3480	rBV7	1110	1119	0.15%	0.018%
76	12.326	3507	3510	3514	rBV6	1514	1324	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030773.D
 Acq On : 21 Apr 2023 18:31
 Operator : SY/MD
 Sample : 02440-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.397	3530	3532	3535	rBV4	1369	1083	0.14%	0.017%
78	12.574	3584	3587	3589	rBV4	1951	1323	0.17%	0.021%
79	12.586	3589	3591	3592	rBV2	1784	795	0.10%	0.013%
80	12.715	3628	3631	3633	rBV3	1142	747	0.10%	0.012%
81	12.863	3675	3677	3680	rBV3	1362	958	0.13%	0.015%
82	12.914	3691	3693	3697	rVB5	1212	676	0.09%	0.011%
83	13.024	3725	3727	3729	rBV3	1405	637	0.08%	0.010%
84	13.072	3739	3742	3747	rBV6	1310	1349	0.18%	0.021%
85	13.210	3776	3785	3795	rBV3	29415	45846	5.99%	0.724%
86	13.326	3819	3821	3823	rBV3	1230	712	0.09%	0.011%
87	13.384	3837	3839	3844	rVB5	2123	1165	0.15%	0.018%
88	13.410	3844	3847	3849	rBV4	1795	1020	0.13%	0.016%
89	13.500	3871	3875	3877	rBV4	1768	1335	0.17%	0.021%
90	13.567	3893	3896	3898	rBV4	1636	891	0.12%	0.014%
91	13.638	3913	3918	3920	rBV4	1643	1311	0.17%	0.021%
92	13.693	3925	3935	3943	rVV6	9230	14946	1.95%	0.236%
93	13.789	3959	3965	3968	rBV7	1844	1983	0.26%	0.031%
94	13.824	3974	3976	3979	rBV4	1068	720	0.09%	0.011%
95	13.979	4021	4024	4026	rBV4	1083	620	0.08%	0.010%
96	14.033	4039	4041	4044	rVB4	1974	1077	0.14%	0.017%
97	14.207	4092	4095	4098	rBV5	1813	1337	0.17%	0.021%
98	14.464	4173	4175	4178	rBV4	1396	843	0.11%	0.013%
99	14.548	4199	4201	4203	rBV3	1485	745	0.10%	0.012%
100	14.615	4219	4222	4223	rBV3	1599	744	0.10%	0.012%




Sum of corrected areas: 6330824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030773.D
Acq On : 21 Apr 2023 18:31
Operator : SY/MD
Sample : 02440-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

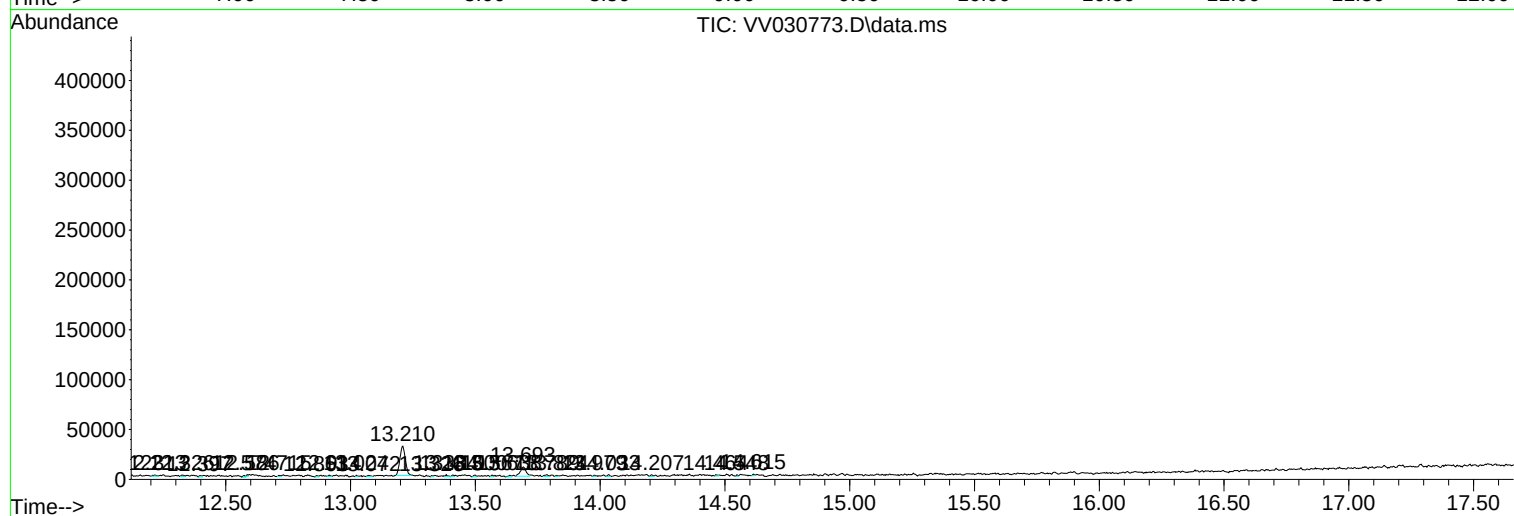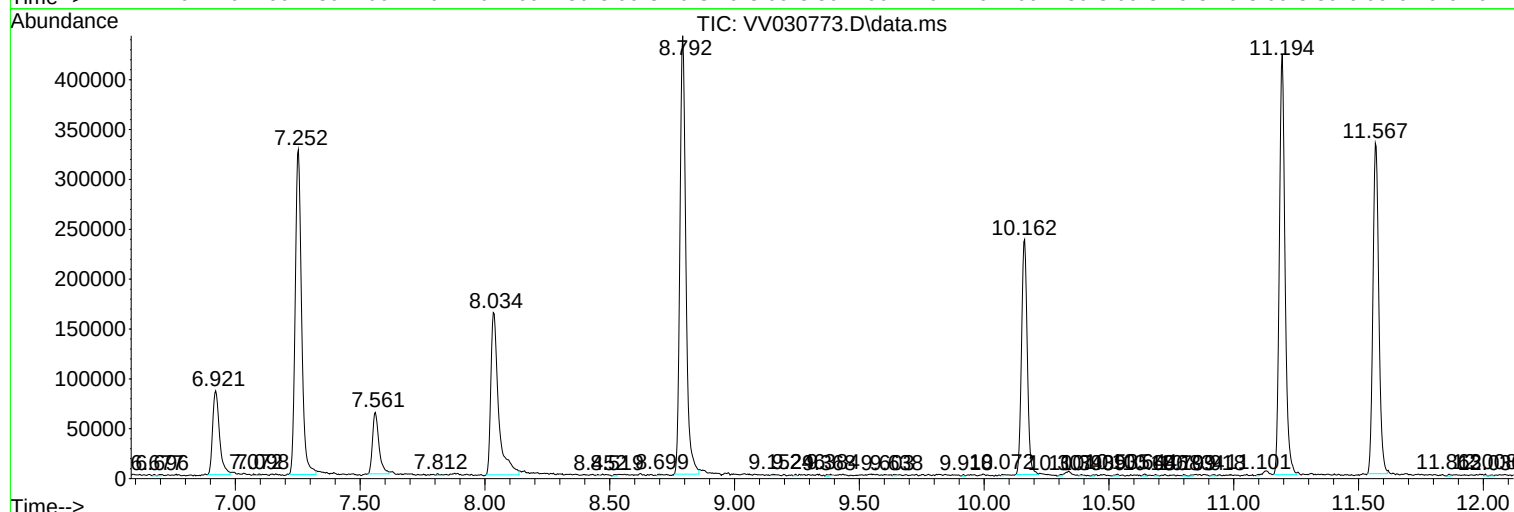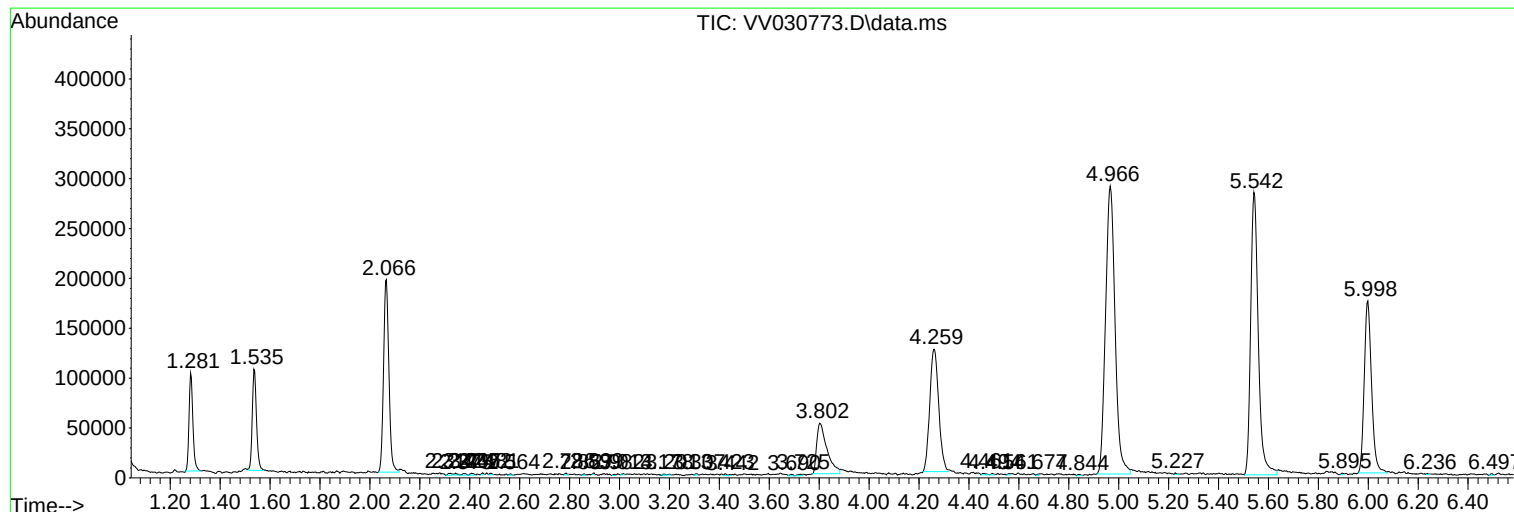

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030773.D
Acq On : 21 Apr 2023 18:31
Operator : SY/MD
Sample : 02440-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030773.D
Acq On : 21 Apr 2023 18:31
Operator : SY/MD
Sample : 02440-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc