

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030774.D
 Acq On : 21 Apr 2023 18:54
 Operator : SY/MD
 Sample : 02440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030774.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	94476	104493	14.08%	1.741%
2	1.536	148	154	168	rVB	97294	117099	15.77%	1.951%
3	2.066	309	319	332	rBV	184704	275902	37.17%	4.597%
4	2.246	371	375	377	rBV3	1903	1248	0.17%	0.021%
5	2.757	531	534	536	rBV4	1652	951	0.13%	0.016%
6	2.809	548	550	554	rBV4	753	527	0.07%	0.009%
7	2.828	554	556	557	rVV	1230	563	0.08%	0.009%
8	2.854	561	564	569	rBV7	1360	1281	0.17%	0.021%
9	2.909	579	581	584	rBV4	1243	811	0.11%	0.014%
10	2.928	584	587	588	rBV3	1341	652	0.09%	0.011%
11	3.021	615	616	619	rBV3	1471	559	0.08%	0.009%
12	3.089	633	637	642	rBV6	1435	1282	0.17%	0.021%
13	3.195	665	670	673	rBV7	1639	1613	0.22%	0.027%
14	3.490	759	762	764	rBV3	1040	535	0.07%	0.009%
15	3.548	777	780	781	rBV3	776	491	0.07%	0.008%
16	3.587	789	792	795	rBV3	1795	1624	0.22%	0.027%
17	3.677	816	820	824	rBV7	1865	1626	0.22%	0.027%
18	3.699	825	827	830	rVB4	1022	526	0.07%	0.009%
19	3.725	832	835	838	rBV5	1519	1209	0.16%	0.020%
20	3.761	844	846	847	rBV2	1447	572	0.08%	0.010%
21	3.802	850	859	882	rBV	49322	140909	18.98%	2.348%
22	4.056	936	938	940	rBV3	1206	574	0.08%	0.010%
23	4.259	989	1001	1023	rVB	120642	301990	40.68%	5.031%
24	4.613	1106	1111	1114	rBV6	1966	1484	0.20%	0.025%
25	4.812	1171	1173	1174	rBV2	1184	617	0.08%	0.010%
26	4.902	1197	1201	1205	rBV7	1188	1373	0.18%	0.023%
27	4.966	1205	1221	1252	rVV3	277044	742366	100.00%	12.368%
28	5.291	1319	1322	1325	rBV5	1317	703	0.09%	0.012%
29	5.400	1354	1356	1358	rBV3	1501	714	0.10%	0.012%
30	5.542	1388	1400	1423	rBV	257359	535793	72.17%	8.927%
31	5.998	1530	1542	1559	rBV	162085	331925	44.71%	5.530%
32	6.394	1663	1665	1668	rBV4	905	522	0.07%	0.009%
33	6.452	1681	1683	1686	rVB3	1734	808	0.11%	0.013%
34	6.471	1686	1689	1690	rBV2	1386	764	0.10%	0.013%
35	6.490	1693	1695	1699	rVV5	1204	847	0.11%	0.014%
36	6.645	1742	1743	1745	rBV2	1294	492	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042123\
 Data File : VW030774.D
 Acq On : 21 Apr 2023 18:54
 Operator : SY/MD
 Sample : 02440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.754	1776	1777	1779	rVB2	1503	507	0.07%	0.008%
38	6.783	1782	1786	1789	rBV4	1566	1086	0.15%	0.018%
39	6.883	1814	1817	1818	rBV3	1384	589	0.08%	0.010%
40	6.921	1818	1829	1852	rVV2	82257	163297	22.00%	2.721%
41	7.252	1921	1932	1951	rBV	308752	541468	72.94%	9.021%
42	7.561	2019	2028	2046	rBV2	58705	104434	14.07%	1.740%
43	7.809	2103	2105	2106	rBV2	1353	601	0.08%	0.010%
44	7.876	2121	2126	2127	rBV4	1566	1131	0.15%	0.019%
45	7.966	2150	2154	2156	rBV5	1182	1080	0.15%	0.018%
46	8.037	2166	2176	2203	rBV	151020	320624	43.19%	5.342%
47	8.577	2340	2344	2348	rBV5	2229	1897	0.26%	0.032%
48	8.793	2399	2411	2437	rBV	397094	682448	91.93%	11.370%
49	8.995	2472	2474	2476	rVB3	1716	603	0.08%	0.010%
50	9.371	2589	2591	2594	rBV4	1013	550	0.07%	0.009%
51	9.407	2599	2602	2607	rBV7	1467	1644	0.22%	0.027%
52	9.487	2623	2627	2628	rBV3	1308	811	0.11%	0.014%
53	9.529	2638	2640	2642	rVB3	1336	550	0.07%	0.009%
54	9.606	2659	2664	2666	rVB5	1398	1108	0.15%	0.018%
55	9.635	2666	2673	2676	rBV6	1571	2203	0.30%	0.037%
56	9.744	2702	2707	2712	rBV7	1048	1141	0.15%	0.019%
57	9.947	2767	2770	2771	rBV3	1997	1066	0.14%	0.018%
58	9.979	2776	2780	2783	rBV5	1931	1250	0.17%	0.021%
59	10.001	2783	2787	2788	rBV3	1497	1025	0.14%	0.017%
60	10.098	2814	2817	2819	rBV4	1243	993	0.13%	0.017%
61	10.159	2825	2836	2856	rVB	224348	364567	49.11%	6.074%
62	10.320	2883	2886	2887	rBV2	2355	1311	0.18%	0.022%
63	10.394	2907	2909	2912	rVB3	940	484	0.07%	0.008%
64	10.419	2912	2917	2920	rBV6	1477	1470	0.20%	0.024%
65	10.645	2985	2987	2988	rBV	1158	581	0.08%	0.010%
66	10.789	3029	3032	3033	rBV3	1279	657	0.09%	0.011%
67	10.860	3047	3054	3055	rBV6	1484	1283	0.17%	0.021%
68	11.114	3131	3133	3135	rBV2	2183	1296	0.17%	0.022%
69	11.194	3146	3158	3179	rBV	379813	617380	83.16%	10.286%
70	11.323	3194	3198	3201	rBV6	1799	1560	0.21%	0.026%
71	11.426	3228	3230	3232	rBV3	1242	623	0.08%	0.010%
72	11.461	3235	3241	3245	rBV9	1138	1313	0.18%	0.022%
73	11.509	3250	3256	3258	rBV6	2425	2427	0.33%	0.040%
74	11.567	3264	3274	3294	rVB	319022	526492	70.92%	8.772%
75	11.792	3342	3344	3347	rBV4	1472	893	0.12%	0.015%
76	11.866	3366	3367	3369	rBV2	1475	554	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030774.D
 Acq On : 21 Apr 2023 18:54
 Operator : SY/MD
 Sample : 02440-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.960	3393	3396	3398	rBV5	1775	986	0.13%	0.016%
78	11.989	3403	3405	3408	rBV4	1548	937	0.13%	0.016%
79	12.088	3434	3436	3440	rBV4	1406	754	0.10%	0.013%
80	12.104	3440	3441	3445	rVB3	1237	629	0.08%	0.010%
81	12.210	3472	3474	3479	rBV6	1013	787	0.11%	0.013%
82	12.255	3484	3488	3489	rBV4	1385	876	0.12%	0.015%
83	12.336	3511	3513	3516	rVB4	1781	646	0.09%	0.011%
84	12.361	3519	3521	3525	rBV5	1697	1260	0.17%	0.021%
85	12.445	3544	3547	3549	rBV4	1198	715	0.10%	0.012%
86	12.458	3549	3551	3554	rBV4	918	618	0.08%	0.010%
87	12.844	3669	3671	3673	rBV4	1005	492	0.07%	0.008%
88	12.898	3686	3688	3692	rBV6	1620	1411	0.19%	0.024%
89	12.966	3703	3709	3712	rBV8	1799	1804	0.24%	0.030%
90	12.995	3716	3718	3721	rVB4	1844	864	0.12%	0.014%
91	13.017	3721	3725	3726	rBV4	2061	1354	0.18%	0.023%
92	13.207	3775	3784	3796	rBV2	31166	50864	6.85%	0.847%
93	13.445	3853	3858	3859	rBV5	1448	955	0.13%	0.016%
94	13.513	3878	3879	3881	rBV2	1057	552	0.07%	0.009%
95	13.786	3960	3964	3965	rBV4	1088	722	0.10%	0.012%
96	14.252	4106	4109	4112	rBV4	1633	1337	0.18%	0.022%
97	14.278	4116	4117	4120	rVB3	1232	521	0.07%	0.009%
98	14.590	4210	4214	4217	rBV5	1776	1225	0.17%	0.020%
99	14.696	4245	4247	4249	rBV2	1163	641	0.09%	0.011%
100	14.998	4339	4341	4343	rBV3	1657	845	0.11%	0.014%


Sum of corrected areas: 6002237

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030774.D
Acq On : 21 Apr 2023 18:54
Operator : SY/MD
Sample : 02440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

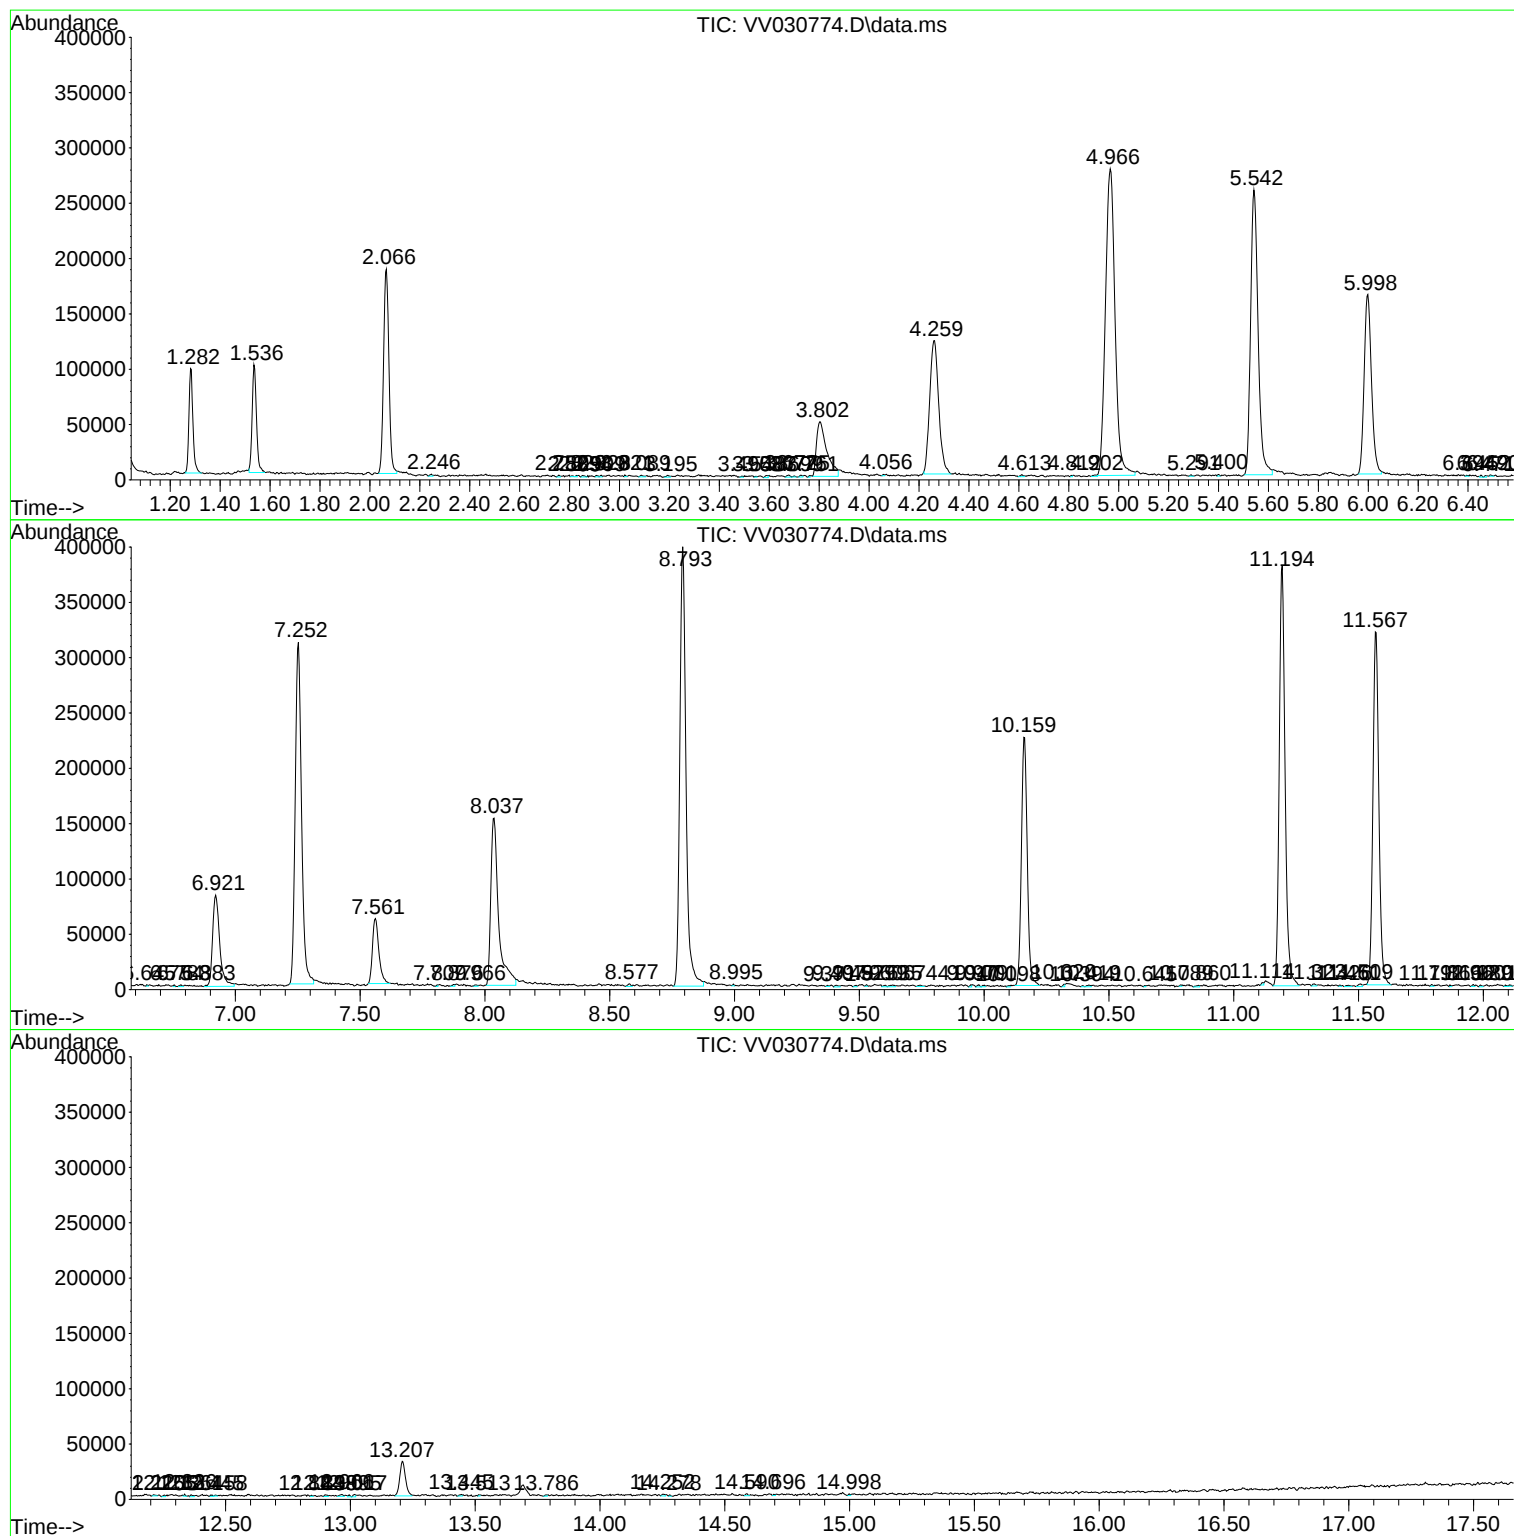

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030774.D
Acq On : 21 Apr 2023 18:54
Operator : SY/MD
Sample : 02440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030774.D
Acq On : 21 Apr 2023 18:54
Operator : SY/MD
Sample : 02440-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------