

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030776.D
 Acq On : 21 Apr 2023 20:19
 Operator : SY/MD
 Sample : 02440-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	90823	102226	13.59%	1.696%
2	1.536	148	154	164	rBV	89099	102083	13.57%	1.694%
3	2.063	310	318	332	rVB	189422	272243	36.19%	4.517%
4	2.597	479	484	486	rBV4	1420	1351	0.18%	0.022%
5	2.709	516	519	527	rBV10	1812	2100	0.28%	0.035%
6	2.773	538	539	541	rBV2	910	294	0.04%	0.005%
7	2.789	541	544	546	rBV4	655	420	0.06%	0.007%
8	3.002	608	610	615	rBV6	1106	566	0.08%	0.009%
9	3.050	623	625	629	rVB3	761	411	0.05%	0.007%
10	3.484	758	760	761	rBV2	1212	501	0.07%	0.008%
11	3.503	764	766	768	rVV3	955	383	0.05%	0.006%
12	3.580	786	790	792	rBV5	1678	1197	0.16%	0.020%
13	3.738	837	839	840	rBV2	708	213	0.03%	0.004%
14	3.751	840	843	846	rVB5	1769	1276	0.17%	0.021%
15	3.799	846	858	883	rBV2	47228	147421	19.60%	2.446%
16	4.156	967	969	973	rBV4	1549	938	0.12%	0.016%
17	4.256	986	1000	1022	rBV	123649	317001	42.14%	5.260%
18	4.439	1055	1057	1060	rBV3	1427	750	0.10%	0.012%
19	4.677	1129	1131	1133	rVB3	1230	380	0.05%	0.006%
20	4.963	1202	1220	1245	rBV2	280308	752275	100.00%	12.483%
21	5.268	1311	1315	1317	rBV4	1751	1061	0.14%	0.018%
22	5.404	1355	1357	1360	rBV4	1556	954	0.13%	0.016%
23	5.539	1386	1399	1422	rBV	271681	569086	75.65%	9.443%
24	5.995	1529	1541	1563	rVB	166541	340446	45.26%	5.649%
25	6.349	1649	1651	1653	rBV3	1567	823	0.11%	0.014%
26	6.429	1673	1676	1680	rBV6	1517	1094	0.15%	0.018%
27	6.641	1740	1742	1744	rBV2	1451	765	0.10%	0.013%
28	6.748	1773	1775	1779	rVB4	1680	792	0.11%	0.013%
29	6.802	1789	1792	1797	rBV8	1143	1176	0.16%	0.020%
30	6.860	1808	1810	1812	rBV3	1271	554	0.07%	0.009%
31	6.918	1819	1828	1848	rBV	80952	149327	19.85%	2.478%
32	7.047	1866	1868	1870	rBV3	1625	527	0.07%	0.009%
33	7.124	1890	1892	1895	rVB4	1304	568	0.08%	0.009%
34	7.169	1899	1906	1912	rBV4	2032	3077	0.41%	0.051%
35	7.249	1920	1931	1954	rBV	314616	560551	74.51%	9.302%
36	7.558	2018	2027	2043	rBV2	60298	108124	14.37%	1.794%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
 Data File : VV030776.D
 Acq On : 21 Apr 2023 20:19
 Operator : SY/MD
 Sample : 02440-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.735	2079	2082	2085	rBV4	1937	1548	0.21%	0.026%
38	7.792	2096	2100	2101	rBV4	1165	903	0.12%	0.015%
39	7.850	2116	2118	2119	rBV	1140	390	0.05%	0.006%
40	8.034	2165	2175	2213	rBV	141566	321276	42.71%	5.331%
41	8.448	2300	2304	2308	rBV6	1513	1485	0.20%	0.025%
42	8.699	2380	2382	2385	rBV3	1235	843	0.11%	0.014%
43	8.789	2399	2410	2429	rBV	414219	697278	92.69%	11.570%
44	9.153	2521	2523	2524	rBV2	1207	607	0.08%	0.010%
45	9.178	2528	2531	2533	rBV4	1741	1017	0.14%	0.017%
46	9.313	2569	2573	2575	rBV3	1373	1226	0.16%	0.020%
47	9.352	2581	2585	2587	rBV3	1942	1342	0.18%	0.022%
48	9.522	2636	2638	2639	rBV2	1686	731	0.10%	0.012%
49	9.680	2686	2687	2689	rBV2	915	469	0.06%	0.008%
50	9.725	2699	2701	2704	rBV3	1737	1006	0.13%	0.017%
51	10.085	2811	2813	2815	rVB4	952	307	0.04%	0.005%
52	10.120	2822	2824	2825	rBV2	1025	355	0.05%	0.006%
53	10.159	2825	2836	2855	rVV	225892	366615	48.73%	6.083%
54	10.381	2903	2905	2907	rBV3	1135	587	0.08%	0.010%
55	10.435	2919	2922	2924	rBV3	779	535	0.07%	0.009%
56	10.689	2999	3001	3004	rVB3	1049	362	0.05%	0.006%
57	10.847	3048	3050	3053	rVB4	1507	710	0.09%	0.012%
58	10.934	3075	3077	3083	rBV6	1155	842	0.11%	0.014%
59	11.056	3112	3115	3117	rBV3	1115	613	0.08%	0.010%
60	11.191	3146	3157	3180	rBV	386516	631357	83.93%	10.476%
61	11.567	3264	3274	3294	rVB	323495	526034	69.93%	8.729%
62	11.744	3323	3329	3331	rBV6	2089	2554	0.34%	0.042%
63	11.805	3346	3348	3354	rVB7	1339	916	0.12%	0.015%
64	11.915	3378	3382	3383	rBV4	1308	857	0.11%	0.014%
65	12.005	3409	3410	3412	rVB2	1487	483	0.06%	0.008%
66	12.281	3493	3496	3497	rBV3	1900	1042	0.14%	0.017%
67	12.525	3570	3572	3577	rBV6	1065	601	0.08%	0.010%
68	12.570	3585	3586	3587	rBV	760	224	0.03%	0.004%
69	12.760	3642	3645	3647	rVB3	1499	818	0.11%	0.014%
70	12.776	3647	3650	3656	rBV8	2173	2126	0.28%	0.035%
71	12.821	3662	3664	3667	rVB3	1454	758	0.10%	0.013%
72	12.850	3670	3673	3677	rBV6	1114	869	0.12%	0.014%
73	12.873	3677	3680	3682	rBV4	875	595	0.08%	0.010%
74	12.934	3696	3699	3701	rBV3	867	566	0.08%	0.009%
75	12.953	3702	3705	3708	rVB5	1964	1285	0.17%	0.021%
76	13.123	3756	3758	3761	rBV3	1146	686	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030776.D
Acq On : 21 Apr 2023 20:19
Operator : SY/MD
Sample : 02440-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis

77	13.140	3761	3763	3765	rVV3	1133	443	0.06%	0.007%
78	13.307	3813	3815	3820	rBV6	1950	1801	0.24%	0.030%
79	13.554	3890	3892	3893	rBV	920	322	0.04%	0.005%
80	13.583	3899	3901	3904	rVB4	2426	1195	0.16%	0.020%
81	13.612	3904	3910	3911	rBV6	2382	2556	0.34%	0.042%
82	13.754	3952	3954	3957	rVB4	1736	848	0.11%	0.014%
83	13.802	3967	3969	3971	rBV3	1136	622	0.08%	0.010%
84	13.844	3979	3982	3983	rBV3	1896	1008	0.13%	0.017%
85	13.892	3995	3997	3998	rBV2	1140	439	0.06%	0.007%
86	14.493	4181	4184	4187	rBV5	1792	1437	0.19%	0.024%

Sum of corrected areas: 6026443




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030776.D
Acq On : 21 Apr 2023 20:19
Operator : SY/MD
Sample : 02440-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

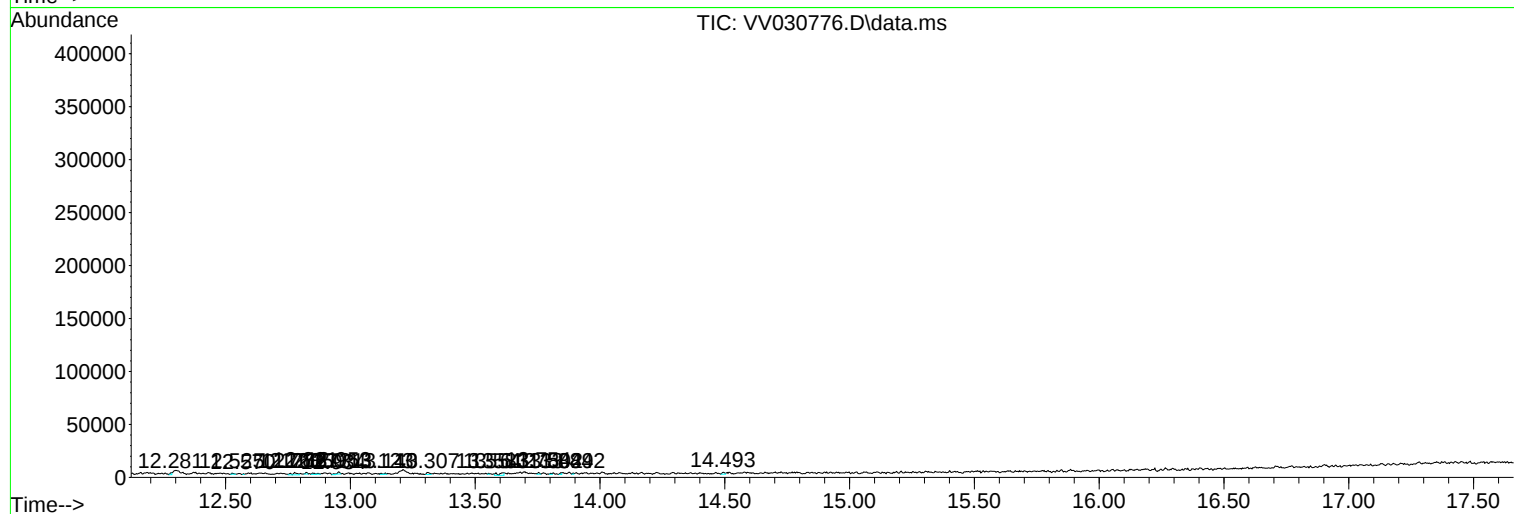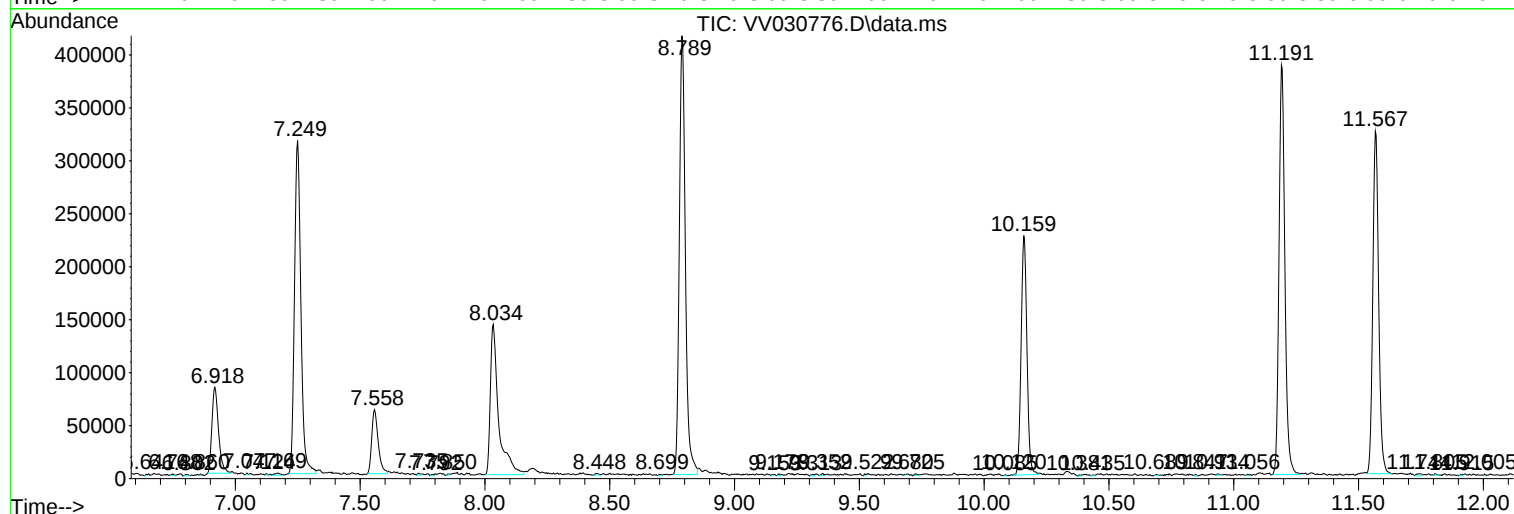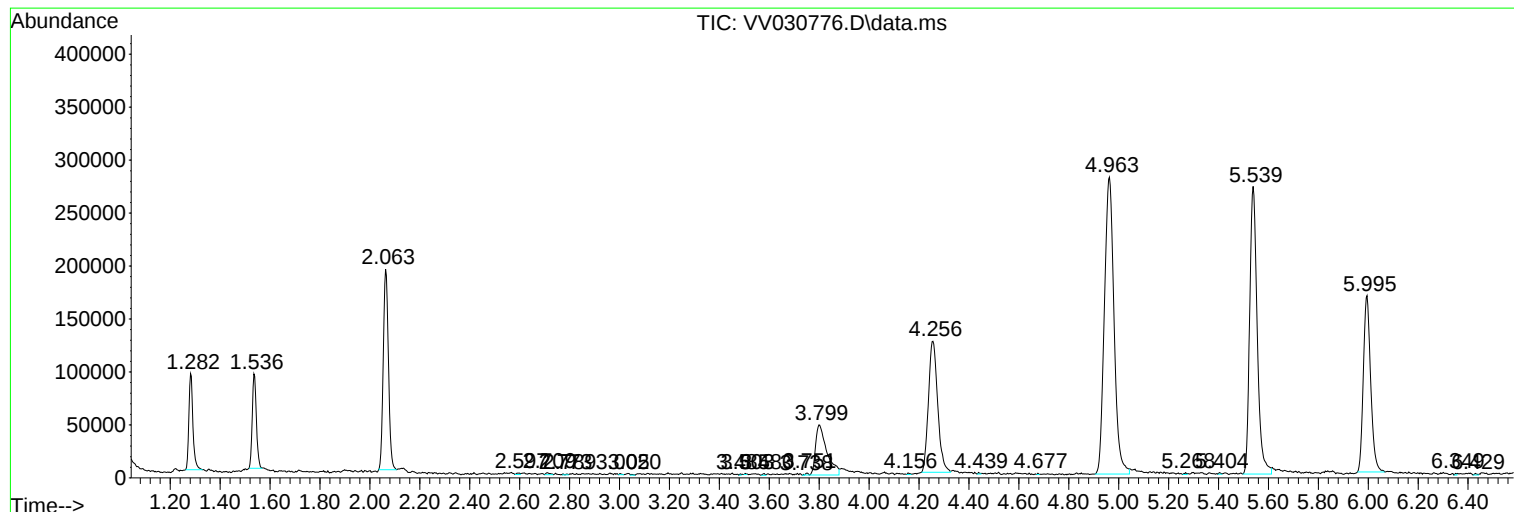

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030776.D
Acq On : 21 Apr 2023 20:19
Operator : SY/MD
Sample : 02440-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030776.D
Acq On : 21 Apr 2023 20:19
Operator : SY/MD
Sample : 02440-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------