


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042123\
Data File : VV030753.D
Acq On : 21 Apr 2023 09:59
Operator : SY/MD
Sample : BFB370
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB370

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis
Last Update : Sat Apr 22 00:43:23 2023

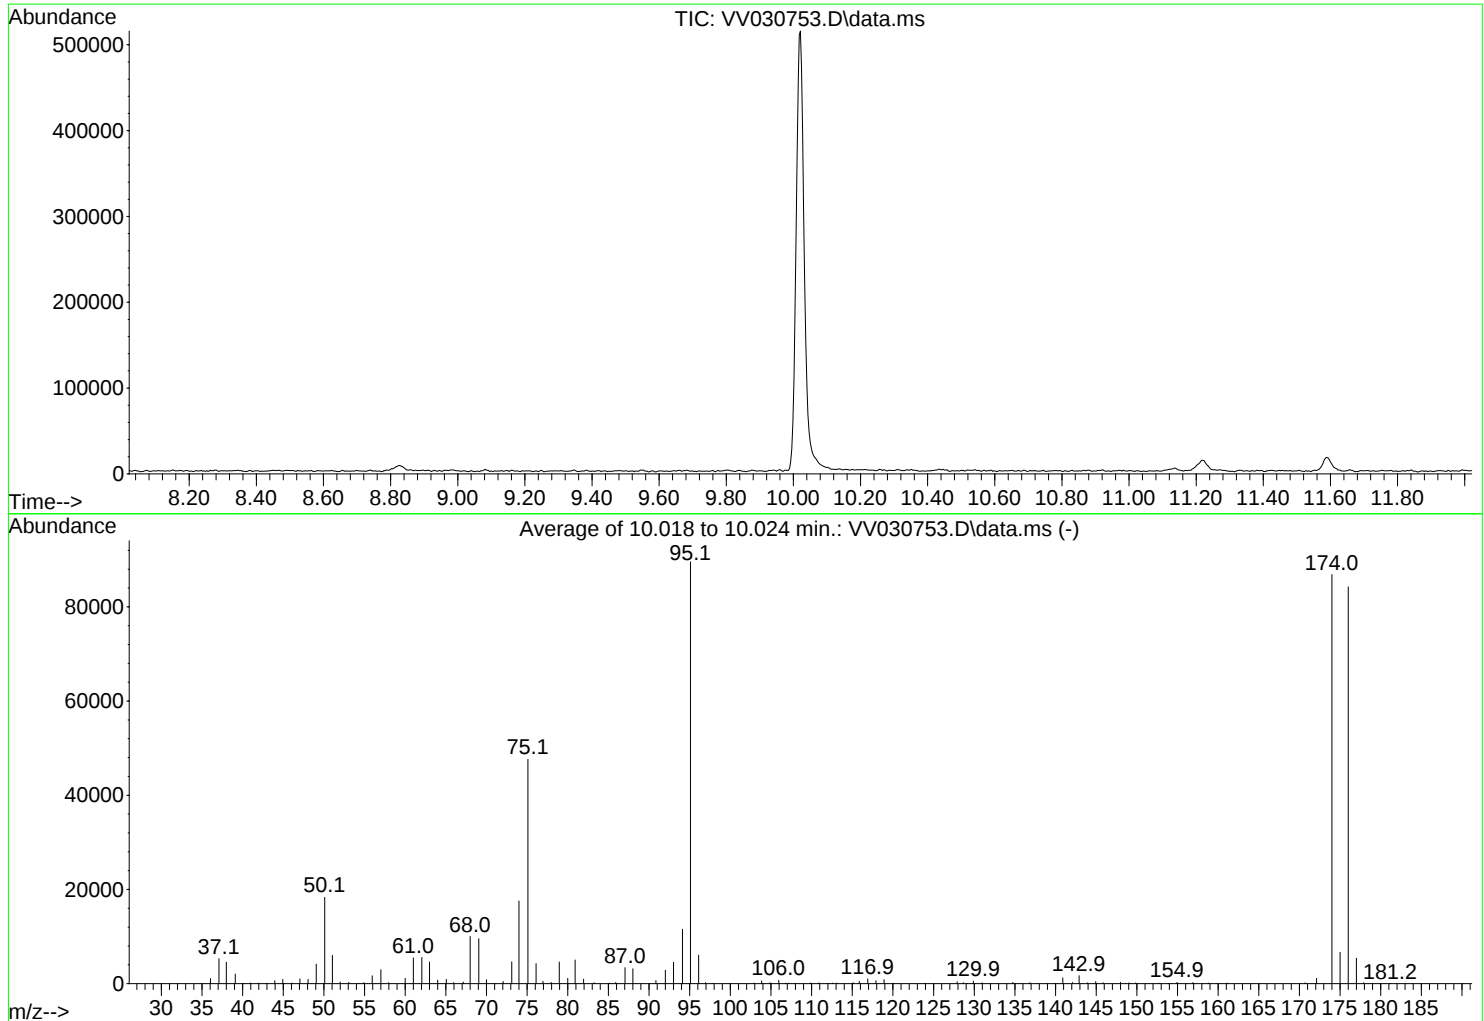

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	18331	PASS
75	95	30	80	53.2	47637	PASS
95	95	100	100	100.0	89555	PASS
96	95	5	9	6.7	6038	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.0	86861	PASS
175	174	5	9	7.7	6646	PASS
176	174	95	105	97.0	84253	PASS
177	176	5	10	6.4	5413	PASS

m/z	Abundance
36.20	112.0
36.70	135.0
37.40	138.0
38.00	102.0
38.40	125.0
39.60	246.0
40.30	227.0
41.50	103.0
42.40	110.0
42.90	119.0
43.90	247.0
44.90	145.0
45.60	131.0
46.00	129.0
48.60	107.0
49.70	105.0
50.40	123.0
51.30	117.0
53.30	121.0
54.20	133.0
54.90	125.0
55.90	125.0
56.50	122.0
58.50	112.0
62.40	109.0
65.00	126.0
66.30	118.0
68.30	153.0
69.00	130.0
71.90	115.0
73.40	124.0
78.10	144.0
101.40	124.0
123.10	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
36.10	1255.0
37.10	5397.0
38.10	4848.0
39.10	2312.0
40.20	244.0
41.00	141.0
41.70	141.0
43.10	182.0
44.00	935.0
45.00	1115.0
46.20	278.0
47.00	971.0
48.00	996.0
49.00	4205.0
50.10	19152.0
51.00	6290.0
52.00	382.0
53.10	297.0
54.10	115.0
55.00	378.0
56.00	1876.0
57.00	3005.0
57.90	163.0
60.00	1166.0
61.00	5625.0
62.10	5708.0
63.00	4771.0
64.00	660.0
65.10	981.0
66.00	179.0
67.20	363.0
68.00	10214.0
69.10	9722.0
70.00	855.0
70.80	103.0
72.10	634.0
73.10	4700.0
74.00	18096.0
75.10	48448.0
76.10	4607.0
76.90	467.0
77.90	342.0
79.00	4592.0
80.00	1118.0
80.90	5230.0
82.00	945.0
83.20	223.0
85.10	101.0
85.90	294.0
87.00	3399.0
88.00	3295.0
90.90	657.0
92.00	2906.0
93.00	4751.0
94.10	12214.0
95.10	91976.0
96.10	6315.0
97.00	253.0
102.90	137.0
103.90	572.0
104.90	200.0
105.90	693.0
107.20	181.0
108.00	108.0
109.80	115.0
111.00	165.0
112.00	106.0
112.60	150.0
113.10	116.0
115.10	177.0
115.90	530.0
116.90	1015.0
117.90	654.0
118.90	863.0
120.10	111.0
127.90	413.0
128.70	214.0
129.90	585.0
130.90	149.0
134.80	285.0
135.60	104.0
136.90	262.0
140.00	155.0
140.90	1422.0
142.10	205.0
142.90	1707.0
143.90	169.0
145.00	448.0
145.80	260.0
148.00	328.0
149.00	154.0
149.80	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

152.80	117.0
153.90	106.0
154.90	271.0
156.90	281.0
158.80	127.0
161.10	166.0
170.70	243.0
172.10	1063.0
174.00	87664.0
175.00	6979.0
176.00	84704.0
177.00	5646.0
177.90	243.0
181.20	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
36.00	1254.0
37.10	5500.0
38.10	4779.0
39.10	2110.0
40.10	255.0
41.00	150.0
41.90	145.0
43.10	174.0
44.00	903.0
45.00	1127.0
46.20	276.0
47.00	1038.0
48.00	967.0
49.10	4266.0
50.10	18832.0
51.00	6268.0
52.00	383.0
53.00	298.0
54.30	112.0
55.00	317.0
56.00	1858.0
57.00	3057.0
57.90	205.0
60.00	1140.0
61.00	5628.0
62.00	5784.0
63.00	4724.0
64.00	771.0
65.10	1079.0
66.00	219.0
67.10	347.0
68.00	10331.0
69.10	10009.0
70.00	880.0
72.10	617.0
73.10	4727.0
74.00	18208.0
75.10	49104.0
76.10	4391.0
76.90	523.0
77.90	423.0
78.90	4751.0
80.00	1139.0
80.90	5186.0
81.90	1002.0
83.20	208.0
85.10	136.0
85.90	243.0
87.00	3453.0
88.00	3303.0
90.90	649.0
92.00	2952.0
93.00	4697.0
94.10	11867.0
95.10	92504.0
96.10	6249.0
96.90	252.0
102.90	126.0
103.90	569.0
104.90	214.0
106.00	752.0
106.80	170.0
107.10	167.0
107.90	102.0
109.90	131.0
110.80	168.0
112.60	164.0
113.10	127.0
115.10	200.0
115.80	499.0
116.90	1043.0
117.90	613.0
118.90	902.0
120.10	123.0
123.90	109.0
127.90	416.0
128.60	181.0
129.90	553.0
131.00	171.0
134.70	299.0
136.90	205.0
140.90	1254.0
142.10	244.0
142.90	1747.0
144.00	153.0
145.00	449.0
145.90	200.0
148.00	286.0
149.00	169.0
149.90	131.0
152.70	107.0
154.90	281.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

156.90	242.0
158.80	135.0
161.10	146.0
170.70	253.0
172.10	1148.0
174.00	89840.0
175.00	6780.0
176.00	86984.0
177.00	5568.0
177.90	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

m/z	Abundance
36.00	1132.0
37.10	4995.0
38.00	4310.0
39.10	1723.0
40.00	251.0
40.90	146.0
42.00	186.0
42.90	192.0
44.00	784.0
45.00	974.0
46.20	232.0
47.10	1052.0
48.10	826.0
49.10	3929.0
50.10	17008.0
51.10	5527.0
52.00	303.0
53.00	260.0
54.30	139.0
54.90	280.0
56.00	1670.0
57.00	2855.0
58.00	213.0
60.00	1033.0
61.00	5137.0
62.00	5236.0
63.00	4287.0
64.00	792.0
65.10	1097.0
65.90	225.0
67.10	326.0
68.00	9498.0
69.10	9268.0
70.00	752.0
72.10	551.0
73.10	4446.0
74.00	16408.0
75.10	45360.0
76.10	3780.0
77.00	580.0
78.00	451.0
78.90	4415.0
80.00	1161.0
80.90	4635.0
81.90	926.0
83.30	170.0
85.10	118.0
85.90	201.0
87.10	3327.0
88.00	2904.0
90.80	591.0
92.00	2667.0
93.00	4142.0
94.10	10567.0
95.10	84184.0
96.10	5549.0
96.90	204.0
97.80	101.0
102.90	105.0
103.80	557.0
104.90	202.0
105.90	719.0
106.80	187.0
109.90	169.0
110.90	181.0
112.20	139.0
112.60	128.0
113.10	135.0
115.10	188.0
115.80	465.0
116.90	957.0
117.90	549.0
118.90	817.0
123.30	114.0
123.90	110.0
127.90	441.0
128.60	171.0
129.10	163.0
129.90	474.0
131.00	161.0
134.70	270.0
136.80	184.0
140.90	999.0
142.10	231.0
142.90	1640.0
143.90	167.0
144.80	441.0
145.80	134.0
148.00	245.0
148.60	118.0
149.10	159.0
149.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370

152.60	104.0
155.00	293.0
156.90	180.0
158.80	144.0
161.10	131.0
172.10	1123.0
174.00	83080.0
175.00	6180.0
176.00	81072.0
177.00	5025.0
177.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB370