

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042220\
 Data File : VV015636.D
 Acq On : 22 Apr 2020 21:10
 Operator : SY/MD
 Sample : L2366-23
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Apr 23 05:05:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 23 03:05:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	131260	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	124117	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	61175	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	31282	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.58	69	31067	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.12	63	52240	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.93	46	112002	50.85	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.70%
24) Chloroform-d	4.38	84	75061	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.06	65	45447	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.08	84	144722	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.09	67	46341	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.34	98	134305	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
43) trans-1,3-Dichloropropene-	7.64	79	14819	4.05	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.00%
46) 2-Hexanone-d5	8.11	63	83976	47.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.08%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	32874	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	51516	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
16) Methylene chloride	2.52	84	2134	0.226 ug/L	93
25) Chloroform	4.40	83	2922	0.164 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042220\
Data File : VV015636.D
Acq On : 22 Apr 2020 21:10
Operator : SY/MD
Sample : L2366-23
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Apr 23 05:05:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 23 03:05:46 2020
Response via : Initial Calibration

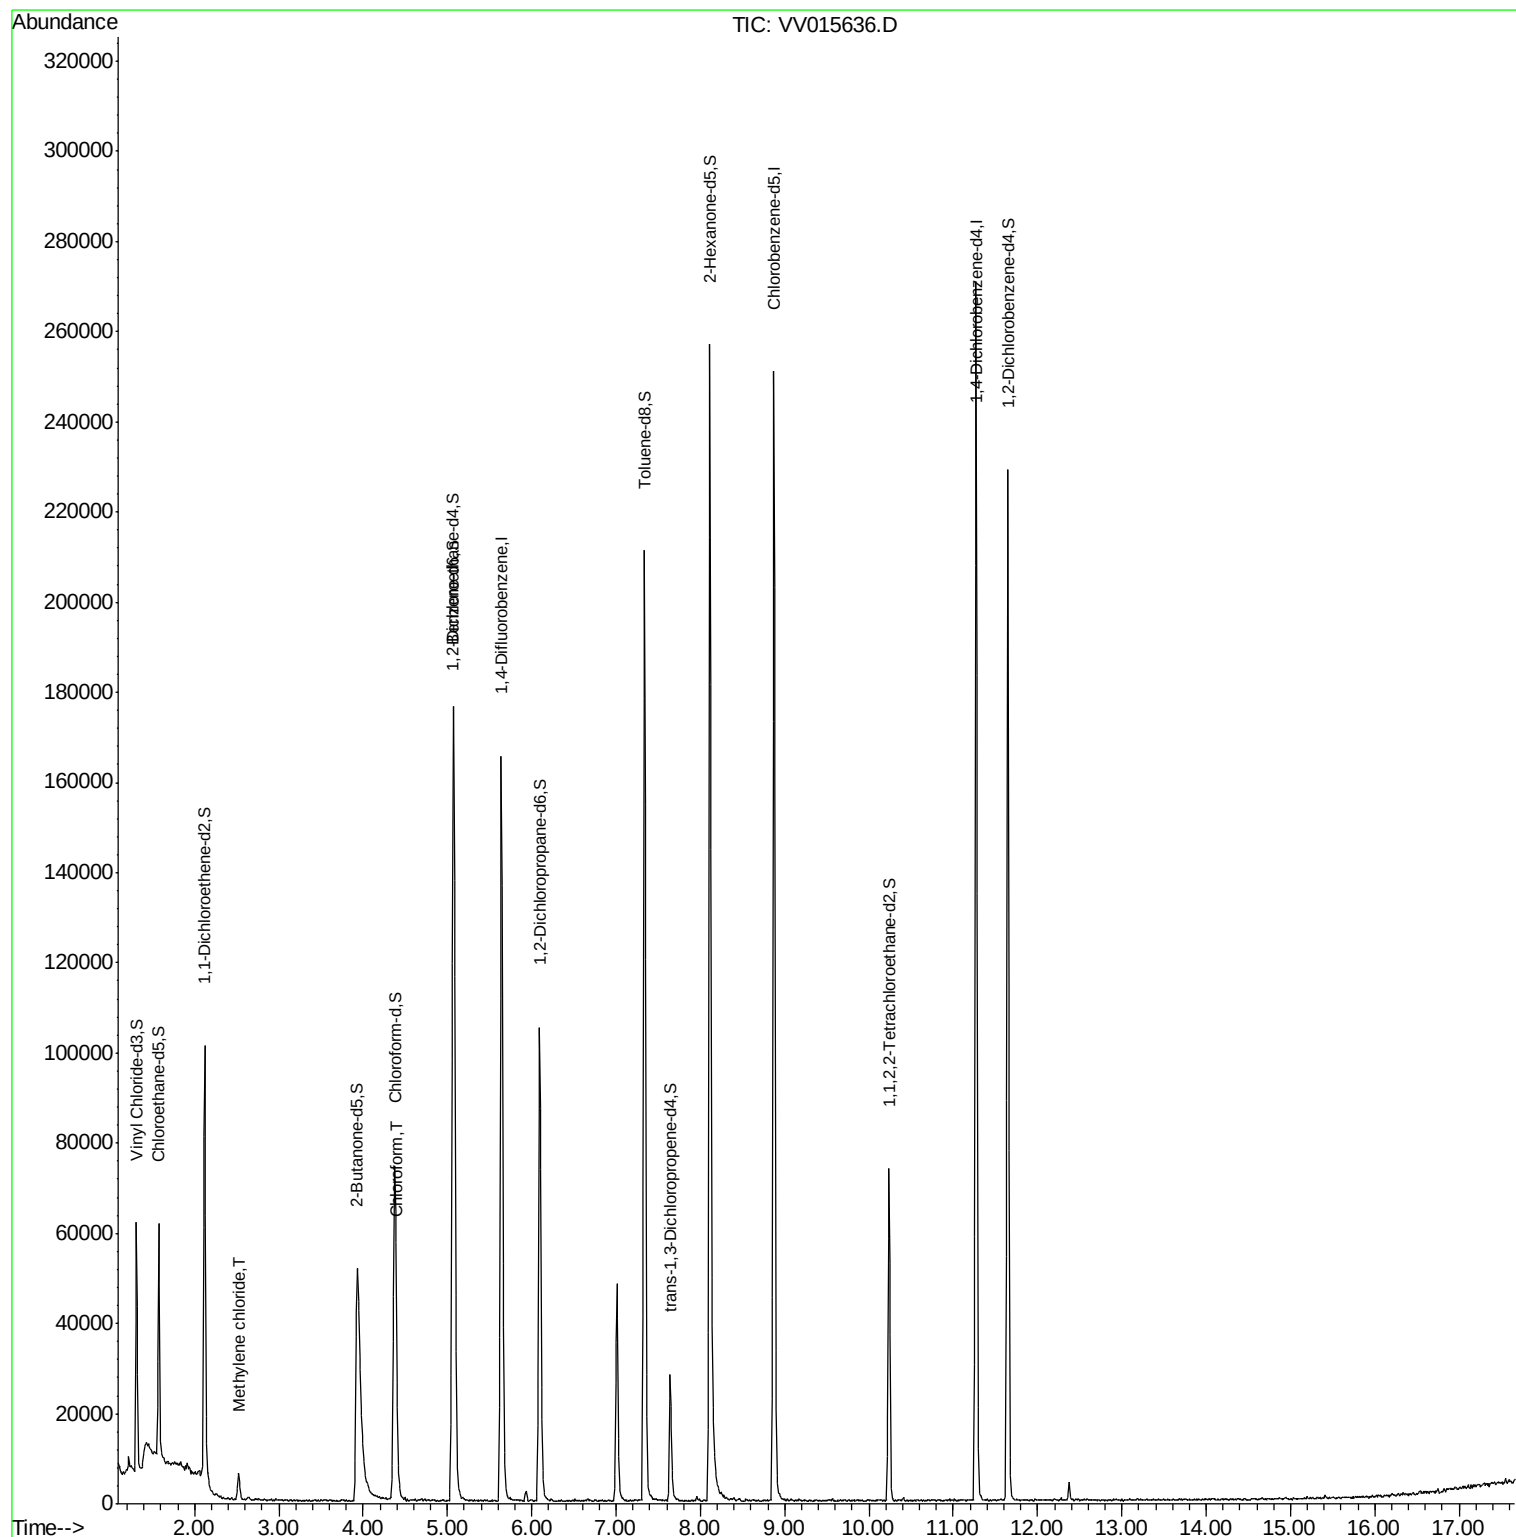


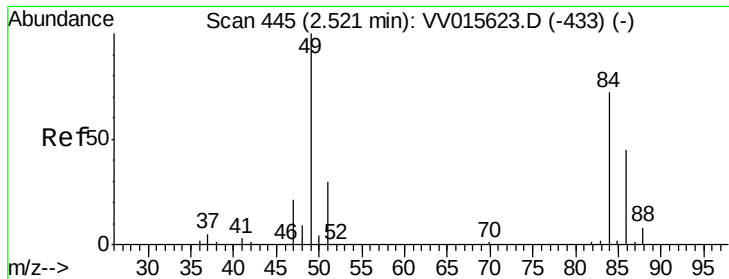




#16
Methylene chloride
Concen: 0.226 ug/L
RT: 2.52 min Scan# 446
Delta R.T. 0.00 min
Lab File: VV015636.D
Acq: 22 Apr 2020 21:10

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion: 84 Resp: 2134
Ion Ratio Lower Upper
84 100
86 73.7 45.1 83.7
49 139.9 94.4 175.4

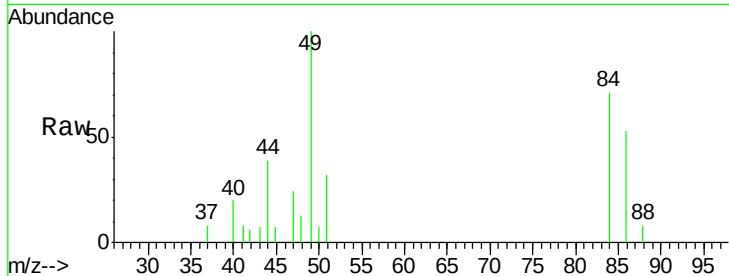


Abundance Ion 84.05 (83.75 to 84.75): VV0
Ion 86.00 (85.70 to 86.70): VV0
Ion 49.10 (48.80 to 49.80): VV0

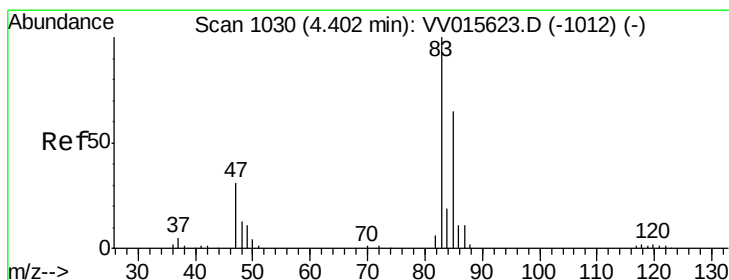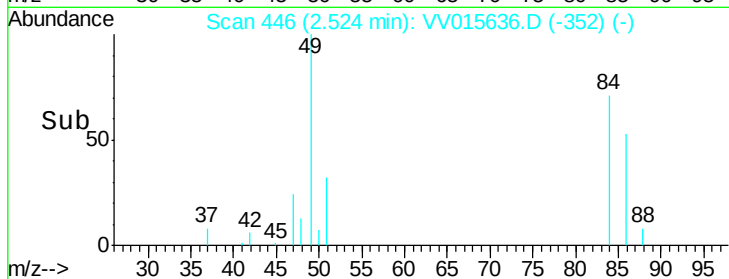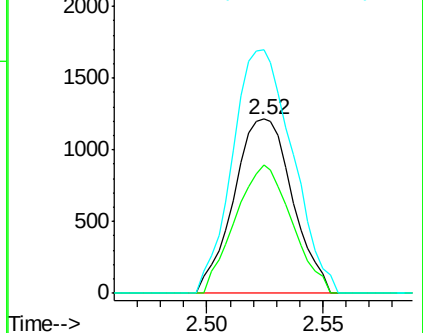

#25
Chloroform
Concen: 0.164 ug/L
RT: 4.40 min Scan# 1030
Delta R.T. 0.00 min
Lab File: VV015636.D
Acq: 22 Apr 2020 21:10

Tgt Ion: 83 Resp: 2922
Ion Ratio Lower Upper
83 100
85 70.7 46.1 85.5

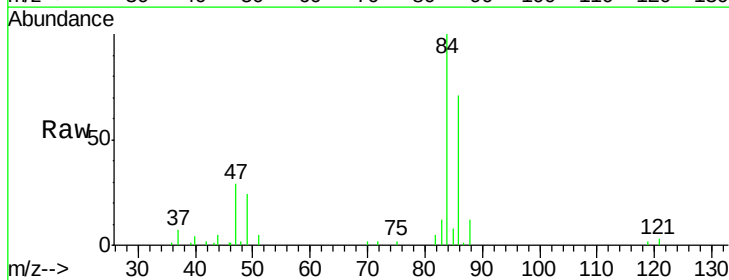

Abundance Ion 83.05 (82.75 to 83.75): VV0
Ion 85.00 (84.70 to 85.70): VV0

