

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042220\
 Data File : VV015638.D
 Acq On : 22 Apr 2020 21:57
 Operator : SY/MD
 Sample : L2370-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKJ7

Quant Time: Apr 23 05:18:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 23 03:05:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	128557	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	124740	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	59328	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	31858	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.57	69	29996	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.12	63	50030	3.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.00%
20) 2-Butanone-d5	3.95	46	101129	46.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.76%
24) Chloroform-d	4.38	84	71216	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.06	65	42510	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.07	84	138718	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.09	67	43962	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.34	98	126896	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.65	79	12691	3.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.00%
46) 2-Hexanone-d5	8.11	63	78040	43.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.00%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	32338	4.56	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	48734	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.94	96	1979	0.214 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042220\
Data File : VV015638.D
Acq On : 22 Apr 2020 21:57
Operator : SY/MD
Sample : L2370-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKJ7

Quant Time: Apr 23 05:18:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 23 03:05:46 2020
Response via : Initial Calibration

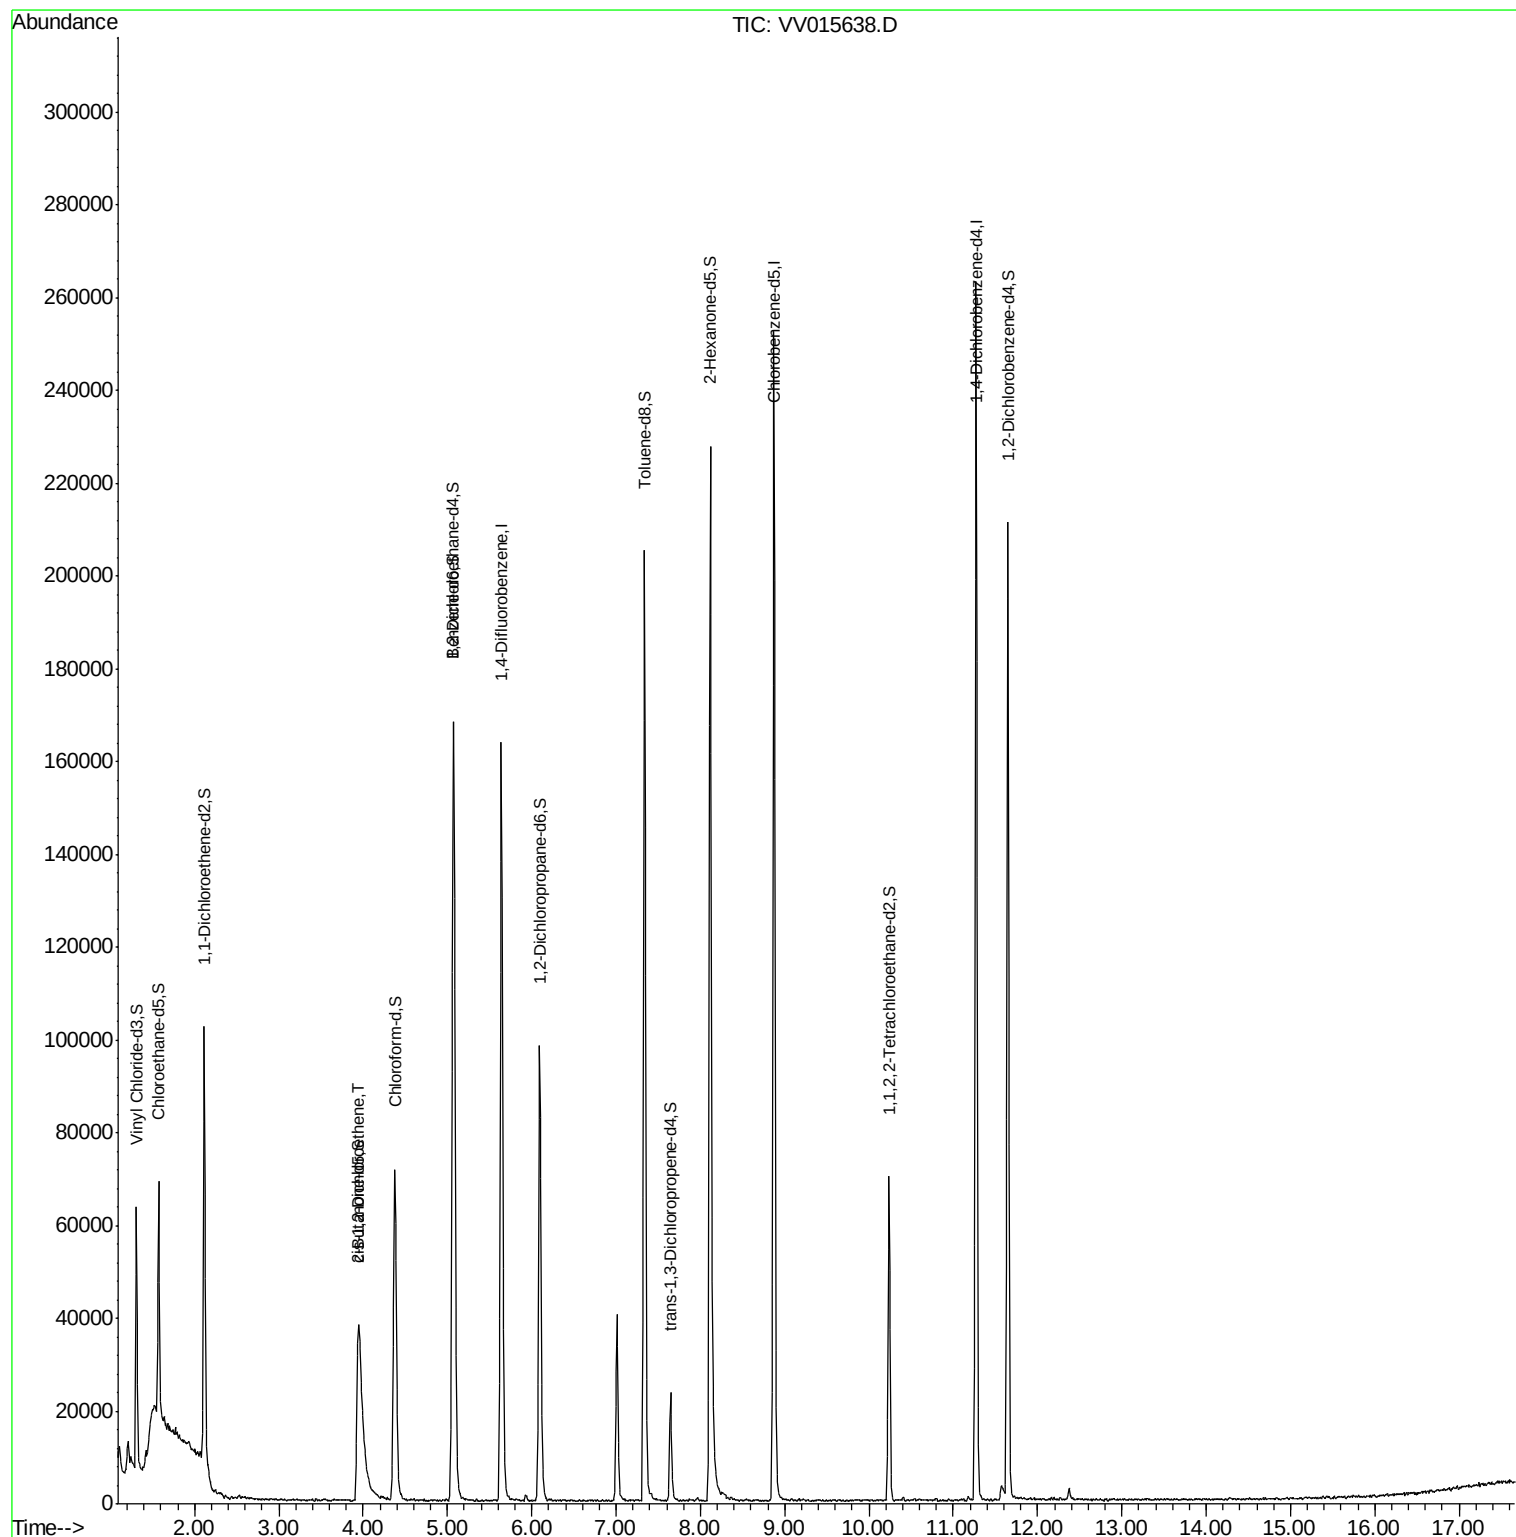

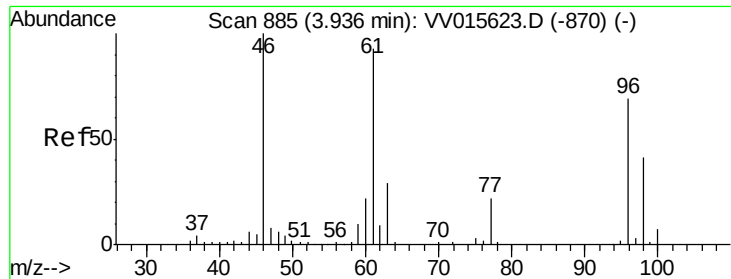

#22
 cis-1,2-Dichloroethene
 Concen: 0.214 ug/L
 RT: 3.94 min Scan# 887
 Delta R.T. 0.01 min
 Lab File: VV015638.D
 Acq: 22 Apr 2020 21:57

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKJ7

Tot Ion:	96	Resp:	1979
Ion	Ratio	Lower	Upper
96	100		
61	136.3	96.4	179.0
68	0.0	0.0	0.0

