

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042220\
 Data File : VV015641.D
 Acq On : 22 Apr 2020 23:07
 Operator : SY/MD
 Sample : L2370-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKK1

Quant Time: Apr 23 05:32:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 23 03:05:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	130529	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	124191	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	57432	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	33297	4.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.60%
7) Chloroethane-d5	1.58	69	32036	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.12	63	51922	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.91	46	97897	44.70	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.40%
24) Chloroform-d	4.38	84	74618	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
26) 1,2-Dichloroethane-d4	5.06	65	42761	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.08	84	141611	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.09	67	44748	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.34	98	127442	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.65	79	11748	3.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	64.20%
46) 2-Hexanone-d5	8.11	63	74512	41.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.44%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	30827	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.40%
64) 1,2-Dichlorobenzene-d4	11.65	152	47593	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	1843	1.212 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042220\
Data File : VV015641.D
Acq On : 22 Apr 2020 23:07
Operator : SY/MD
Sample : L2370-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETKK1

Quant Time: Apr 23 05:32:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 23 03:05:46 2020
Response via : Initial Calibration

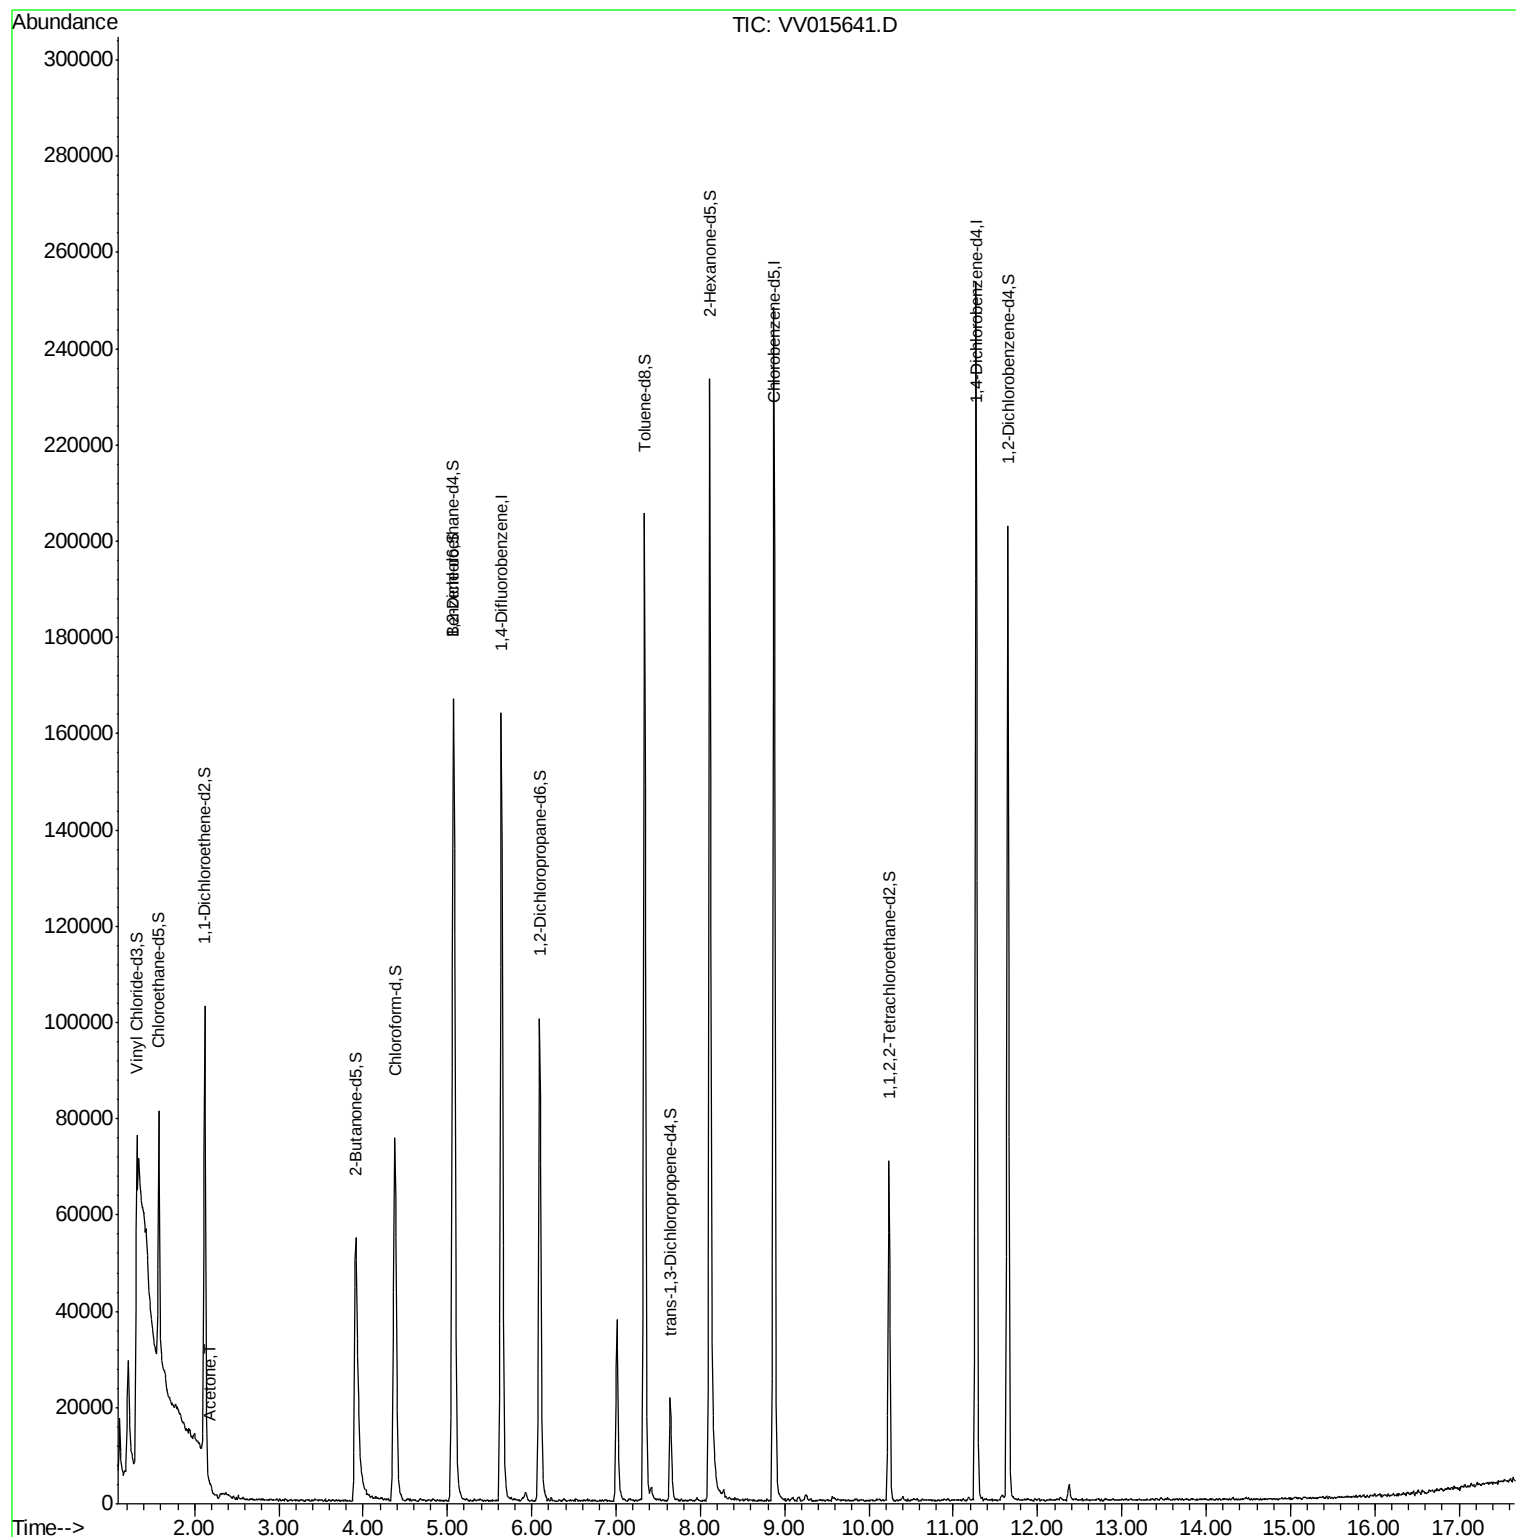

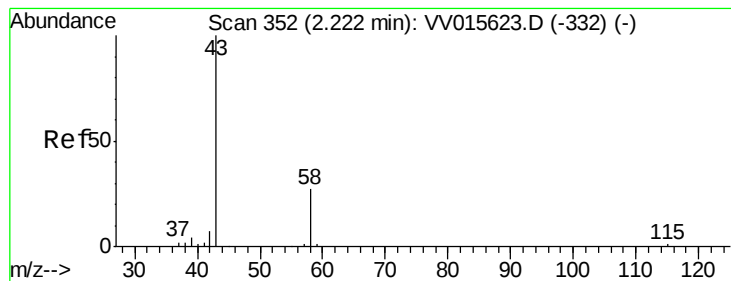

#13
 Acetone
 Concen: 1.212 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.04 min
 Lab File: VV015641.D
 Acq: 22 Apr 2020 23:07

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKK1

Tot Ion: 43 Resp: 1843
 Ion Ratio Lower Upper
 43 100
 58 24.3 0.0 57.6

