


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042220\
 Data File : VV015615.D
 Acq On : 22 Apr 2020 09:37
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 23 03:05:46 2020

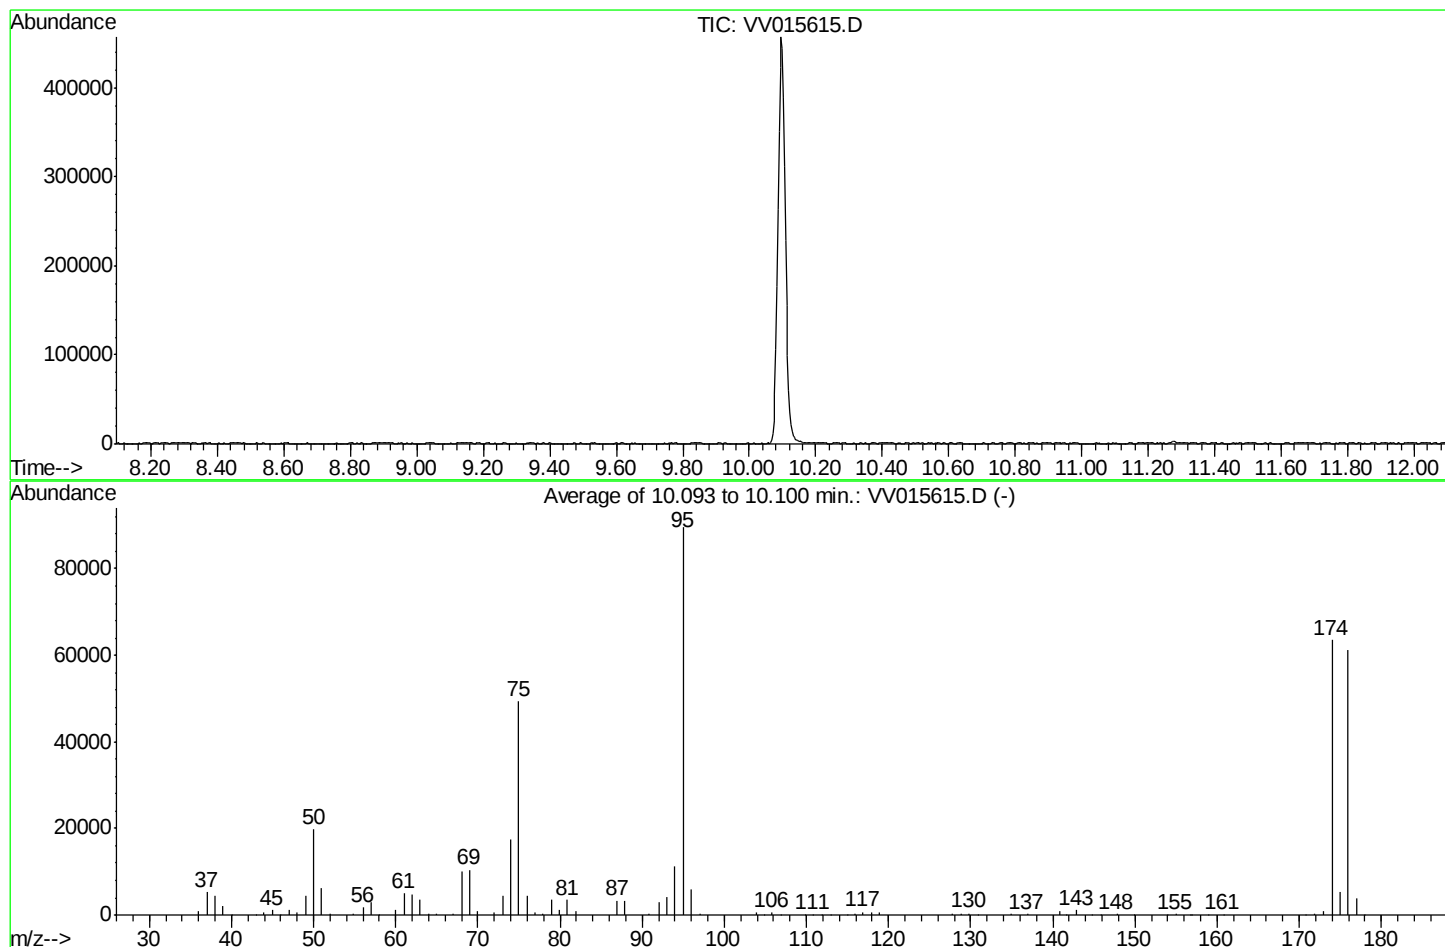

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	19773	PASS
75	95	30	80	55.0	49290	PASS
95	95	100	100	100.0	89549	PASS
96	95	5	9	6.7	6011	PASS
173	174	0.00	2	1.3	832	PASS
174	95	50	120	71.0	63546	PASS
175	174	5	9	8.2	5234	PASS
176	174	95	101	96.3	61178	PASS
177	176	5	9	6.4	3897	PASS

m/z	Abundance
36.00	1000.0
37.00	5131.0
38.00	4494.0
39.00	1923.0
40.00	357.0
43.00	111.0
44.00	1047.0
45.00	1000.0
46.00	132.0
47.00	1137.0
48.00	676.0
49.00	4325.0
50.00	19224.0
51.00	6054.0
52.00	326.0
54.90	430.0
56.00	1681.0
57.00	2734.0
57.90	139.0
60.00	1141.0
61.00	5024.0
62.00	4694.0
63.00	3535.0
64.00	389.0
65.00	304.0
66.90	308.0
68.00	9716.0
69.00	10157.0
70.00	784.0
72.00	676.0
73.00	4283.0
74.00	16920.0
75.00	47656.0
76.00	4395.0
77.00	522.0
77.90	337.0
78.90	3252.0
79.90	1019.0
80.90	3359.0
81.90	868.0
87.00	3203.0
87.90	3085.0
90.80	280.0
92.00	2871.0
93.00	3998.0
94.00	11110.0
95.00	85792.0
96.00	5932.0
97.00	201.0
103.80	472.0
104.80	139.0
105.80	514.0
106.90	154.0
110.80	140.0
115.00	134.0
115.90	390.0
116.90	607.0
117.90	460.0
118.80	486.0
127.80	339.0
128.80	202.0
129.80	399.0
130.80	107.0
135.00	168.0
136.90	184.0
140.90	979.0
141.60	131.0
142.90	1100.0
144.80	155.0
145.80	150.0
147.90	175.0
149.90	116.0
154.90	204.0
156.70	157.0
158.90	128.0
160.70	113.0
171.90	442.0
173.00	692.0
173.90	59784.0
174.90	4990.0
175.90	56864.0
177.00	3688.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	1041.0
37.00	5366.0
38.00	4800.0
39.00	2028.0
40.00	355.0
43.00	116.0
44.00	1111.0
45.00	1116.0
46.00	143.0
47.00	1221.0
48.00	690.0
49.00	4530.0
50.00	20504.0
51.00	6318.0
52.00	332.0
54.90	424.0
56.00	1758.0
57.00	2964.0
57.90	138.0
60.00	1182.0
61.00	5188.0
62.00	4932.0
63.00	3682.0
64.00	395.0
65.00	342.0
66.90	390.0
68.00	10433.0
69.00	10835.0
70.00	838.0
72.00	770.0
73.00	4603.0
74.00	17920.0
75.00	50936.0
76.00	4790.0
76.90	544.0
77.90	352.0
78.90	3585.0
79.90	1106.0
80.90	3563.0
81.90	925.0
87.00	3488.0
87.90	3374.0
90.80	338.0
92.00	2973.0
93.00	4172.0
94.00	11577.0
95.00	93008.0
96.00	6262.0
97.00	216.0
103.90	496.0
104.80	156.0
105.80	558.0
106.90	146.0
109.80	105.0
110.80	126.0
112.90	128.0
114.90	138.0
115.90	367.0
116.90	694.0
117.90	480.0
118.80	527.0
127.80	392.0
128.90	189.0
129.80	423.0
130.80	148.0
134.90	178.0
136.90	227.0
140.90	1074.0
142.90	1244.0
144.80	142.0
145.80	136.0
147.80	228.0
149.90	133.0
153.90	106.0
155.00	235.0
156.70	149.0
158.90	121.0
160.70	124.0
170.80	107.0
171.90	462.0
173.00	870.0
174.00	65784.0
174.90	5499.0
175.90	63416.0
177.00	3992.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	991.0
37.00	5207.0
38.00	4487.0
39.00	1919.0
40.00	321.0
42.90	112.0
44.00	1152.0
45.00	1097.0
46.00	162.0
47.00	1143.0
48.00	609.0
49.00	4292.0
50.00	19592.0
51.00	6077.0
52.00	308.0
54.90	388.0
56.00	1651.0
57.00	2922.0
58.00	111.0
60.00	1062.0
61.00	4851.0
62.00	4806.0
63.00	3552.0
63.90	366.0
65.00	328.0
66.90	439.0
68.00	9881.0
69.00	10328.0
70.00	808.0
71.90	732.0
73.00	4640.0
74.00	17280.0
75.00	49280.0
76.00	4584.0
76.90	474.0
77.90	330.0
78.90	3514.0
79.90	1083.0
80.90	3495.0
81.90	909.0
86.90	3267.0
87.90	3338.0
90.80	371.0
92.00	2792.0
93.00	3970.0
94.00	10890.0
95.00	89848.0
96.00	5839.0
97.00	198.0
103.90	469.0
104.80	158.0
105.80	546.0
106.90	109.0
111.90	108.0
112.90	146.0
114.80	123.0
115.90	335.0
116.90	688.0
117.90	464.0
118.90	519.0
127.80	389.0
128.90	153.0
129.80	377.0
130.80	169.0
134.80	179.0
136.90	244.0
140.90	1059.0
141.70	160.0
142.90	1203.0
144.80	106.0
145.80	126.0
147.80	232.0
149.90	128.0
153.90	102.0
155.00	218.0
156.90	132.0
160.80	122.0
170.70	127.0
171.90	456.0
173.00	934.0
174.00	65072.0
174.90	5213.0
175.90	63256.0
177.00	4013.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

Scan 2788 (10.055 min): VV015615.D
BFB40

m/z	Abundance
39.90	281.0
41.00	102.0
43.90	417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40