

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021091.D
 Acq On : 22 Apr 2021 12:44
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	437533	443201	15.97%	2.071%
2	1.571	158	165	177	rVB	337289	383756	13.83%	1.794%
3	2.108	323	332	345	rBV	735079	1040485	37.49%	4.863%
4	2.429	427	432	434	rBV3	932	968	0.03%	0.005%
5	2.661	502	504	507	rVB3	829	371	0.01%	0.002%
6	2.728	520	525	526	rBV2	797	625	0.02%	0.003%
7	2.864	564	567	570	rBV2	548	368	0.01%	0.002%
8	2.966	596	599	603	rVB4	614	411	0.01%	0.002%
9	2.982	603	604	605	rBV4	283	73	0.00%	0.000%
10	3.011	610	613	614	rBV	746	363	0.01%	0.002%
11	3.047	621	624	630	rVB2	1046	988	0.04%	0.005%
12	3.076	630	633	635	rBV	710	501	0.02%	0.002%
13	3.134	649	651	656	rVB4	882	501	0.02%	0.002%
14	3.172	660	663	666	rVV3	742	501	0.02%	0.002%
15	3.195	668	670	675	rVB3	581	422	0.02%	0.002%
16	3.343	713	716	720	rVB3	760	659	0.02%	0.003%
17	3.362	720	722	723	rBV	319	110	0.00%	0.001%
18	3.372	723	725	726	rBV	395	164	0.01%	0.001%
19	3.455	747	751	752	rBV2	809	496	0.02%	0.002%
20	3.500	763	765	766	rBV	304	140	0.01%	0.001%
21	3.539	773	777	779	rBV2	951	777	0.03%	0.004%
22	3.603	795	797	803	rBV3	483	397	0.01%	0.002%
23	3.648	809	811	816	rVB2	715	529	0.02%	0.002%
24	3.680	816	821	824	rBV2	805	665	0.02%	0.003%
25	3.699	825	827	830	rVV3	688	316	0.01%	0.001%
26	3.712	830	831	832	rVV	315	72	0.00%	0.000%
27	3.722	832	834	837	rVB2	401	188	0.01%	0.001%
28	3.738	837	839	843	rBV3	445	384	0.01%	0.002%
29	3.780	849	852	853	rBV	411	237	0.01%	0.001%
30	3.831	862	868	871	rBV2	568	557	0.02%	0.003%
31	3.899	878	889	925	rBV2	132865	500423	18.03%	2.339%
32	4.349	1014	1029	1055	rBV	472102	1172546	42.24%	5.480%
33	4.658	1122	1125	1127	rBV3	939	602	0.02%	0.003%
34	4.677	1127	1131	1133	rBV3	1271	1005	0.04%	0.005%
35	4.741	1146	1151	1155	rBV6	793	889	0.03%	0.004%
36	4.841	1179	1182	1186	rBV3	1283	1051	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021091.D
 Acq On : 22 Apr 2021 12:44
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.870	1189	1191	1193	rVB2	1136	456	0.02%	0.002%
38	4.896	1196	1199	1200	rBV3	552	315	0.01%	0.001%
39	4.966	1219	1221	1227	rVB5	1666	1196	0.04%	0.006%
40	5.047	1229	1246	1278	rBV2	1076292	2775731	100.00%	12.973%
41	5.478	1378	1380	1382	rBV2	867	455	0.02%	0.002%
42	5.548	1399	1402	1407	rVB4	1263	754	0.03%	0.004%
43	5.619	1411	1424	1451	rBV	847824	1694722	61.05%	7.921%
44	5.905	1505	1513	1514	rBV6	7020	6822	0.25%	0.032%
45	5.979	1533	1536	1539	rBV3	1379	908	0.03%	0.004%
46	6.072	1550	1565	1590	rBV2	617304	1250074	45.04%	5.842%
47	6.288	1630	1632	1634	rBV2	950	578	0.02%	0.003%
48	6.375	1657	1659	1663	rBV4	566	479	0.02%	0.002%
49	6.452	1680	1683	1686	rBV4	1209	1053	0.04%	0.005%
50	6.513	1700	1702	1704	rBV2	540	237	0.01%	0.001%
51	6.532	1706	1708	1710	rBV2	570	217	0.01%	0.001%
52	6.545	1710	1712	1714	rBV	798	375	0.01%	0.002%
53	6.629	1736	1738	1740	rBV2	604	353	0.01%	0.002%
54	6.744	1771	1774	1776	rVB	843	445	0.02%	0.002%
55	6.757	1776	1778	1781	rBV2	583	322	0.01%	0.002%
56	6.780	1783	1785	1790	rVB3	918	480	0.02%	0.002%
57	6.873	1812	1814	1816	rBV	405	207	0.01%	0.001%
58	6.989	1838	1850	1873	rBV	346620	639376	23.03%	2.988%
59	7.317	1940	1952	1971	rBV	1305126	2253783	81.20%	10.533%
60	7.625	2037	2048	2071	rBV	246737	438611	15.80%	2.050%
61	7.886	2126	2129	2131	rBV3	895	657	0.02%	0.003%
62	7.899	2131	2133	2135	rVB2	939	389	0.01%	0.002%
63	7.979	2155	2158	2159	rBV	1218	579	0.02%	0.003%
64	8.037	2174	2176	2179	rBV2	968	791	0.03%	0.004%
65	8.092	2182	2193	2228	rBV	649879	1195504	43.07%	5.587%
66	8.612	2353	2355	2360	rVB5	969	488	0.02%	0.002%
67	8.760	2399	2401	2404	rVB4	467	164	0.01%	0.001%
68	8.786	2407	2409	2414	rVB4	629	254	0.01%	0.001%
69	8.857	2418	2431	2463	rBV	1251221	2065988	74.43%	9.656%
70	9.243	2549	2551	2552	rBV	794	283	0.01%	0.001%
71	9.272	2556	2560	2567	rBV4	921	1071	0.04%	0.005%
72	9.516	2634	2636	2639	rBV	643	457	0.02%	0.002%
73	9.558	2643	2649	2652	rBV5	1279	1428	0.05%	0.007%
74	9.612	2663	2666	2668	rBV3	910	483	0.02%	0.002%
75	9.786	2717	2720	2721	rBV2	619	345	0.01%	0.002%
76	9.847	2735	2739	2743	rBV3	700	691	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021091.D
 Acq On : 22 Apr 2021 12:44
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.892	2750	2753	2756	rBV2	436	387	0.01%	0.002%
78	10.095	2813	2816	2820	rVB3	1018	602	0.02%	0.003%
79	10.130	2820	2827	2836	rVB3	6266	9280	0.33%	0.043%
80	10.220	2843	2855	2874	rBV	892919	1409839	50.79%	6.589%
81	10.577	2962	2966	2968	rBV4	1444	1301	0.05%	0.006%
82	10.751	3015	3020	3022	rBV3	1036	1020	0.04%	0.005%
83	10.847	3048	3050	3052	rBV3	1014	539	0.02%	0.003%
84	10.921	3067	3073	3084	rVB8	5676	8113	0.29%	0.038%
85	10.982	3090	3092	3096	rVB2	714	365	0.01%	0.002%
86	11.005	3097	3099	3101	rBV2	623	351	0.01%	0.002%
87	11.030	3105	3107	3108	rBV2	722	295	0.01%	0.001%
88	11.156	3137	3146	3147	rBV6	2467	3111	0.11%	0.015%
89	11.201	3155	3160	3162	rBV5	1899	1861	0.07%	0.009%
90	11.255	3165	3177	3210	rBV	1244464	1955342	70.44%	9.139%
91	11.632	3282	3294	3312	rBV	1325156	2100976	75.69%	9.819%
92	11.982	3401	3403	3405	rBV2	658	279	0.01%	0.001%
93	12.056	3423	3426	3431	rVB4	1409	1107	0.04%	0.005%
94	12.140	3450	3452	3456	rBV3	682	373	0.01%	0.002%
95	12.390	3525	3530	3533	rBV3	1305	1148	0.04%	0.005%
96	12.654	3608	3612	3613	rBV4	2206	1326	0.05%	0.006%
97	13.271	3800	3804	3806	rBV4	2330	1798	0.06%	0.008%
98	13.831	3975	3978	3984	rBV4	1282	1170	0.04%	0.005%
99	13.915	3999	4004	4008	rBV2	1536	1605	0.06%	0.008%
100	14.320	4127	4130	4133	rBV4	1571	1077	0.04%	0.005%




Sum of corrected areas: 21396527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021091.D
Acq On : 22 Apr 2021 12:44
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

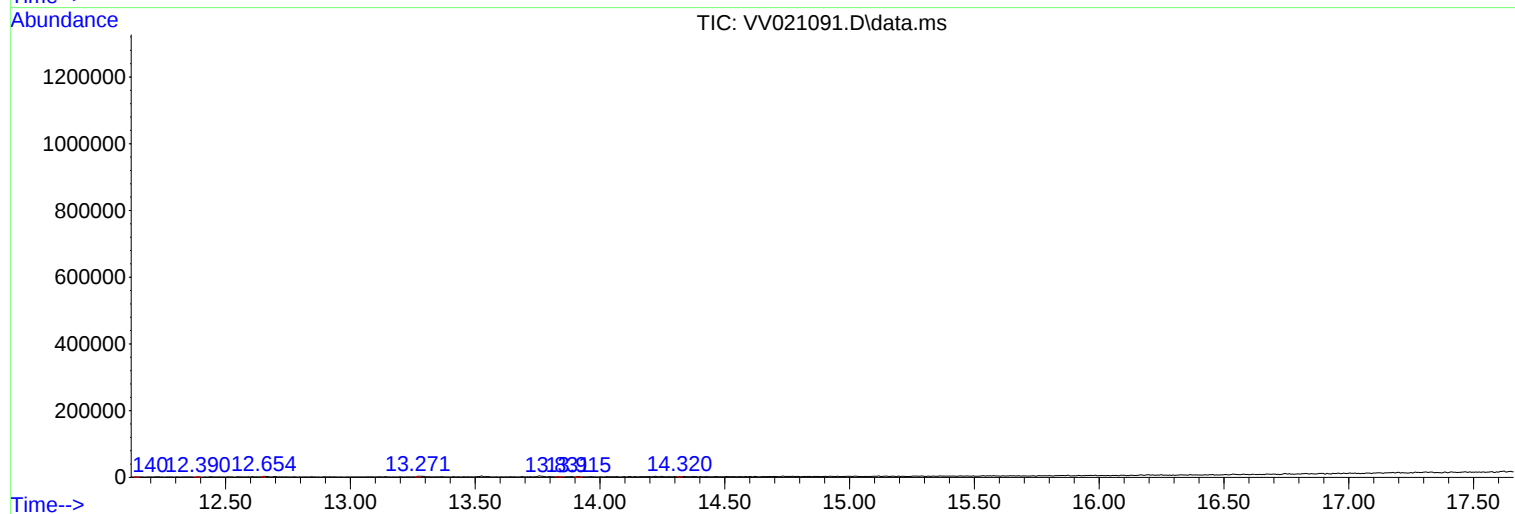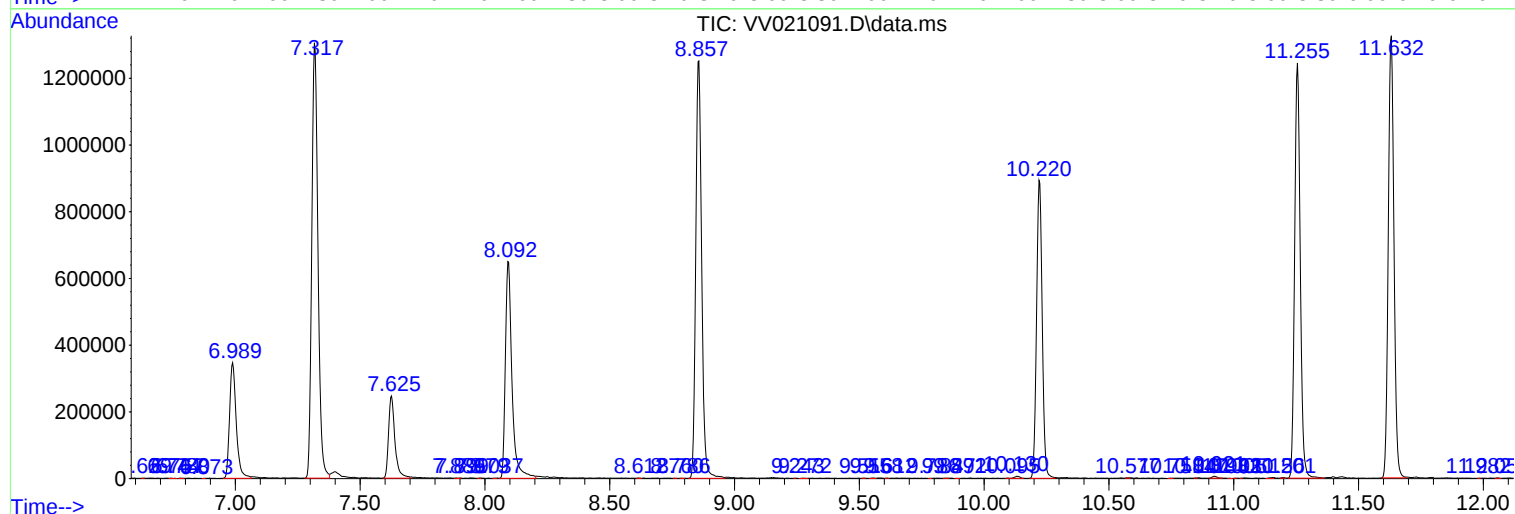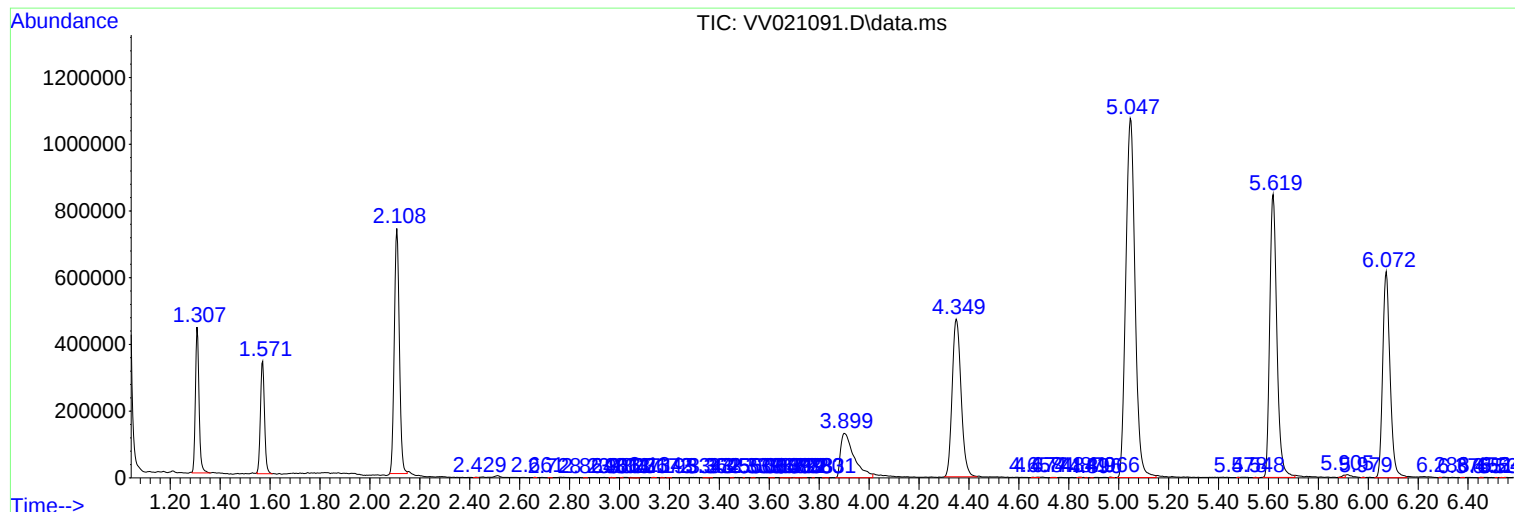

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021091.D
Acq On : 22 Apr 2021 12:44
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021091.D
Acq On : 22 Apr 2021 12:44
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
