

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V042221\
 Data File : VV021092.D
 Acq On : 22 Apr 2021 13:16
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	359377	365260	6.43%	1.451%
2	1.568	158	164	174	rVB	269890	304261	5.36%	1.209%
3	2.108	322	332	361	rVB	622259	927302	16.34%	3.684%
4	2.851	558	563	567	rBV4	819	909	0.02%	0.004%
5	2.947	591	593	594	rBV	427	181	0.00%	0.001%
6	2.989	604	606	607	rBV	540	239	0.00%	0.001%
7	3.214	674	676	678	rVB2	565	193	0.00%	0.001%
8	3.265	690	692	694	rBV	408	187	0.00%	0.001%
9	3.288	697	699	703	rVB	1311	696	0.01%	0.003%
10	3.307	703	705	707	rBV2	710	307	0.01%	0.001%
11	3.378	725	727	730	rBV3	699	439	0.01%	0.002%
12	3.397	730	733	734	rBV	680	372	0.01%	0.001%
13	3.606	794	798	799	rBV2	783	491	0.01%	0.002%
14	3.616	799	801	807	rVB3	1110	1003	0.02%	0.004%
15	3.654	809	813	815	rBV2	252	206	0.00%	0.001%
16	3.667	815	817	821	rBV3	452	290	0.01%	0.001%
17	3.728	833	836	838	rBV3	1085	692	0.01%	0.003%
18	3.854	870	875	878	rVB3	545	435	0.01%	0.002%
19	3.912	878	893	925	rBV2	103108	407597	7.18%	1.620%
20	4.285	1006	1009	1011	rBV3	1578	981	0.02%	0.004%
21	4.349	1014	1029	1057	rVB	383396	952654	16.78%	3.785%
22	4.632	1113	1117	1120	rVB3	1024	678	0.01%	0.003%
23	4.654	1120	1124	1126	rBV4	688	499	0.01%	0.002%
24	4.889	1195	1197	1198	rVB	451	130	0.00%	0.001%
25	4.902	1198	1201	1204	rBV	789	467	0.01%	0.002%
26	4.941	1210	1213	1214	rBV	713	381	0.01%	0.002%
27	4.970	1219	1222	1224	rBV3	710	421	0.01%	0.002%
28	5.047	1229	1246	1277	rBV2	886657	2328317	41.02%	9.251%
29	5.555	1400	1404	1405	rBV2	1085	687	0.01%	0.003%
30	5.619	1411	1424	1455	rBV	617236	1256663	22.14%	4.993%
31	5.915	1503	1516	1547	rBV	1352612	2659883	46.86%	10.569%
32	6.072	1553	1565	1587	rVB	486636	997699	17.58%	3.964%
33	6.365	1654	1656	1659	rVB2	1272	732	0.01%	0.003%
34	6.458	1683	1685	1686	rBV	915	457	0.01%	0.002%
35	6.539	1706	1710	1713	rBV2	1117	864	0.02%	0.003%
36	6.687	1754	1756	1758	rBV2	793	268	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021092.D
 Acq On : 22 Apr 2021 13:16
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.703	1758	1761	1762	rBV2	867	480	0.01%	0.002%
38	6.744	1772	1774	1776	rBV	687	384	0.01%	0.002%
39	6.789	1786	1788	1794	rVB4	1074	945	0.02%	0.004%
40	6.834	1799	1802	1805	rBV3	490	336	0.01%	0.001%
41	6.886	1816	1818	1820	rBV2	592	385	0.01%	0.002%
42	6.918	1825	1828	1829	rBV	520	272	0.00%	0.001%
43	6.989	1839	1850	1870	rBV	282218	513891	9.05%	2.042%
44	7.262	1933	1935	1938	rVB3	1245	521	0.01%	0.002%
45	7.317	1941	1952	1972	rBV	1050707	1827617	32.19%	7.262%
46	7.625	2038	2048	2071	rBV	194171	351028	6.18%	1.395%
47	7.780	2094	2096	2099	rBV4	1155	647	0.01%	0.003%
48	7.873	2121	2125	2129	rBV4	1261	1196	0.02%	0.005%
49	7.976	2143	2157	2183	rBV	3433019	5676721	100.00%	22.556%
50	8.092	2184	2193	2213	rBV	481989	875783	15.43%	3.480%
51	8.574	2340	2343	2345	rBV2	933	646	0.01%	0.003%
52	8.622	2355	2358	2361	rVB3	1014	568	0.01%	0.002%
53	8.645	2361	2365	2368	rBV	628	599	0.01%	0.002%
54	8.789	2405	2410	2411	rBV2	704	586	0.01%	0.002%
55	8.854	2419	2430	2451	rBV	926791	1493762	26.31%	5.935%
56	9.082	2497	2501	2502	rBV4	892	601	0.01%	0.002%
57	9.236	2547	2549	2554	rVB4	723	597	0.01%	0.002%
58	9.265	2555	2558	2559	rBV2	785	483	0.01%	0.002%
59	9.288	2562	2565	2567	rVB2	805	414	0.01%	0.002%
60	9.301	2567	2569	2571	rBV	444	249	0.00%	0.001%
61	9.387	2592	2596	2598	rBV3	642	505	0.01%	0.002%
62	9.455	2615	2617	2621	rBV2	667	477	0.01%	0.002%
63	9.500	2627	2631	2636	rBV4	1313	1234	0.02%	0.005%
64	9.561	2643	2650	2654	rBV5	1610	1875	0.03%	0.007%
65	9.728	2699	2702	2704	rBV	779	444	0.01%	0.002%
66	9.796	2721	2723	2726	rBV5	811	374	0.01%	0.001%
67	9.873	2744	2747	2749	rBV	625	362	0.01%	0.001%
68	10.008	2787	2789	2791	rBV2	542	246	0.00%	0.001%
69	10.085	2810	2813	2816	rBV2	553	508	0.01%	0.002%
70	10.220	2843	2855	2880	rBV	710940	1118211	19.70%	4.443%
71	10.452	2925	2927	2930	rBV2	826	434	0.01%	0.002%
72	10.719	3009	3010	3011	rBV2	516	147	0.00%	0.001%
73	10.805	3034	3037	3039	rBV	876	430	0.01%	0.002%
74	10.918	3067	3072	3083	rVB9	4066	7185	0.13%	0.029%
75	11.034	3106	3108	3109	rBV	1151	421	0.01%	0.002%
76	11.255	3166	3177	3197	rBV	910342	1404817	24.75%	5.582%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021092.D
 Acq On : 22 Apr 2021 13:16
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	11.429	3228	3231	3233	rBV3	2607	1619	0.03%	0.006%
78	11.506	3253	3255	3257	rBV2	693	332	0.01%	0.001%
79	11.632	3280	3294	3317	rBV	1053972	1659496	29.23%	6.594%
80	11.767	3333	3336	3339	rBV2	1347	977	0.02%	0.004%
81	11.908	3377	3380	3384	rBV4	1248	762	0.01%	0.003%
82	12.053	3422	3425	3426	rBV2	910	496	0.01%	0.002%
83	12.760	3642	3645	3647	rBV2	1142	608	0.01%	0.002%
84	12.808	3659	3660	3662	rBV2	618	203	0.00%	0.001%
85	12.882	3681	3683	3686	rBV3	1194	775	0.01%	0.003%
86	12.934	3694	3699	3703	rBV4	1396	1582	0.03%	0.006%
87	13.252	3796	3798	3802	rBV3	876	875	0.02%	0.003%
88	13.934	4008	4010	4013	rVB2	1543	794	0.01%	0.003%




Sum of corrected areas: 25167741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021092.D
Acq On : 22 Apr 2021 13:16
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

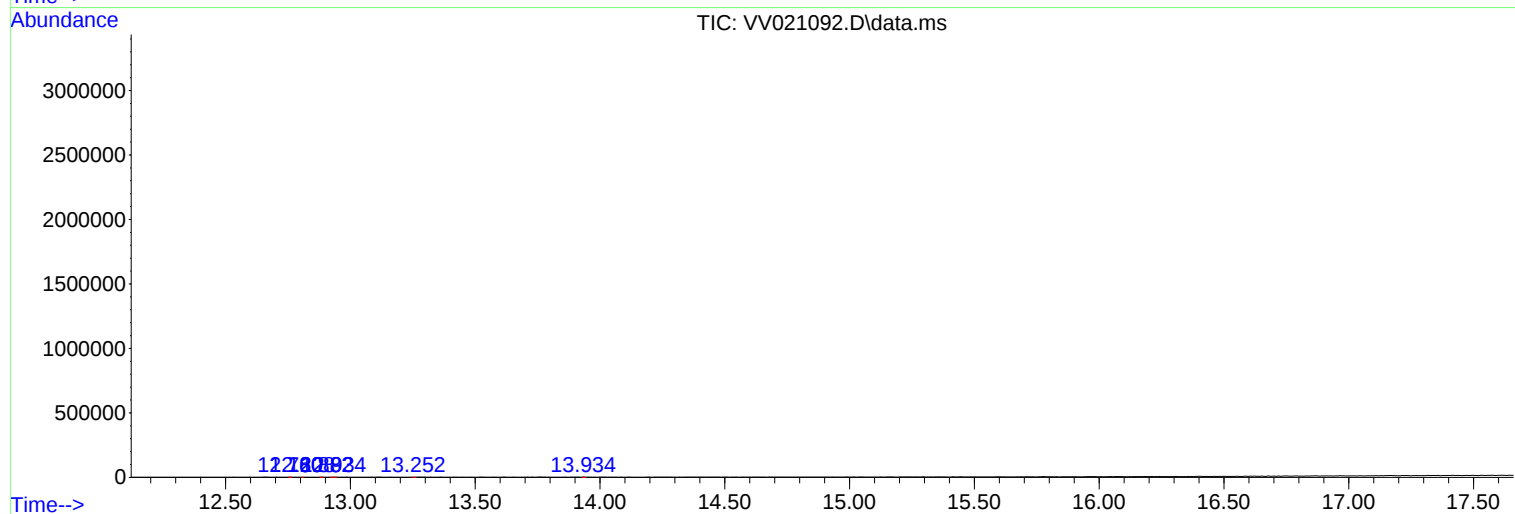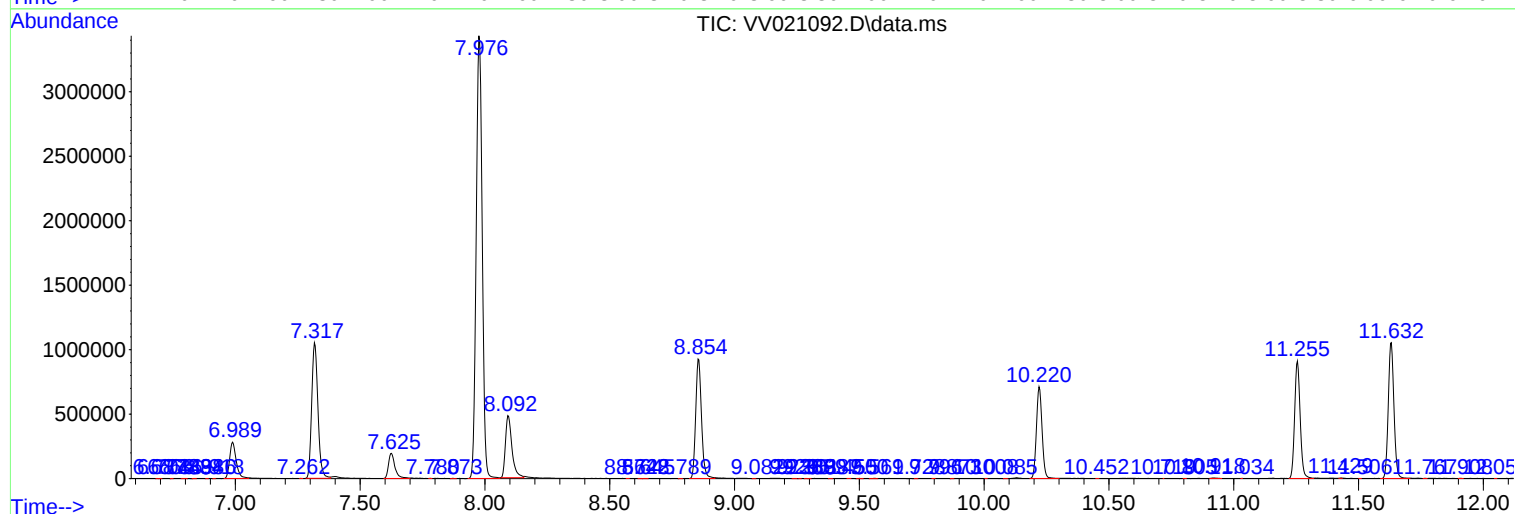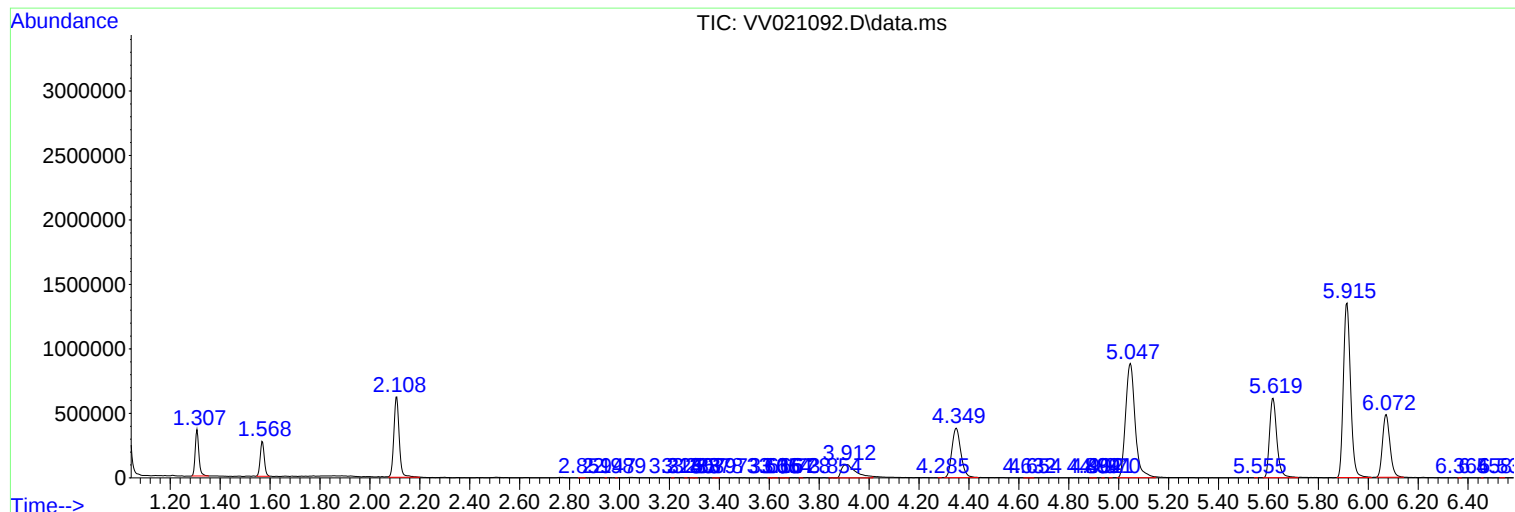

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021092.D
Acq On : 22 Apr 2021 13:16
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021092.D
Acq On : 22 Apr 2021 13:16
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
