

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021093.D
 Acq On : 22 Apr 2021 13:39
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	401410	408509	1.37%	0.509%
2	1.568	157	164	175	rVB	309047	344544	1.16%	0.429%
3	2.108	322	332	345	rBV	685777	981829	3.29%	1.222%
4	2.847	561	562	564	rBV2	511	271	0.00%	0.000%
5	2.892	573	576	579	rBV2	781	577	0.00%	0.001%
6	2.921	583	585	592	rVB2	384	365	0.00%	0.000%
7	2.989	602	606	610	rBV4	783	490	0.00%	0.001%
8	3.044	619	623	626	rBV3	600	438	0.00%	0.001%
9	3.098	636	640	641	rBV	427	278	0.00%	0.000%
10	3.108	641	643	647	rVV2	724	414	0.00%	0.001%
11	3.146	653	655	659	rBV3	608	352	0.00%	0.000%
12	3.240	681	684	685	rBV2	605	234	0.00%	0.000%
13	3.288	694	699	702	rBV2	469	305	0.00%	0.000%
14	3.326	704	711	713	rBV3	981	828	0.00%	0.001%
15	3.349	713	718	720	rVB	360	296	0.00%	0.000%
16	3.381	724	728	730	rBV3	954	822	0.00%	0.001%
17	3.413	735	738	741	rVB	700	371	0.00%	0.000%
18	3.462	750	753	754	rBV2	357	231	0.00%	0.000%
19	3.471	754	756	758	rBV3	511	289	0.00%	0.000%
20	3.526	771	773	778	rVB2	1145	612	0.00%	0.001%
21	3.555	780	782	784	rBV2	582	344	0.00%	0.000%
22	3.597	793	795	798	rVB2	492	272	0.00%	0.000%
23	3.680	817	821	824	rBV3	933	595	0.00%	0.001%
24	3.709	824	830	831	rBV4	609	626	0.00%	0.001%
25	3.767	845	848	852	rBV3	704	531	0.00%	0.001%
26	3.790	852	855	857	rBV	410	237	0.00%	0.000%
27	3.844	870	872	875	rVB	974	536	0.00%	0.001%
28	3.908	875	892	940	rBV2	137789	609946	2.05%	0.759%
29	4.352	1015	1030	1058	rVB2	446004	1106407	3.71%	1.377%
30	4.716	1139	1143	1144	rBV2	804	524	0.00%	0.001%
31	4.867	1188	1190	1192	rBV2	465	287	0.00%	0.000%
32	4.896	1197	1199	1202	rBV2	459	317	0.00%	0.000%
33	4.931	1208	1210	1213	rBV3	949	506	0.00%	0.001%
34	5.047	1230	1246	1259	rBV3	1019781	2606780	8.74%	3.245%
35	5.420	1358	1362	1367	rBV5	1038	1105	0.00%	0.001%
36	5.445	1367	1370	1371	rBV2	960	532	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021093.D
 Acq On : 22 Apr 2021 13:39
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.548	1399	1402	1405	rVB4	1100	692	0.00%	0.001%
38	5.564	1405	1407	1410	rBV3	831	556	0.00%	0.001%
39	5.619	1413	1424	1448	rBV	497750	996007	3.34%	1.240%
40	5.912	1506	1515	1526	rBV5	12675	26891	0.09%	0.033%
41	5.992	1538	1540	1542	rBV3	946	476	0.00%	0.001%
42	6.072	1552	1565	1590	rBV	568359	1157984	3.88%	1.442%
43	6.256	1620	1622	1627	rBV4	1183	817	0.00%	0.001%
44	6.387	1661	1663	1665	rBV3	1105	429	0.00%	0.001%
45	6.465	1683	1687	1691	rBV4	845	930	0.00%	0.001%
46	6.494	1694	1696	1699	rVV2	872	414	0.00%	0.001%
47	6.542	1709	1711	1713	rVB3	903	295	0.00%	0.000%
48	6.600	1727	1729	1732	rBV2	502	228	0.00%	0.000%
49	6.619	1732	1735	1737	rBV3	491	302	0.00%	0.000%
50	6.744	1772	1774	1776	rBV3	915	502	0.00%	0.001%
51	6.834	1799	1802	1803	rBV2	892	558	0.00%	0.001%
52	6.860	1807	1810	1812	rVV2	723	345	0.00%	0.000%
53	6.889	1816	1819	1824	rBV2	1062	1026	0.00%	0.001%
54	6.989	1839	1850	1875	rBV	328531	605066	2.03%	0.753%
55	7.320	1940	1953	1970	rBV	1241587	2141793	7.18%	2.667%
56	7.625	2037	2048	2078	rBV	231675	415957	1.39%	0.518%
57	7.947	2141	2148	2152	rBV6	2616	3717	0.01%	0.005%
58	8.034	2172	2175	2176	rBV3	772	476	0.00%	0.001%
59	8.092	2183	2193	2230	rBV	598043	1072492	3.60%	1.335%
60	8.558	2335	2338	2340	rBV2	627	350	0.00%	0.000%
61	8.625	2355	2359	2361	rBV2	823	653	0.00%	0.001%
62	8.738	2391	2394	2396	rBV2	831	485	0.00%	0.001%
63	8.805	2411	2415	2417	rBV3	592	420	0.00%	0.001%
64	8.883	2417	2439	2487	rBV2	6408420	11336871	38.02%	14.115%
65	9.146	2513	2521	2536	rBV2	3980	8697	0.03%	0.011%
66	9.214	2536	2542	2543	rBV4	1428	1321	0.00%	0.002%
67	9.487	2624	2627	2629	rBV2	600	423	0.00%	0.001%
68	9.526	2637	2639	2640	rBV	677	252	0.00%	0.000%
69	9.622	2667	2669	2670	rBV	625	262	0.00%	0.000%
70	9.651	2676	2678	2685	rVB4	749	823	0.00%	0.001%
71	9.680	2685	2687	2692	rBV5	883	817	0.00%	0.001%
72	9.738	2701	2705	2706	rBV2	908	563	0.00%	0.001%
73	9.786	2718	2720	2722	rBV3	650	269	0.00%	0.000%
74	9.850	2738	2740	2746	rVB3	943	582	0.00%	0.001%
75	9.879	2746	2749	2754	rBV2	475	470	0.00%	0.001%
76	9.969	2775	2777	2780	rBV2	863	506	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021093.D
 Acq On : 22 Apr 2021 13:39
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.985	2780	2782	2785	rBV2	598	460	0.00%	0.001%
78	10.053	2799	2803	2805	rVB5	1062	717	0.00%	0.001%
79	10.069	2805	2808	2809	rBV	765	358	0.00%	0.000%
80	10.130	2821	2827	2836	rVB7	5899	7348	0.02%	0.009%
81	10.220	2843	2855	2876	rBV	840068	1306925	4.38%	1.627%
82	10.535	2949	2953	2956	rBV2	1241	888	0.00%	0.001%
83	10.641	2983	2986	2988	rBV2	677	347	0.00%	0.000%
84	10.690	2999	3001	3004	rBV2	675	331	0.00%	0.000%
85	10.924	3065	3074	3084	rVV8	6033	9659	0.03%	0.012%
86	11.021	3102	3104	3106	rBV3	880	444	0.00%	0.001%
87	11.188	3144	3156	3167	rBV	791912	1219542	4.09%	1.518%
88	11.278	3168	3184	3208	rVB2	7814647	13030045	43.69%	16.223%
89	11.651	3282	3300	3321	rBV2	18468382	29820711	100.00%	37.127%
90	12.281	3494	3496	3499	rBV4	1055	744	0.00%	0.001%
91	12.407	3526	3535	3550	rVB2	27821	45402	0.15%	0.057%
92	12.648	3600	3610	3629	rVB2	113636	186525	0.63%	0.232%
93	12.757	3637	3644	3655	rVB4	28941	43896	0.15%	0.055%
94	12.953	3703	3705	3709	rBV4	1042	858	0.00%	0.001%
95	12.995	3715	3718	3720	rBV2	1199	765	0.00%	0.001%
96	13.169	3770	3772	3775	rBV3	1123	605	0.00%	0.001%
97	13.268	3790	3803	3834	rBV	4923979	7349449	24.65%	9.150%
98	13.751	3941	3953	3973	rBV	2017174	3051847	10.23%	3.800%
99	14.162	4073	4081	4092	rVB4	26583	45877	0.15%	0.057%
100	15.406	4458	4468	4481	rVB2	216546	343144	1.15%	0.427%



Sum of corrected areas: 80320204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021093.D
Acq On : 22 Apr 2021 13:39
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

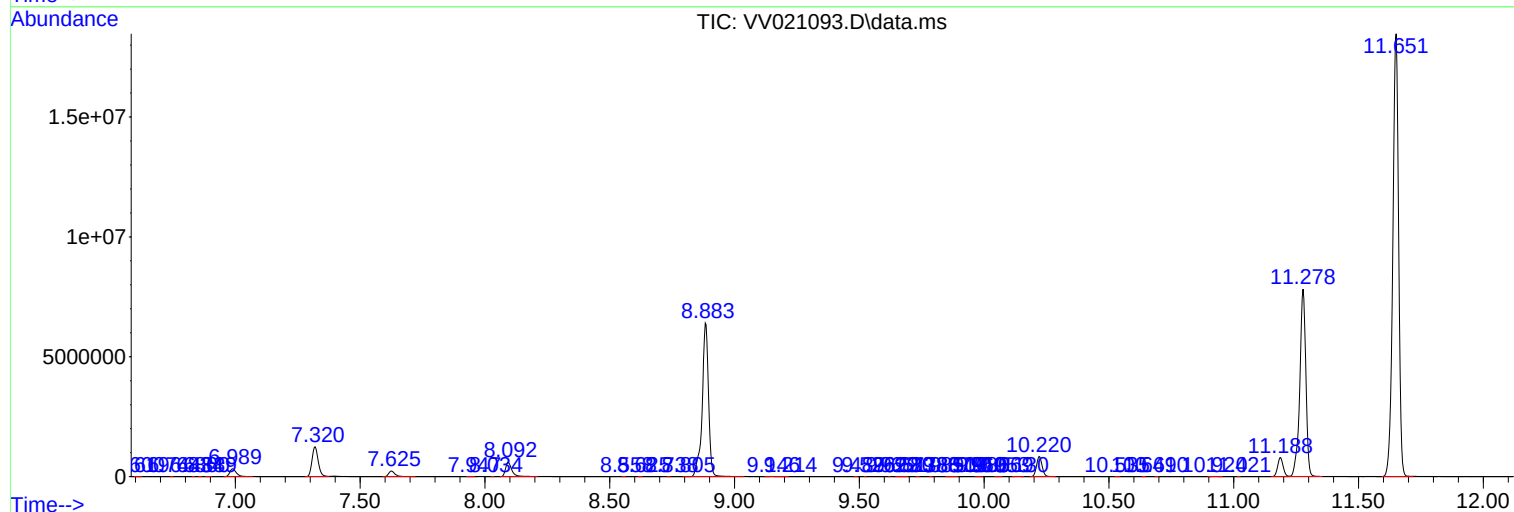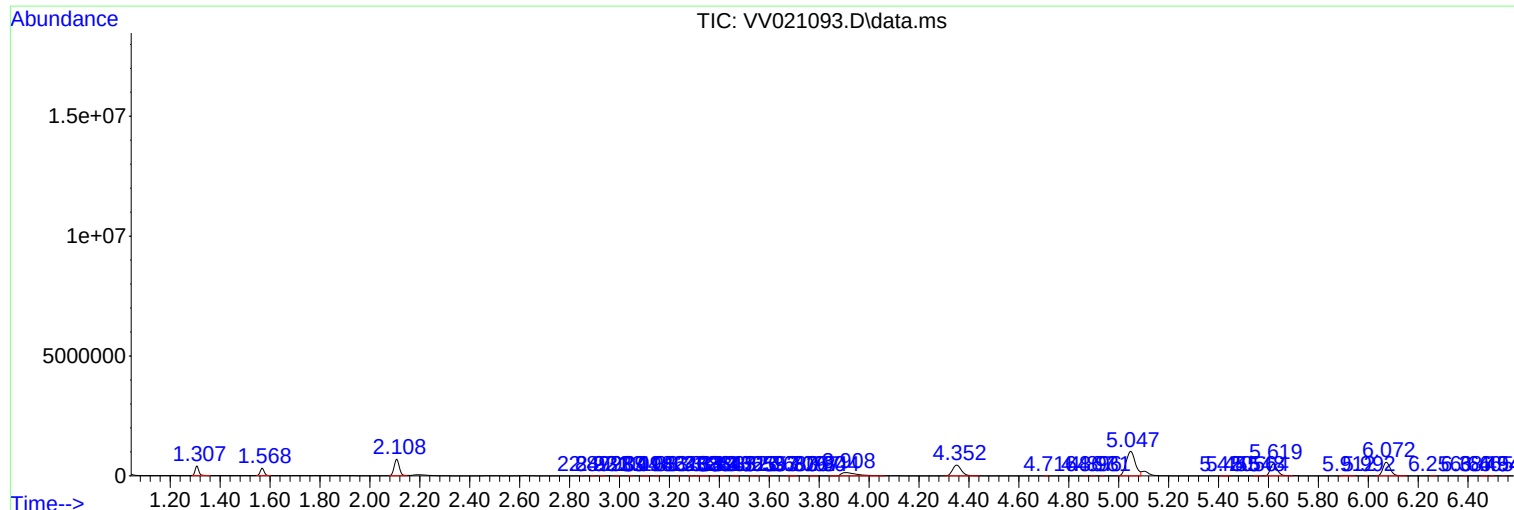

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021093.D
Acq On : 22 Apr 2021 13:39
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021093.D
Acq On : 22 Apr 2021 13:39
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
