

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021095.D
 Acq On : 22 Apr 2021 14:32
 Operator : SY/MD
 Sample : M2067-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	396083	395697	15.10%	1.832%
2	1.568	158	164	178	rVB	301704	343556	13.11%	1.591%
3	2.108	323	332	343	rBV	675589	954146	36.42%	4.419%
4	2.429	429	432	434	rBV3	1292	724	0.03%	0.003%
5	2.510	450	457	465	rBV6	5681	8445	0.32%	0.039%
6	2.593	480	483	484	rBV	637	348	0.01%	0.002%
7	2.770	518	538	567	rBV	664827	1453401	55.48%	6.731%
8	2.963	595	598	602	rBV3	1413	1037	0.04%	0.005%
9	2.982	602	604	607	rVB2	735	398	0.02%	0.002%
10	3.072	630	632	637	rVB3	962	633	0.02%	0.003%
11	3.111	641	644	645	rBV3	922	416	0.02%	0.002%
12	3.201	669	672	673	rBV2	707	431	0.02%	0.002%
13	3.227	677	680	682	rBV3	746	458	0.02%	0.002%
14	3.294	687	701	706	rBV4	4830	9736	0.37%	0.045%
15	3.420	738	740	741	rBV	517	278	0.01%	0.001%
16	3.458	748	752	756	rBV3	606	613	0.02%	0.003%
17	3.552	776	781	783	rBV3	591	578	0.02%	0.003%
18	3.584	788	791	793	rBV3	637	307	0.01%	0.001%
19	3.600	793	796	798	rBV3	688	508	0.02%	0.002%
20	3.757	843	845	849	rBV2	608	392	0.01%	0.002%
21	3.783	850	853	854	rBV3	890	529	0.02%	0.002%
22	3.908	881	892	938	rBV2	104392	463967	17.71%	2.149%
23	4.349	1014	1029	1053	rBV	434692	1073041	40.96%	4.969%
24	4.719	1141	1144	1148	rBV5	711	698	0.03%	0.003%
25	4.793	1163	1167	1169	rBV	620	480	0.02%	0.002%
26	4.870	1188	1191	1192	rBV2	527	287	0.01%	0.001%
27	4.924	1203	1208	1210	rBV3	949	790	0.03%	0.004%
28	4.963	1216	1220	1222	rVB2	873	621	0.02%	0.003%
29	5.047	1230	1246	1279	rBV2	1009884	2619829	100.00%	12.133%
30	5.452	1370	1372	1376	rBV2	620	429	0.02%	0.002%
31	5.532	1395	1397	1401	rBV5	694	456	0.02%	0.002%
32	5.551	1401	1403	1408	rVB2	788	623	0.02%	0.003%
33	5.574	1408	1410	1411	rBV	742	376	0.01%	0.002%
34	5.619	1411	1424	1453	rBV	857216	1729004	66.00%	8.007%
35	6.072	1553	1565	1587	rBV	548105	1116776	42.63%	5.172%
36	6.317	1638	1641	1643	rBV3	875	623	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021095.D
 Acq On : 22 Apr 2021 14:32
 Operator : SY/MD
 Sample : M2067-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.342	1647	1649	1653	rBV4	596	499	0.02%	0.002%
38	6.445	1679	1681	1686	rVB4	1156	834	0.03%	0.004%
39	6.471	1686	1689	1694	rVB4	913	732	0.03%	0.003%
40	6.500	1694	1698	1702	rBV2	1380	1003	0.04%	0.005%
41	6.523	1702	1705	1707	rBV2	698	517	0.02%	0.002%
42	6.551	1712	1714	1715	rBV	767	281	0.01%	0.001%
43	6.593	1724	1727	1729	rBV3	808	475	0.02%	0.002%
44	6.670	1750	1751	1753	rVB2	820	311	0.01%	0.001%
45	6.760	1777	1779	1782	rBV2	753	547	0.02%	0.003%
46	6.812	1793	1795	1798	rVB	785	362	0.01%	0.002%
47	6.841	1801	1804	1805	rBV	448	275	0.01%	0.001%
48	6.886	1816	1818	1823	rVB2	546	390	0.01%	0.002%
49	6.937	1830	1834	1837	rBV2	787	634	0.02%	0.003%
50	6.989	1839	1850	1878	rBV2	325292	601131	22.95%	2.784%
51	7.188	1910	1912	1916	rBV3	725	543	0.02%	0.003%
52	7.317	1940	1952	1972	rBV	1175084	2034701	77.67%	9.423%
53	7.625	2038	2048	2068	rBV2	222080	387966	14.81%	1.797%
54	7.979	2155	2158	2161	rBV4	1651	1081	0.04%	0.005%
55	8.034	2170	2175	2177	rBV3	878	751	0.03%	0.003%
56	8.095	2183	2194	2212	rBV	580223	1049237	40.05%	4.859%
57	8.529	2327	2329	2335	rVB3	1030	545	0.02%	0.003%
58	8.567	2339	2341	2343	rVB2	1018	390	0.01%	0.002%
59	8.580	2343	2345	2348	rVB	693	348	0.01%	0.002%
60	8.606	2348	2353	2354	rBV3	1019	990	0.04%	0.005%
61	8.657	2367	2369	2371	rVB2	660	274	0.01%	0.001%
62	8.677	2371	2375	2376	rBV3	499	330	0.01%	0.002%
63	8.719	2383	2388	2392	rBV5	442	562	0.02%	0.003%
64	8.767	2401	2403	2406	rBV2	858	587	0.02%	0.003%
65	8.809	2414	2416	2419	rVB2	932	322	0.01%	0.001%
66	8.857	2419	2431	2453	rBV	1281146	2102860	80.27%	9.738%
67	9.120	2510	2513	2515	rBV3	1092	716	0.03%	0.003%
68	9.194	2533	2536	2539	rVB4	1369	864	0.03%	0.004%
69	9.210	2539	2541	2543	rBV2	637	298	0.01%	0.001%
70	9.243	2550	2551	2554	rBV	669	363	0.01%	0.002%
71	9.259	2554	2556	2559	rVB2	1040	480	0.02%	0.002%
72	9.391	2594	2597	2601	rBV3	733	466	0.02%	0.002%
73	9.442	2607	2613	2615	rVB3	872	936	0.04%	0.004%
74	9.465	2615	2620	2621	rBV2	854	802	0.03%	0.004%
75	9.587	2655	2658	2660	rVB3	890	441	0.02%	0.002%
76	9.648	2674	2677	2678	rBV2	443	267	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021095.D
 Acq On : 22 Apr 2021 14:32
 Operator : SY/MD
 Sample : M2067-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.735	2701	2704	2706	rBV	1132	677	0.03%	0.003%
78	10.027	2792	2795	2797	rBV	687	459	0.02%	0.002%
79	10.133	2822	2828	2834	rBV5	5203	6534	0.25%	0.030%
80	10.220	2841	2855	2873	rBV	819182	1280608	48.88%	5.931%
81	10.484	2930	2937	2939	rBV2	837	793	0.03%	0.004%
82	10.500	2939	2942	2946	rBV4	775	554	0.02%	0.003%
83	10.577	2961	2966	2969	rBV4	1475	1706	0.07%	0.008%
84	10.670	2993	2995	2998	rVB3	1158	501	0.02%	0.002%
85	10.686	2998	3000	3004	rBV2	623	389	0.01%	0.002%
86	10.754	3019	3021	3023	rBV2	1406	746	0.03%	0.003%
87	10.767	3023	3025	3031	rVB2	1104	703	0.03%	0.003%
88	10.821	3039	3042	3044	rBV2	1113	518	0.02%	0.002%
89	10.969	3086	3088	3092	rBV3	683	454	0.02%	0.002%
90	11.034	3104	3108	3111	rBV3	1580	1192	0.05%	0.006%
91	11.095	3124	3127	3130	rBV3	829	543	0.02%	0.003%
92	11.149	3135	3144	3150	rBV7	3346	5429	0.21%	0.025%
93	11.255	3165	3177	3209	rBV	1274587	1998296	76.28%	9.254%
94	11.493	3247	3251	3252	rBV3	847	637	0.02%	0.003%
95	11.632	3281	3294	3315	rBV	1206815	1913043	73.02%	8.859%
96	12.648	3608	3610	3614	rBV3	1034	641	0.02%	0.003%
97	12.693	3622	3624	3629	rBV4	977	724	0.03%	0.003%
98	13.333	3820	3823	3825	rBV2	638	343	0.01%	0.002%
99	13.972	4019	4022	4027	rBV6	1528	1569	0.06%	0.007%
100	14.770	4268	4270	4271	rBV	1286	593	0.02%	0.003%




Sum of corrected areas: 21593394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021095.D
Acq On : 22 Apr 2021 14:32
Operator : SY/MD
Sample : M2067-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

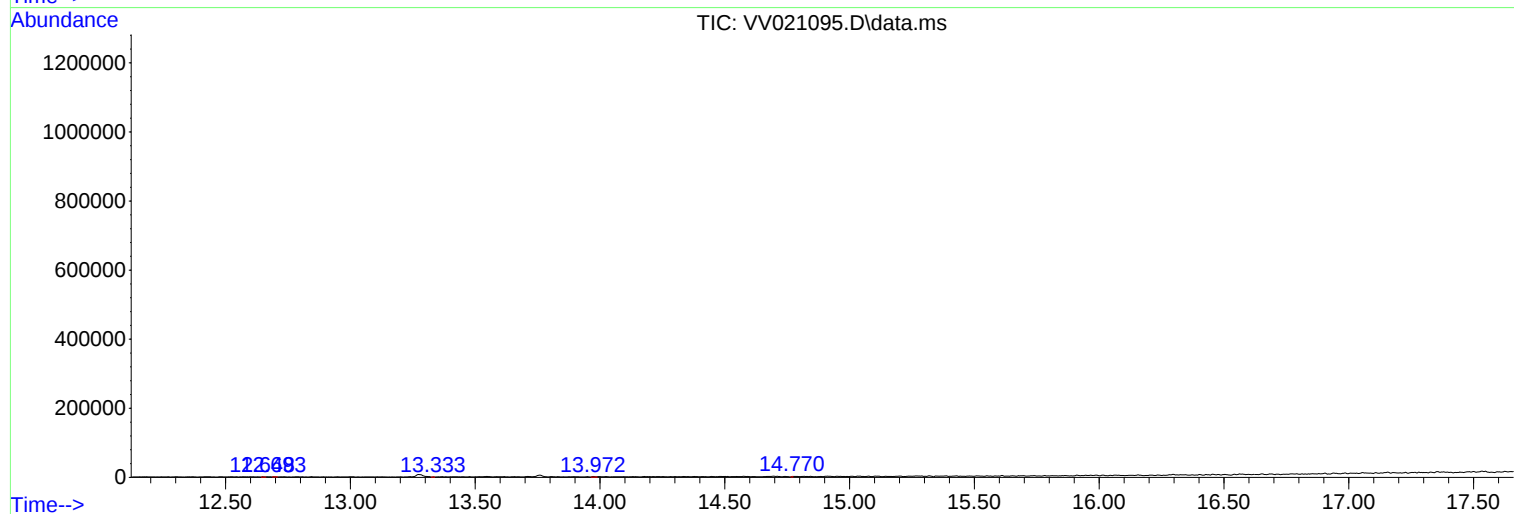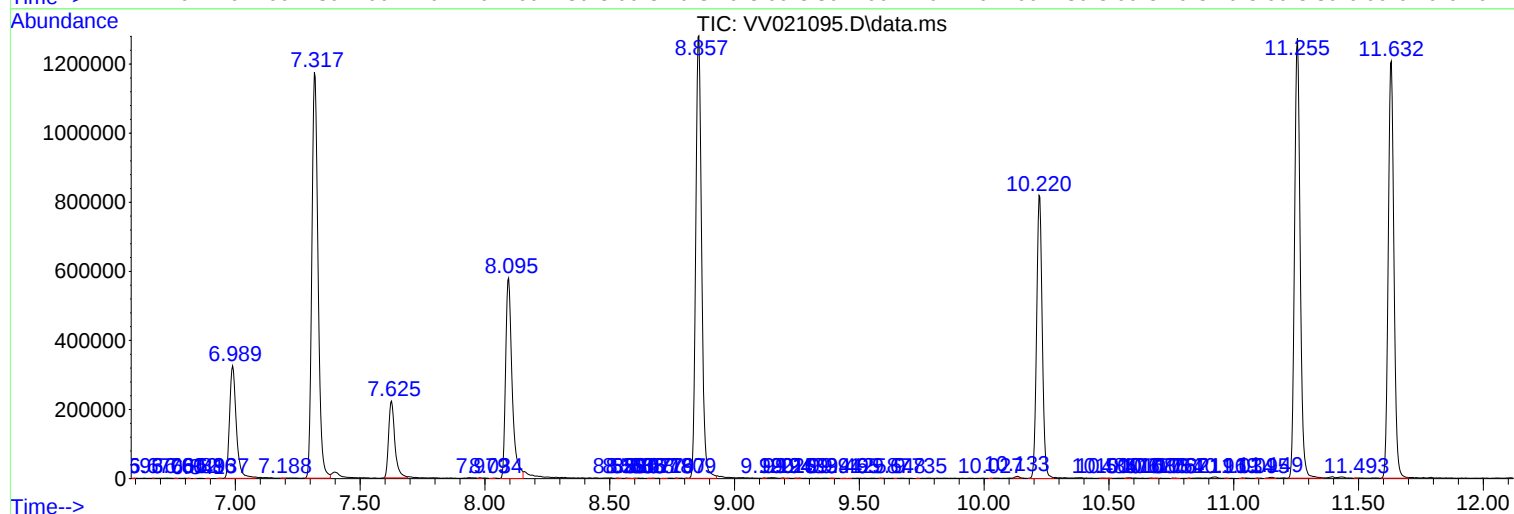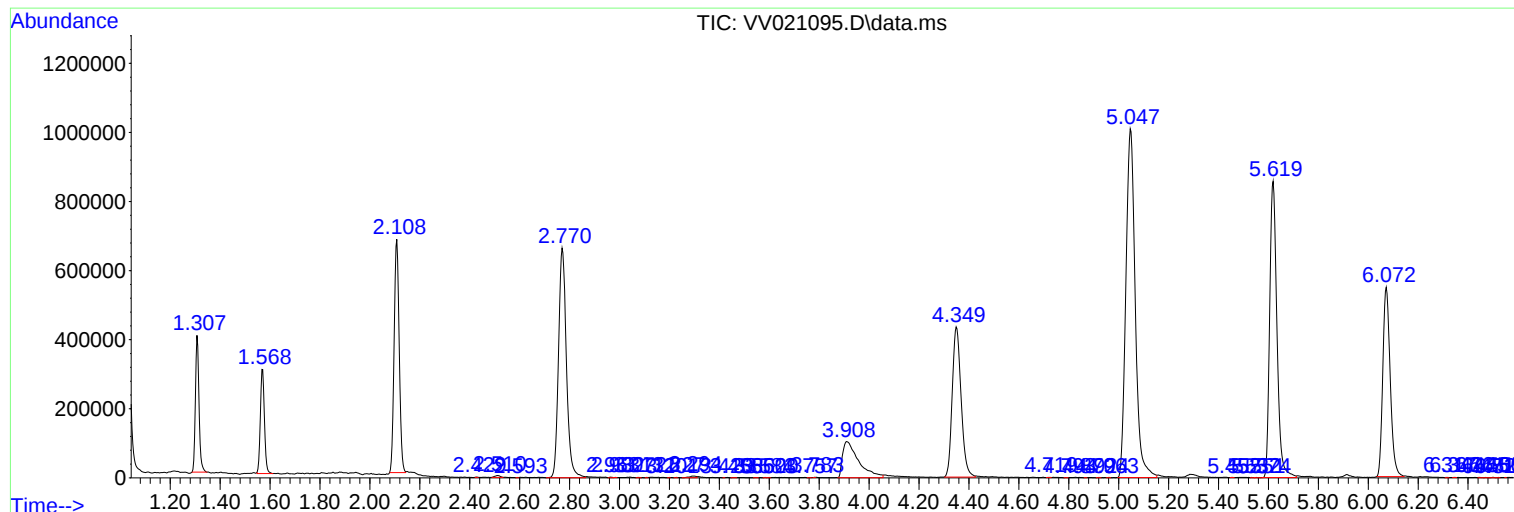

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021095.D
Acq On : 22 Apr 2021 14:32
Operator : SY/MD
Sample : M2067-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021095.D
Acq On : 22 Apr 2021 14:32
Operator : SY/MD
Sample : M2067-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
