

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021096.D
 Acq On : 22 Apr 2021 14:55
 Operator : SY/MD
 Sample : M2067-17DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	102	rVB	414934	421064	15.55%	1.821%
2	1.571	158	165	178	rVB	318872	368061	13.59%	1.591%
3	2.108	323	332	346	rBV	706478	997423	36.84%	4.313%
4	2.664	502	505	507	rBV	955	661	0.02%	0.003%
5	2.774	524	539	567	rBV	1142769	2464780	91.04%	10.658%
6	3.137	650	652	656	rBV4	567	403	0.01%	0.002%
7	3.211	671	675	678	rBV3	642	634	0.02%	0.003%
8	3.256	687	689	691	rVB2	516	239	0.01%	0.001%
9	3.269	691	693	694	rBV	421	158	0.01%	0.001%
10	3.343	713	716	719	rBV3	729	423	0.02%	0.002%
11	3.359	719	721	728	rVB4	788	853	0.03%	0.004%
12	3.388	728	730	735	rBV3	827	691	0.03%	0.003%
13	3.410	735	737	740	rBV2	437	261	0.01%	0.001%
14	3.449	748	749	755	rVB2	609	449	0.02%	0.002%
15	3.487	759	761	763	rBV	333	175	0.01%	0.001%
16	3.529	772	774	776	rVB	954	419	0.02%	0.002%
17	3.545	776	779	784	rBV3	591	523	0.02%	0.002%
18	3.568	784	786	789	rVB2	367	192	0.01%	0.001%
19	3.600	793	796	797	rBV	277	146	0.01%	0.001%
20	3.655	810	813	818	rBV2	510	568	0.02%	0.002%
21	3.738	835	839	842	rBV	886	659	0.02%	0.003%
22	3.770	847	849	852	rBV3	839	495	0.02%	0.002%
23	3.822	863	865	866	rBV3	662	287	0.01%	0.001%
24	3.847	870	873	874	rBV2	360	157	0.01%	0.001%
25	3.870	877	880	882	rBV	546	306	0.01%	0.001%
26	3.915	882	894	937	rBV	107683	507390	18.74%	2.194%
27	4.352	1014	1030	1059	rBV	470202	1152309	42.56%	4.982%
28	4.555	1090	1093	1097	rBV3	1292	1058	0.04%	0.005%
29	4.767	1156	1159	1162	rBV4	1238	880	0.03%	0.004%
30	4.809	1166	1172	1174	rBV4	1054	910	0.03%	0.004%
31	4.838	1179	1181	1183	rBV2	757	347	0.01%	0.002%
32	4.925	1205	1208	1212	rVB2	1135	688	0.03%	0.003%
33	4.944	1212	1214	1219	rBV4	894	527	0.02%	0.002%
34	4.966	1219	1221	1223	rBV4	575	225	0.01%	0.001%
35	5.050	1230	1247	1278	rBV2	1062437	2707475	100.00%	11.707%
36	5.365	1343	1345	1349	rVB4	1922	945	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042221\
 Data File : VW021096.D
 Acq On : 22 Apr 2021 14:55
 Operator : SY/MD
 Sample : M2067-17DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.478	1375	1380	1382	rBV3	850	641	0.02%	0.003%
38	5.561	1403	1406	1409	rVB2	908	489	0.02%	0.002%
39	5.577	1409	1411	1412	rBV2	630	313	0.01%	0.001%
40	5.619	1412	1424	1455	rBV	818007	1651151	60.98%	7.139%
41	6.072	1548	1565	1590	rBV	588332	1214354	44.85%	5.251%
42	6.339	1646	1648	1653	rVB3	1334	792	0.03%	0.003%
43	6.371	1656	1658	1659	rBV2	698	322	0.01%	0.001%
44	6.539	1706	1710	1715	rVB4	811	896	0.03%	0.004%
45	6.571	1719	1720	1723	rBV2	697	278	0.01%	0.001%
46	6.603	1729	1730	1732	rVB	734	268	0.01%	0.001%
47	6.616	1732	1734	1735	rBV	746	346	0.01%	0.001%
48	6.642	1740	1742	1745	rVB3	1086	648	0.02%	0.003%
49	6.674	1749	1752	1754	rBV3	947	506	0.02%	0.002%
50	6.712	1761	1764	1765	rBV	637	302	0.01%	0.001%
51	6.783	1783	1786	1790	rBV3	723	532	0.02%	0.002%
52	6.857	1807	1809	1811	rBV	666	356	0.01%	0.002%
53	6.921	1823	1829	1831	rBV2	827	623	0.02%	0.003%
54	6.989	1837	1850	1871	rBV	333109	611615	22.59%	2.645%
55	7.211	1914	1919	1921	rBV3	1123	965	0.04%	0.004%
56	7.320	1940	1953	1970	rBV	1249824	2159412	79.76%	9.337%
57	7.625	2038	2048	2076	rBV	235910	418073	15.44%	1.808%
58	7.831	2109	2112	2113	rBV2	807	457	0.02%	0.002%
59	8.095	2183	2194	2214	rBV	633596	1152439	42.57%	4.983%
60	8.519	2320	2326	2331	rBV8	1469	1419	0.05%	0.006%
61	8.645	2364	2365	2368	rBV3	727	358	0.01%	0.002%
62	8.754	2397	2399	2403	rVB3	1021	535	0.02%	0.002%
63	8.773	2403	2405	2406	rVB3	637	155	0.01%	0.001%
64	8.783	2406	2408	2409	rVB	575	156	0.01%	0.001%
65	8.793	2409	2411	2413	rVB2	818	301	0.01%	0.001%
66	8.809	2413	2416	2418	rBV3	890	545	0.02%	0.002%
67	8.857	2419	2431	2459	rBV	1216566	1984759	73.31%	8.582%
68	9.014	2478	2480	2481	rBV	1412	519	0.02%	0.002%
69	9.098	2504	2506	2510	rBV5	1475	1071	0.04%	0.005%
70	9.239	2548	2550	2552	rBV3	835	442	0.02%	0.002%
71	9.352	2583	2585	2588	rBV2	691	349	0.01%	0.002%
72	9.481	2623	2625	2627	rBV3	645	329	0.01%	0.001%
73	9.500	2629	2631	2634	rVB2	1114	534	0.02%	0.002%
74	9.561	2642	2650	2651	rBV2	1288	1255	0.05%	0.005%
75	9.712	2695	2697	2700	rBV2	647	255	0.01%	0.001%
76	9.802	2722	2725	2729	rVV2	649	387	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021096.D
 Acq On : 22 Apr 2021 14:55
 Operator : SY/MD
 Sample : M2067-17DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.834	2732	2735	2736	rVV	499	317	0.01%	0.001%
78	9.863	2740	2744	2747	rVB2	1052	705	0.03%	0.003%
79	9.937	2765	2767	2769	rBV2	886	464	0.02%	0.002%
80	9.998	2784	2786	2788	rVB	682	259	0.01%	0.001%
81	10.021	2791	2793	2796	rBV2	715	325	0.01%	0.001%
82	10.130	2821	2827	2836	rVB5	5944	8361	0.31%	0.036%
83	10.220	2842	2855	2875	rBV	876183	1384730	51.14%	5.987%
84	10.436	2918	2922	2926	rBV3	1176	1306	0.05%	0.006%
85	10.580	2960	2967	2972	rBV8	2494	3391	0.13%	0.015%
86	10.828	3041	3044	3046	rBV2	980	571	0.02%	0.002%
87	10.979	3088	3091	3093	rVB3	968	532	0.02%	0.002%
88	11.069	3115	3119	3122	rVB3	929	697	0.03%	0.003%
89	11.153	3140	3145	3150	rVB6	2620	3033	0.11%	0.013%
90	11.255	3165	3177	3198	rBV	1211828	1864926	68.88%	8.064%
91	11.426	3226	3230	3231	rBV3	2438	1948	0.07%	0.008%
92	11.628	3281	3293	3314	rBV	1272911	2003390	73.99%	8.663%
93	11.886	3371	3373	3376	rBV2	1053	622	0.02%	0.003%
94	12.037	3418	3420	3421	rBV2	544	196	0.01%	0.001%
95	12.291	3497	3499	3502	rBV2	646	413	0.02%	0.002%
96	12.333	3510	3512	3513	rBV	641	247	0.01%	0.001%
97	12.744	3638	3640	3641	rBV	487	165	0.01%	0.001%
98	12.886	3682	3684	3685	rBV2	791	264	0.01%	0.001%
99	13.278	3799	3806	3817	rVB2	4024	7883	0.29%	0.034%
100	14.252	4107	4109	4111	rBV2	971	452	0.02%	0.002%



Sum of corrected areas: 23127125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021096.D
Acq On : 22 Apr 2021 14:55
Operator : SY/MD
Sample : M2067-17DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

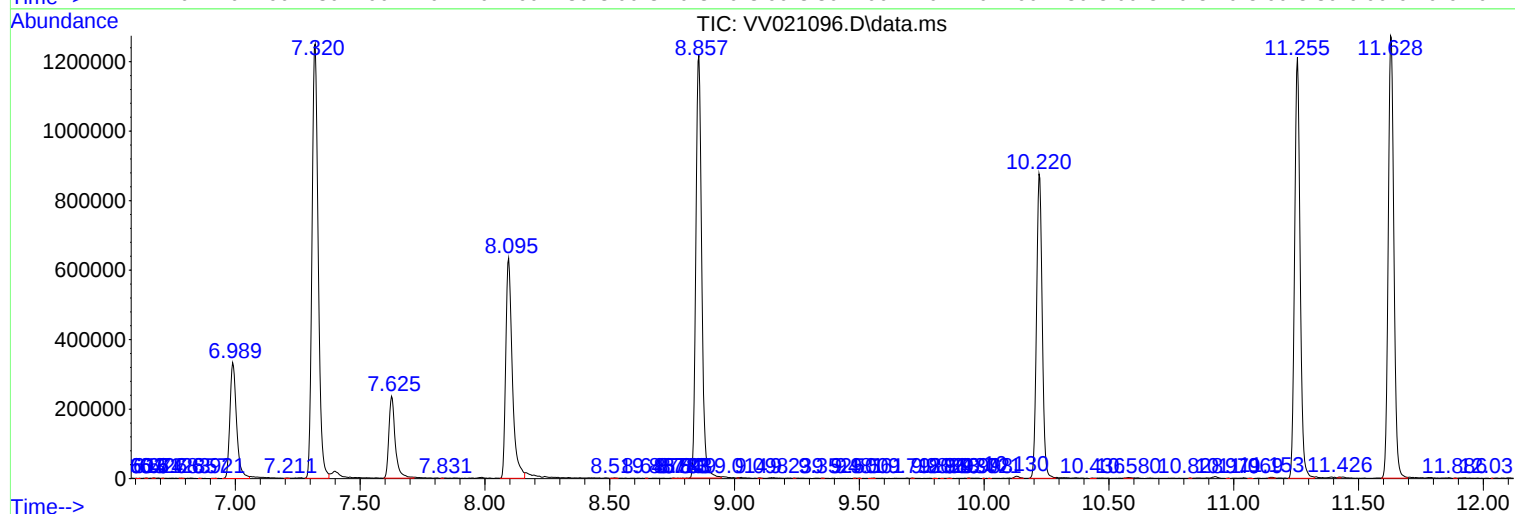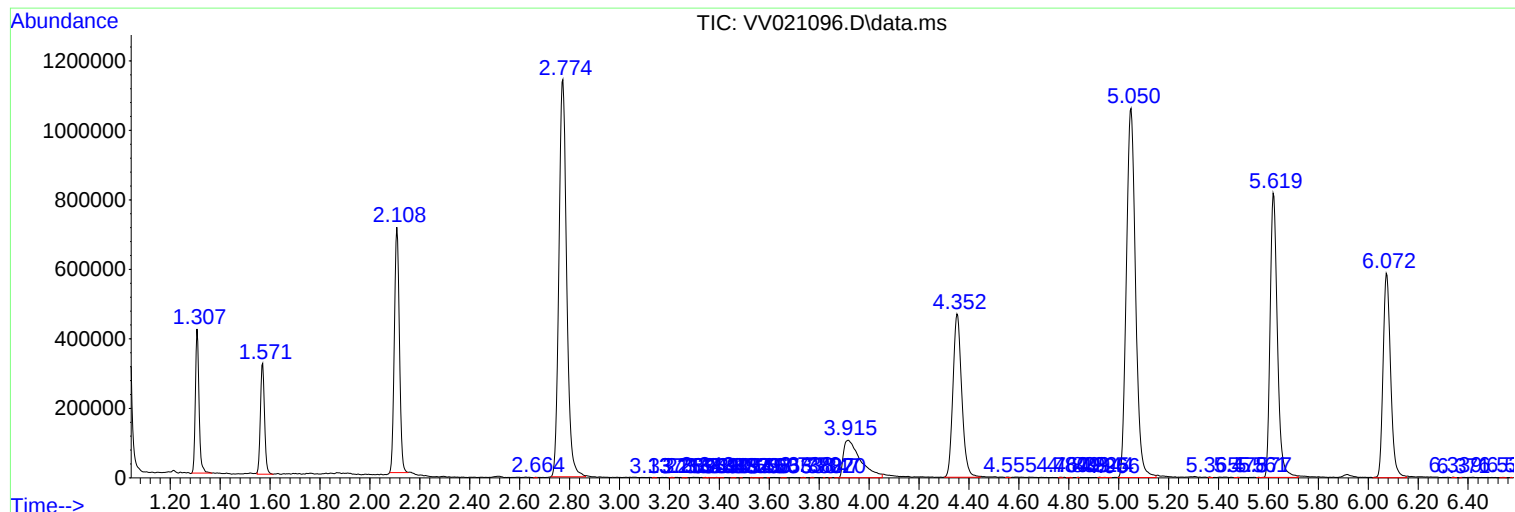

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021096.D
Acq On : 22 Apr 2021 14:55
Operator : SY/MD
Sample : M2067-17DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021096.D
Acq On : 22 Apr 2021 14:55
Operator : SY/MD
Sample : M2067-17DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
