

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021097.D
 Acq On : 22 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2067-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	35	rVB2	50459	48393	1.61%	0.202%
2	1.307	77	83	104	rVB	479852	495301	16.44%	2.070%
3	1.568	158	164	179	rVB	358880	413313	13.72%	1.727%
4	2.108	322	332	344	rBV	800830	1137422	37.76%	4.754%
5	2.619	488	491	497	rBV6	879	833	0.03%	0.003%
6	3.118	643	646	647	rBV	1199	538	0.02%	0.002%
7	3.153	655	657	658	rBV2	793	323	0.01%	0.001%
8	3.195	668	670	672	rVB	636	263	0.01%	0.001%
9	3.214	672	676	680	rBV4	1095	1077	0.04%	0.005%
10	3.236	680	683	685	rVB3	943	475	0.02%	0.002%
11	3.288	685	699	715	rBV4	28621	70132	2.33%	0.293%
12	3.449	743	749	753	rBV6	1129	1211	0.04%	0.005%
13	3.468	753	755	758	rVB3	875	442	0.01%	0.002%
14	3.490	758	762	765	rBV2	750	534	0.02%	0.002%
15	3.539	773	777	782	rBV3	924	756	0.03%	0.003%
16	3.642	806	809	811	rVB2	407	172	0.01%	0.001%
17	3.693	823	825	828	rBV3	1066	596	0.02%	0.002%
18	3.741	834	840	842	rBV4	1980	1720	0.06%	0.007%
19	3.802	857	859	864	rBV4	690	446	0.01%	0.002%
20	3.825	864	866	874	rVB5	1145	1332	0.04%	0.006%
21	3.857	874	876	879	rBV2	609	517	0.02%	0.002%
22	3.905	879	891	928	rBV2	116026	495929	16.46%	2.073%
23	4.349	1012	1029	1062	rBV	512381	1278869	42.45%	5.345%
24	4.873	1190	1192	1194	rBV2	447	217	0.01%	0.001%
25	4.886	1194	1196	1198	rVV2	653	301	0.01%	0.001%
26	4.915	1203	1205	1207	rVV2	891	444	0.01%	0.002%
27	4.934	1207	1211	1213	rVV3	1419	1056	0.04%	0.004%
28	4.947	1213	1215	1217	rVB	482	191	0.01%	0.001%
29	4.957	1217	1218	1222	rBV	442	335	0.01%	0.001%
30	5.047	1229	1246	1273	rBV2	1181221	3012584	100.00%	12.591%
31	5.468	1374	1377	1379	rBV3	1432	1002	0.03%	0.004%
32	5.564	1402	1407	1410	rBV3	945	750	0.02%	0.003%
33	5.616	1411	1423	1446	rBV	935186	1854134	61.55%	7.750%
34	5.921	1505	1518	1534	rBV7	38808	91584	3.04%	0.383%
35	6.069	1551	1564	1590	rBV	651577	1335131	44.32%	5.580%
36	6.317	1638	1641	1645	rVB3	1552	868	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021097.D
 Acq On : 22 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2067-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1659	rBV4	1125	796	0.03%	0.003%
38	6.458	1683	1685	1687	rBV3	916	331	0.01%	0.001%
39	6.648	1742	1744	1748	rVB4	1461	754	0.03%	0.003%
40	6.757	1776	1778	1781	rBV2	490	297	0.01%	0.001%
41	6.773	1781	1783	1788	rBV4	794	809	0.03%	0.003%
42	6.844	1804	1805	1808	rBV2	582	291	0.01%	0.001%
43	6.883	1812	1817	1819	rBV2	638	433	0.01%	0.002%
44	6.915	1824	1827	1829	rBV	371	285	0.01%	0.001%
45	6.989	1838	1850	1874	rBV	375039	695484	23.09%	2.907%
46	7.317	1939	1952	1970	rBV	1435305	2450006	81.33%	10.240%
47	7.622	2037	2047	2066	rBV	268828	464782	15.43%	1.943%
48	7.821	2105	2109	2113	rVB3	1308	1133	0.04%	0.005%
49	7.841	2113	2115	2117	rBV2	835	438	0.01%	0.002%
50	7.912	2135	2137	2141	rBV4	1326	889	0.03%	0.004%
51	7.976	2146	2157	2172	rVV	431429	739237	24.54%	3.090%
52	8.092	2183	2193	2215	rBV	648687	1174808	39.00%	4.910%
53	8.677	2374	2375	2377	rBV2	743	245	0.01%	0.001%
54	8.706	2382	2384	2388	rVB2	850	370	0.01%	0.002%
55	8.854	2418	2430	2458	rBV	1400429	2248254	74.63%	9.397%
56	9.194	2534	2536	2539	rBV4	946	392	0.01%	0.002%
57	9.278	2560	2562	2564	rBV2	754	376	0.01%	0.002%
58	9.400	2597	2600	2604	rBV3	1046	716	0.02%	0.003%
59	9.436	2609	2611	2615	rVB	843	475	0.02%	0.002%
60	9.481	2623	2625	2631	rVB4	1377	1235	0.04%	0.005%
61	9.513	2631	2635	2640	rBV5	1104	980	0.03%	0.004%
62	9.542	2640	2644	2646	rBV4	1074	972	0.03%	0.004%
63	9.654	2677	2679	2680	rBV2	437	153	0.01%	0.001%
64	9.719	2697	2699	2700	rBV2	545	256	0.01%	0.001%
65	9.792	2719	2722	2724	rBV2	584	400	0.01%	0.002%
66	9.876	2746	2748	2754	rVB3	1436	914	0.03%	0.004%
67	9.953	2769	2772	2773	rBV	608	325	0.01%	0.001%
68	9.989	2782	2783	2784	rBV	312	106	0.00%	0.000%
69	10.001	2785	2787	2792	rVB4	931	636	0.02%	0.003%
70	10.220	2841	2855	2876	rBV	943930	1478616	49.08%	6.180%
71	10.442	2922	2924	2925	rBV	670	250	0.01%	0.001%
72	10.471	2931	2933	2934	rBV2	797	303	0.01%	0.001%
73	10.481	2934	2936	2939	rVB	1376	638	0.02%	0.003%
74	10.718	3006	3010	3012	rBV2	895	581	0.02%	0.002%
75	10.924	3068	3074	3084	rVB6	5447	8021	0.27%	0.034%
76	11.146	3136	3143	3144	rBV5	2184	2076	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021097.D
 Acq On : 22 Apr 2021 15:38
 Operator : SY/MD
 Sample : M2067-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A3

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	11.198	3157	3159	3165	rBV5	1013	844	0.03%	0.004%
78	11.252	3165	3176	3197	rBV	1369534	2129253	70.68%	8.899%
79	11.497	3248	3252	3256	rBV5	1070	910	0.03%	0.004%
80	11.628	3282	3293	3315	rBV	1420573	2254930	74.85%	9.425%
81	11.937	3387	3389	3392	rBV4	1112	725	0.02%	0.003%
82	11.985	3401	3404	3408	rBV3	1437	1055	0.04%	0.004%
83	12.005	3408	3410	3413	rBV4	790	478	0.02%	0.002%
84	12.294	3497	3500	3502	rBV3	1398	778	0.03%	0.003%
85	12.333	3509	3512	3515	rBV3	980	467	0.02%	0.002%
86	12.413	3535	3537	3539	rBV2	865	485	0.02%	0.002%
87	12.442	3544	3546	3548	rVB3	966	427	0.01%	0.002%
88	12.461	3548	3552	3553	rBV2	871	518	0.02%	0.002%
89	12.558	3580	3582	3585	rBV2	1112	874	0.03%	0.004%
90	12.616	3598	3600	3605	rVB4	1044	642	0.02%	0.003%
91	12.667	3614	3616	3619	rBV3	785	475	0.02%	0.002%
92	12.988	3713	3716	3717	rBV	613	374	0.01%	0.002%
93	13.014	3722	3724	3728	rBV3	1111	724	0.02%	0.003%
94	13.085	3744	3746	3751	rBV3	764	587	0.02%	0.002%
95	13.194	3777	3780	3783	rBV2	1166	851	0.03%	0.004%
96	13.432	3852	3854	3856	rBV3	1081	536	0.02%	0.002%
97	13.805	3967	3970	3974	rBV2	1505	1011	0.03%	0.004%
98	14.214	4095	4097	4100	rBV3	1053	763	0.03%	0.003%
99	14.558	4202	4204	4206	rBV2	1492	832	0.03%	0.003%




Sum of corrected areas: 23925793

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021097.D
Acq On : 22 Apr 2021 15:38
Operator : SY/MD
Sample : M2067-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

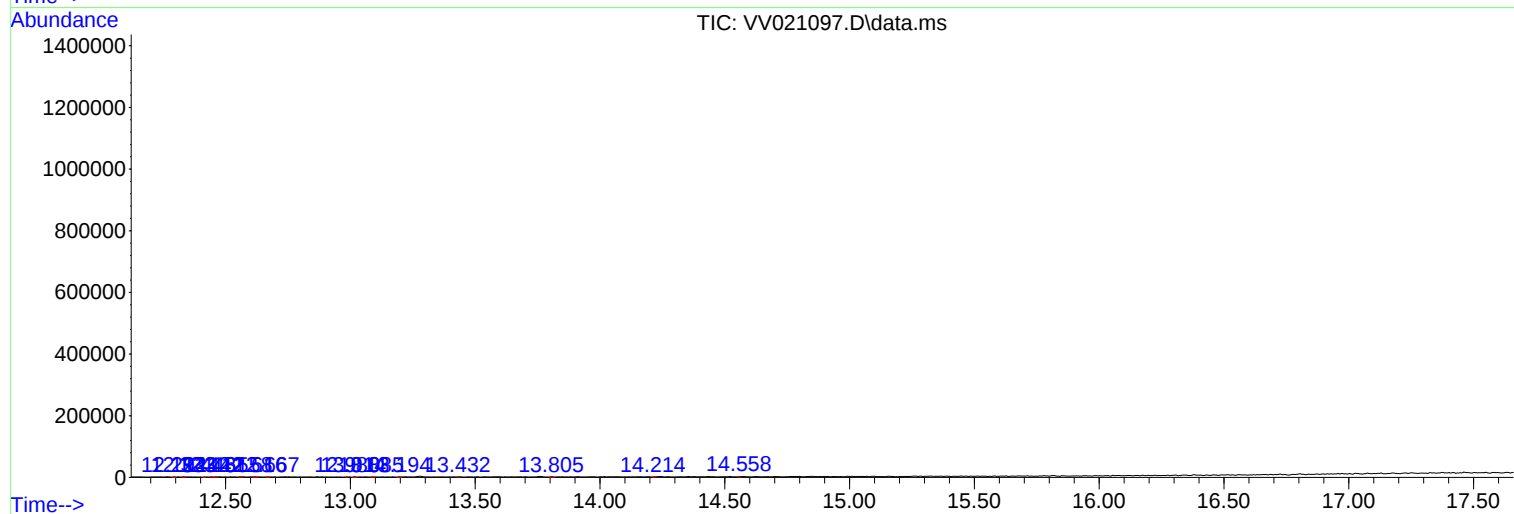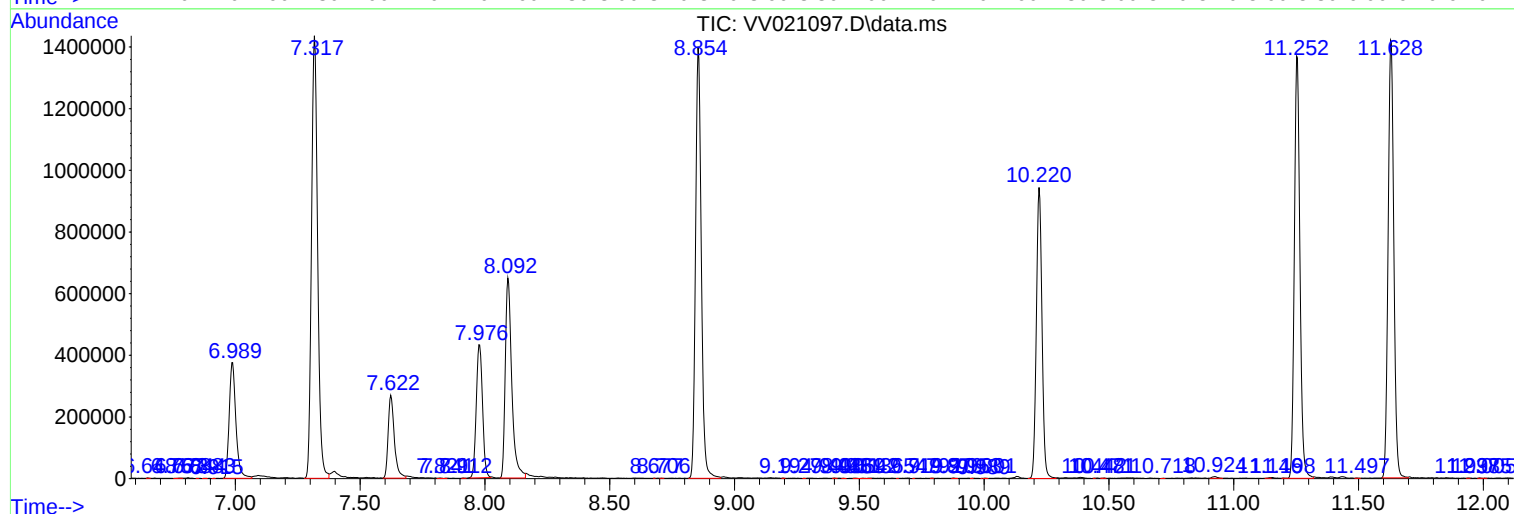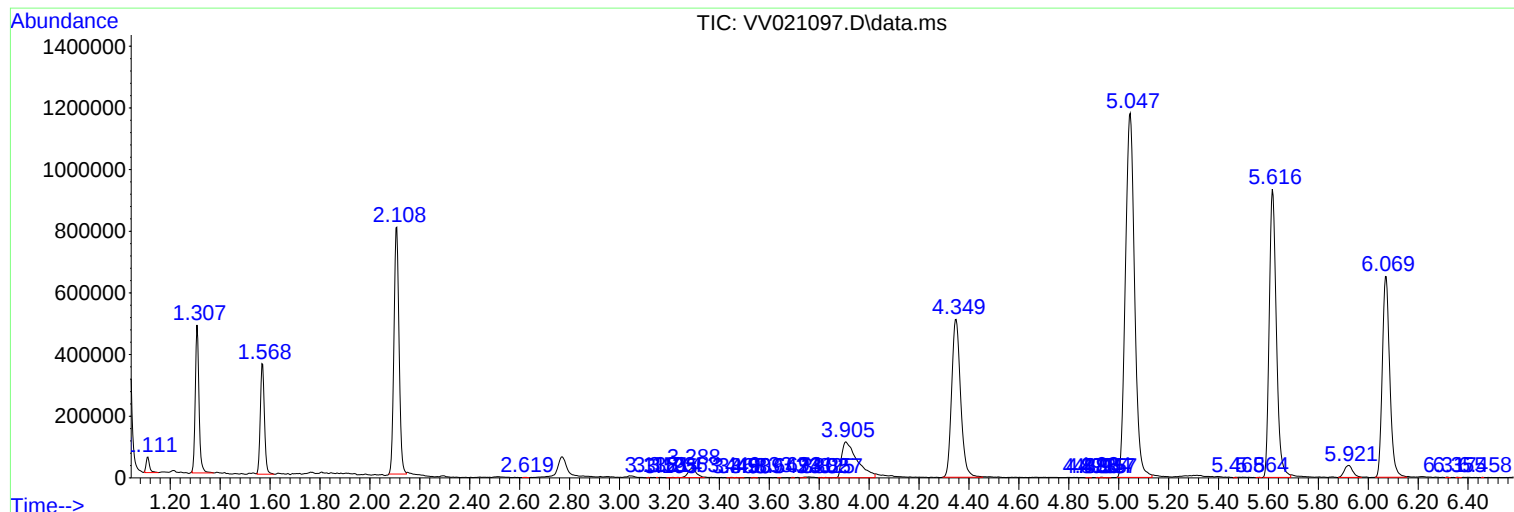

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021097.D
Acq On : 22 Apr 2021 15:38
Operator : SY/MD
Sample : M2067-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021097.D
Acq On : 22 Apr 2021 15:38
Operator : SY/MD
Sample : M2067-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
