

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021098.D
 Acq On : 22 Apr 2021 16:02
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rBV	397040	402965	3.41%	1.104%
2	1.568	158	164	177	rVB	308947	352636	2.98%	0.966%
3	2.108	323	332	346	rBV	703158	995377	8.42%	2.726%
4	2.632	493	495	497	rVB	691	235	0.00%	0.001%
5	2.658	501	503	509	rVB4	981	745	0.01%	0.002%
6	2.873	566	570	573	rVB2	604	416	0.00%	0.001%
7	2.912	580	582	589	rVB2	774	743	0.01%	0.002%
8	2.937	589	590	593	rBV	505	323	0.00%	0.001%
9	2.960	594	597	599	rBV2	657	442	0.00%	0.001%
10	3.043	614	623	636	rBV6	8554	17054	0.14%	0.047%
11	3.150	655	656	660	rBV	423	333	0.00%	0.001%
12	3.169	660	662	664	rVB	390	196	0.00%	0.001%
13	3.223	677	679	680	rBV	385	146	0.00%	0.000%
14	3.272	692	694	699	rVB2	876	535	0.00%	0.001%
15	3.301	699	703	704	rBV	566	330	0.00%	0.001%
16	3.352	715	719	720	rBV	634	434	0.00%	0.001%
17	3.426	737	742	747	rVB3	919	1052	0.01%	0.003%
18	3.452	747	750	752	rBV2	414	153	0.00%	0.000%
19	3.481	756	759	761	rBV3	663	408	0.00%	0.001%
20	3.503	764	766	768	rVB2	479	176	0.00%	0.000%
21	3.522	769	772	774	rBV2	652	380	0.00%	0.001%
22	3.555	779	782	783	rBV	343	145	0.00%	0.000%
23	3.571	783	787	789	rBV3	621	491	0.00%	0.001%
24	3.616	799	801	804	rVB	689	316	0.00%	0.001%
25	3.680	818	821	822	rBV	465	236	0.00%	0.001%
26	3.825	861	866	867	rBV	797	526	0.00%	0.001%
27	3.918	883	895	934	rBV2	110492	512664	4.34%	1.404%
28	4.352	1014	1030	1059	rBV2	461627	1133168	9.59%	3.104%
29	4.674	1128	1130	1131	rBV2	593	280	0.00%	0.001%
30	4.731	1147	1148	1151	rBV3	740	499	0.00%	0.001%
31	4.879	1190	1194	1197	rVB4	706	608	0.01%	0.002%
32	4.902	1197	1201	1205	rBV2	576	489	0.00%	0.001%
33	4.953	1216	1217	1219	rBV	412	197	0.00%	0.001%
34	4.966	1219	1221	1226	rVV2	1239	883	0.01%	0.002%
35	5.050	1229	1247	1294	rBV2	1067341	2792055	23.63%	7.648%
36	5.375	1345	1348	1353	rBV4	1378	990	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021098.D
 Acq On : 22 Apr 2021 16:02
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.455	1369	1373	1374	rBV	858	621	0.01%	0.002%
38	5.493	1383	1385	1386	rBV2	880	300	0.00%	0.001%
39	5.619	1412	1424	1454	rBV	782695	1590921	13.46%	4.358%
40	5.915	1503	1516	1550	rBV	2132518	4131089	34.96%	11.315%
41	6.072	1554	1565	1599	rVB	587626	1199719	10.15%	3.286%
42	6.304	1634	1637	1640	rBV3	1150	747	0.01%	0.002%
43	6.339	1644	1648	1650	rBV4	922	810	0.01%	0.002%
44	6.622	1734	1736	1740	rBV3	930	602	0.01%	0.002%
45	6.738	1770	1772	1776	rBV3	578	353	0.00%	0.001%
46	6.783	1784	1786	1789	rVB2	586	285	0.00%	0.001%
47	6.889	1817	1819	1821	rBV2	363	213	0.00%	0.001%
48	6.934	1831	1833	1836	rBV3	555	213	0.00%	0.001%
49	6.989	1839	1850	1870	rBV	341481	625164	5.29%	1.712%
50	7.320	1940	1953	1971	rBV	1251839	2172102	18.38%	5.950%
51	7.625	2036	2048	2076	rBV	233971	427179	3.62%	1.170%
52	7.834	2110	2113	2114	rBV2	604	315	0.00%	0.001%
53	7.895	2129	2132	2137	rVB3	880	823	0.01%	0.002%
54	7.918	2137	2139	2141	rBV2	580	377	0.00%	0.001%
55	7.979	2143	2158	2184	rBV	7200145	11816584	100.00%	32.367%
56	8.095	2185	2194	2228	rVB	633483	1171466	9.91%	3.209%
57	8.522	2325	2327	2331	rBV4	817	548	0.00%	0.002%
58	8.731	2389	2392	2394	rBV3	960	661	0.01%	0.002%
59	8.857	2419	2431	2458	rBV	1186648	1913275	16.19%	5.241%
60	9.098	2505	2506	2516	rVB4	1288	940	0.01%	0.003%
61	9.246	2550	2552	2559	rVB4	1120	723	0.01%	0.002%
62	9.284	2562	2564	2567	rVB3	1151	515	0.00%	0.001%
63	9.326	2574	2577	2580	rBV2	859	596	0.01%	0.002%
64	9.365	2587	2589	2591	rBV3	643	291	0.00%	0.001%
65	9.390	2591	2597	2600	rBV5	871	919	0.01%	0.003%
66	9.461	2616	2619	2620	rBV	839	433	0.00%	0.001%
67	9.506	2631	2633	2636	rVB2	752	368	0.00%	0.001%
68	9.641	2673	2675	2680	rBV	499	395	0.00%	0.001%
69	9.699	2689	2693	2695	rVB3	859	555	0.00%	0.002%
70	9.722	2698	2700	2704	rVB2	1161	649	0.01%	0.002%
71	9.751	2704	2709	2710	rBV3	671	435	0.00%	0.001%
72	9.841	2733	2737	2741	rBV4	660	645	0.01%	0.002%
73	9.918	2759	2761	2762	rBV	631	228	0.00%	0.001%
74	9.982	2778	2781	2783	rBV	932	438	0.00%	0.001%
75	10.017	2789	2792	2796	rBV2	761	486	0.00%	0.001%
76	10.133	2821	2828	2837	rVB6	6361	8535	0.07%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021098.D
 Acq On : 22 Apr 2021 16:02
 Operator : SY/MD
 Sample : M2067-05DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.220	2844	2855	2874	rBV	876087	1378264	11.66%	3.775%
78	10.632	2979	2983	2986	rBB4	772	604	0.01%	0.002%
79	10.654	2987	2990	2991	rBV2	791	421	0.00%	0.001%
80	10.796	3031	3034	3035	rBV	583	377	0.00%	0.001%
81	10.892	3060	3064	3065	rBV2	778	549	0.00%	0.002%
82	10.921	3067	3073	3084	rVB5	5721	8429	0.07%	0.023%
83	10.972	3087	3089	3090	rBV	496	186	0.00%	0.001%
84	11.088	3123	3125	3128	rBV3	904	607	0.01%	0.002%
85	11.136	3138	3140	3141	rBV	995	361	0.00%	0.001%
86	11.255	3166	3177	3196	rBV	1171878	1811321	15.33%	4.961%
87	11.554	3267	3270	3272	rBV2	1124	612	0.01%	0.002%
88	11.631	3281	3294	3314	rBV	1283746	2009985	17.01%	5.506%
89	11.947	3389	3392	3394	rBV2	846	519	0.00%	0.001%
90	12.024	3414	3416	3417	rBV2	698	301	0.00%	0.001%
91	12.191	3466	3468	3471	rBV2	920	446	0.00%	0.001%
92	12.262	3488	3490	3492	rVB3	868	314	0.00%	0.001%
93	12.390	3528	3530	3532	rBV2	1131	647	0.01%	0.002%
94	12.432	3540	3543	3545	rBV3	1251	668	0.01%	0.002%
95	12.471	3553	3555	3556	rBV	868	394	0.00%	0.001%
96	12.638	3603	3607	3610	rVB4	1328	951	0.01%	0.003%
97	12.657	3610	3613	3616	rBV3	1513	1177	0.01%	0.003%
98	13.111	3752	3754	3756	rBV2	813	379	0.00%	0.001%
99	13.483	3869	3870	3875	rVB3	1076	518	0.00%	0.001%
100	13.908	4000	4002	4004	rBV3	690	366	0.00%	0.001%

Sum of corrected areas: 36508540




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021098.D
Acq On : 22 Apr 2021 16:02
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

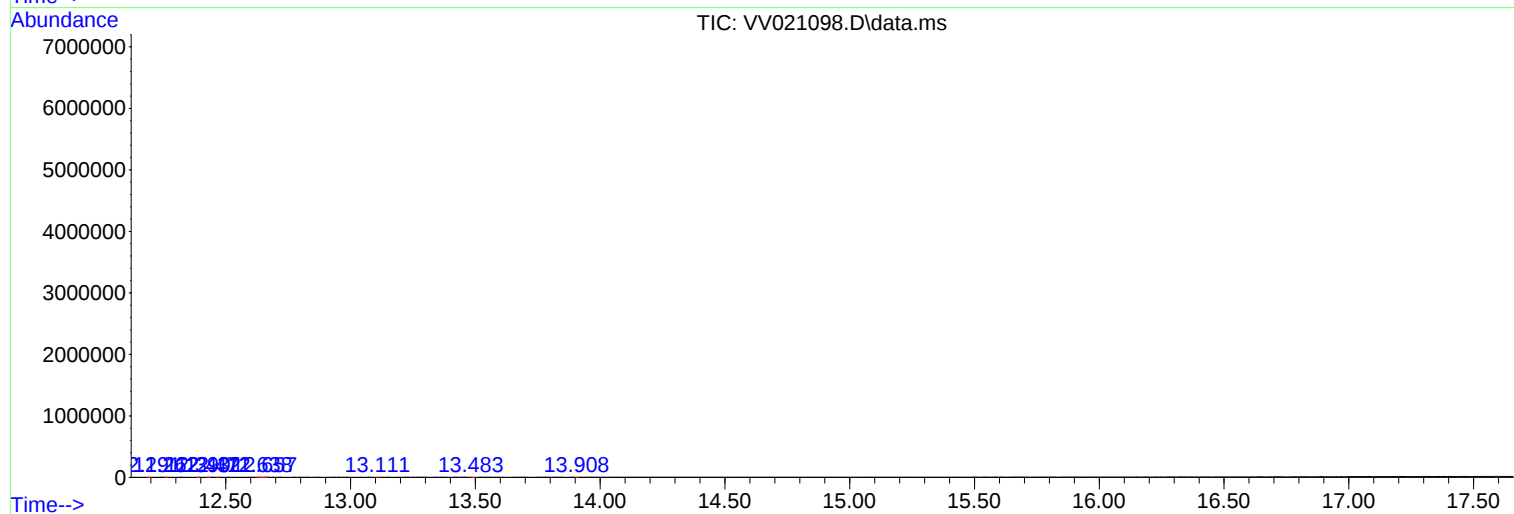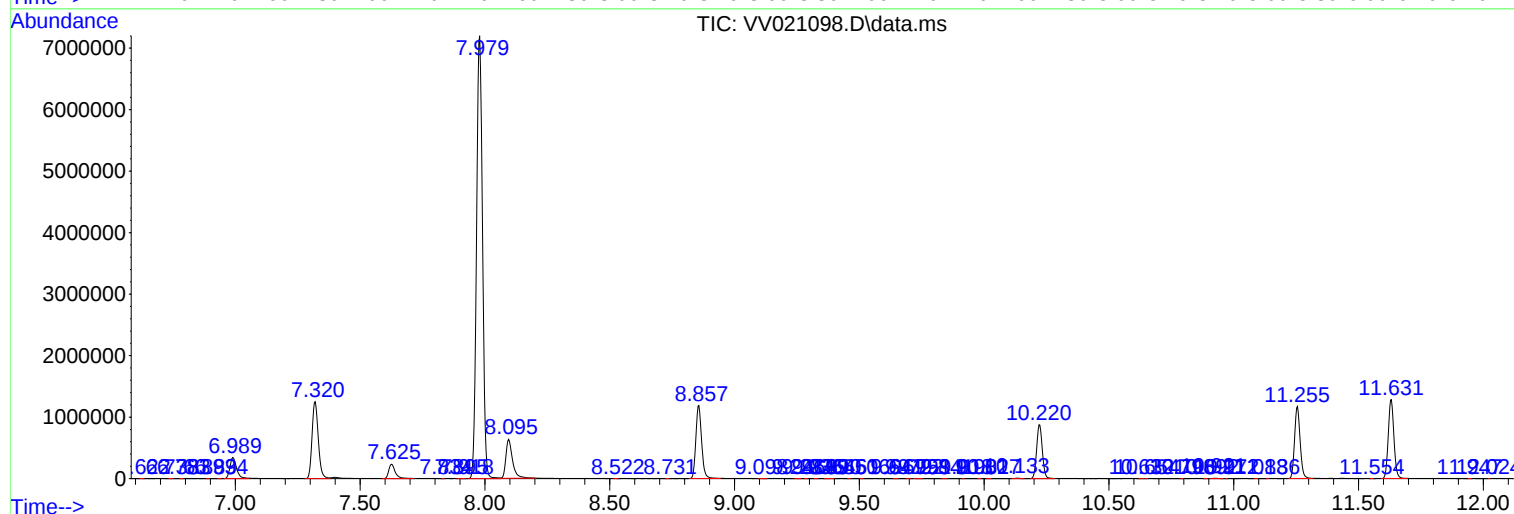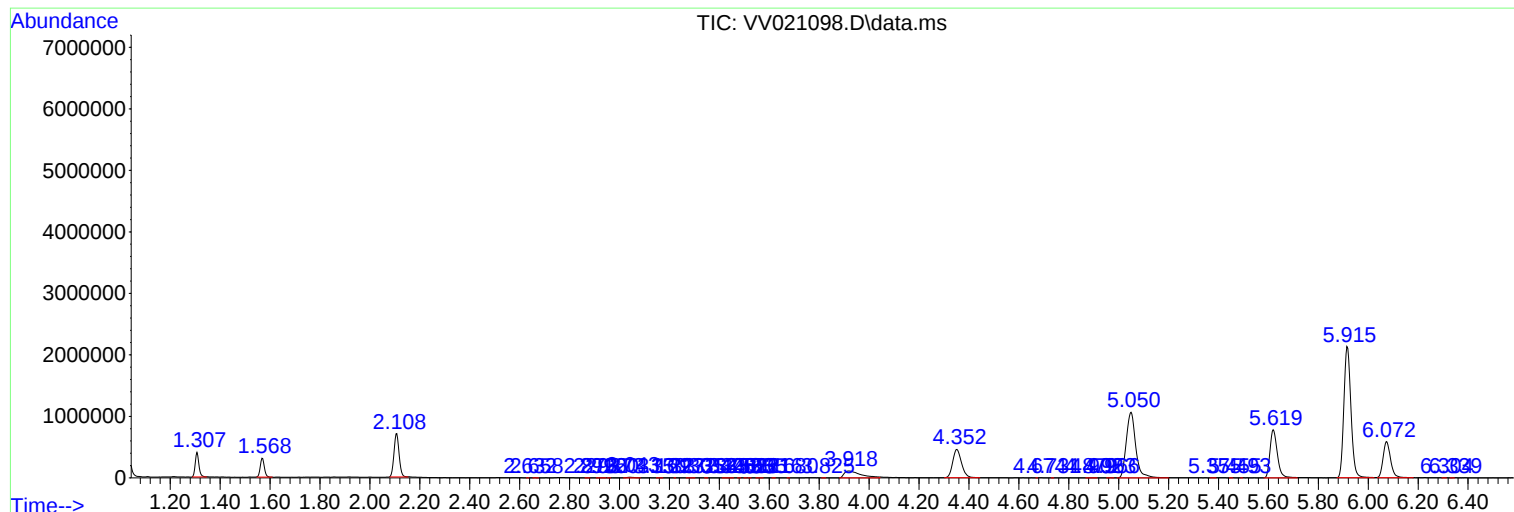

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021098.D
Acq On : 22 Apr 2021 16:02
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021098.D
Acq On : 22 Apr 2021 16:02
Operator : SY/MD
Sample : M2067-05DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
