

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021099.D
 Acq On : 22 Apr 2021 16:25
 Operator : SY/MD
 Sample : M2067-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	383422	386762	15.00%	1.928%
2	1.571	158	165	175	rVB	297595	338515	13.13%	1.687%
3	2.108	323	332	344	rBV	681239	953441	36.97%	4.752%
4	2.468	441	444	448	rBV5	1063	899	0.03%	0.004%
5	2.719	518	522	527	rVB3	921	838	0.03%	0.004%
6	2.744	527	530	531	rBV	834	446	0.02%	0.002%
7	2.857	563	565	572	rVB3	911	706	0.03%	0.004%
8	2.905	578	580	583	rVB4	1014	510	0.02%	0.003%
9	2.982	602	604	608	rBV3	613	404	0.02%	0.002%
10	3.005	608	611	616	rVB4	726	613	0.02%	0.003%
11	3.031	616	619	621	rVB2	646	422	0.02%	0.002%
12	3.053	621	626	629	rBV4	1502	1333	0.05%	0.007%
13	3.108	641	643	648	rVB3	688	487	0.02%	0.002%
14	3.178	659	665	668	rBV3	716	757	0.03%	0.004%
15	3.236	681	683	686	rBV2	890	556	0.02%	0.003%
16	3.323	707	710	712	rBV3	562	308	0.01%	0.002%
17	3.349	716	718	721	rVV	595	313	0.01%	0.002%
18	3.539	775	777	782	rVB4	468	336	0.01%	0.002%
19	3.561	782	784	789	rBV2	610	531	0.02%	0.003%
20	3.638	806	808	810	rBV	510	306	0.01%	0.002%
21	3.683	819	822	826	rBV3	545	358	0.01%	0.002%
22	3.732	834	837	843	rBV3	838	774	0.03%	0.004%
23	3.812	860	862	868	rVB3	668	510	0.02%	0.003%
24	3.857	873	876	880	rBV3	680	574	0.02%	0.003%
25	3.921	883	896	937	rBV2	98265	481319	18.66%	2.399%
26	4.352	1015	1030	1052	rBV2	449050	1090659	42.29%	5.436%
27	4.838	1178	1181	1182	rBV2	824	521	0.02%	0.003%
28	4.895	1197	1199	1206	rBV5	1084	710	0.03%	0.004%
29	4.931	1206	1210	1213	rBV3	754	491	0.02%	0.002%
30	4.989	1221	1228	1230	rBV2	943	772	0.03%	0.004%
31	5.050	1230	1247	1275	rBV2	1009614	2578991	100.00%	12.854%
32	5.375	1347	1348	1351	rBV	614	378	0.01%	0.002%
33	5.407	1355	1358	1360	rBV4	1058	677	0.03%	0.003%
34	5.619	1411	1424	1455	rBV	809038	1659847	64.36%	8.273%
35	6.072	1553	1565	1594	rBV	563808	1149093	44.56%	5.727%
36	6.358	1652	1654	1657	rVB3	706	294	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021099.D
 Acq On : 22 Apr 2021 16:25
 Operator : SY/MD
 Sample : M2067-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.387	1661	1663	1665	rBV2	627	291	0.01%	0.001%
38	6.555	1712	1715	1718	rBV2	638	379	0.01%	0.002%
39	6.693	1756	1758	1761	rBV3	739	494	0.02%	0.002%
40	6.754	1773	1777	1781	rVB2	901	775	0.03%	0.004%
41	6.780	1781	1785	1789	rBV4	831	798	0.03%	0.004%
42	6.818	1794	1797	1803	rBV2	863	652	0.03%	0.003%
43	6.860	1807	1810	1813	rBV	659	505	0.02%	0.003%
44	6.892	1817	1820	1822	rBV2	664	461	0.02%	0.002%
45	6.989	1835	1850	1876	rBV	324148	598981	23.23%	2.985%
46	7.320	1940	1953	1972	rBV	1200376	2079425	80.63%	10.364%
47	7.625	2039	2048	2066	rBV	223095	389769	15.11%	1.943%
48	7.940	2143	2146	2151	rVB3	774	651	0.03%	0.003%
49	7.985	2151	2160	2172	rBV5	13726	23859	0.93%	0.119%
50	8.095	2184	2194	2229	rBV	600750	1114333	43.21%	5.554%
51	8.677	2372	2375	2379	rBV2	555	434	0.02%	0.002%
52	8.786	2407	2409	2412	rVB3	672	373	0.01%	0.002%
53	8.857	2418	2431	2464	rBV	1228260	1998798	77.50%	9.962%
54	9.153	2520	2523	2524	rBV2	1397	795	0.03%	0.004%
55	9.210	2539	2541	2544	rBV	667	334	0.01%	0.002%
56	9.271	2557	2560	2564	rBV3	1182	843	0.03%	0.004%
57	9.329	2575	2578	2580	rBV2	613	390	0.02%	0.002%
58	9.390	2593	2597	2600	rBV3	907	875	0.03%	0.004%
59	9.452	2615	2616	2619	rVB	852	430	0.02%	0.002%
60	9.506	2627	2633	2634	rBV	1132	670	0.03%	0.003%
61	9.728	2699	2702	2704	rBV	670	389	0.02%	0.002%
62	9.751	2706	2709	2712	rBV3	623	467	0.02%	0.002%
63	9.857	2737	2742	2743	rBV2	909	648	0.03%	0.003%
64	9.879	2747	2749	2752	rVV3	831	434	0.02%	0.002%
65	9.908	2755	2758	2761	rVB2	879	557	0.02%	0.003%
66	9.976	2776	2779	2781	rBV	920	625	0.02%	0.003%
67	10.050	2799	2802	2805	rBV2	570	361	0.01%	0.002%
68	10.104	2816	2819	2820	rBV2	663	383	0.01%	0.002%
69	10.130	2820	2827	2839	rVB7	5162	8488	0.33%	0.042%
70	10.220	2843	2855	2875	rBV	839979	1337316	51.85%	6.665%
71	10.542	2951	2955	2958	rBV4	872	654	0.03%	0.003%
72	10.574	2962	2965	2967	rBV3	1065	732	0.03%	0.004%
73	10.635	2982	2984	2987	rVB2	796	367	0.01%	0.002%
74	10.693	3000	3002	3008	rVB4	904	615	0.02%	0.003%
75	10.921	3065	3073	3081	rBV9	4990	7724	0.30%	0.038%
76	10.992	3093	3095	3098	rBV	524	295	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021099.D
 Acq On : 22 Apr 2021 16:25
 Operator : SY/MD
 Sample : M2067-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	11.008	3098	3100	3105	rVV2	660	506	0.02%	0.003%
78	11.082	3121	3123	3127	rBV3	383	304	0.01%	0.002%
79	11.146	3139	3143	3149	rBV6	2482	2810	0.11%	0.014%
80	11.255	3165	3177	3197	rBV	1206051	1863031	72.24%	9.285%
81	11.387	3215	3218	3224	rBV8	2631	2415	0.09%	0.012%
82	11.542	3264	3266	3272	rVB5	1002	697	0.03%	0.003%
83	11.632	3281	3294	3318	rBV	1228247	1954866	75.80%	9.743%
84	11.902	3374	3378	3380	rBV3	737	672	0.03%	0.003%
85	11.988	3403	3405	3407	rBV	846	371	0.01%	0.002%
86	12.046	3420	3423	3427	rBV2	1136	894	0.03%	0.004%
87	12.069	3427	3430	3431	rBV2	739	388	0.02%	0.002%
88	12.098	3435	3439	3441	rBV4	1513	1278	0.05%	0.006%
89	12.246	3482	3485	3489	rVB3	774	637	0.02%	0.003%
90	12.268	3490	3492	3495	rBV3	858	639	0.02%	0.003%
91	12.406	3532	3535	3537	rBV2	646	348	0.01%	0.002%
92	12.603	3594	3596	3597	rBV	920	401	0.02%	0.002%
93	12.654	3610	3612	3614	rBV3	911	520	0.02%	0.003%
94	12.738	3637	3638	3640	rBV2	697	328	0.01%	0.002%
95	12.831	3664	3667	3669	rBV2	1018	575	0.02%	0.003%
96	13.004	3718	3721	3723	rBV3	928	655	0.03%	0.003%
97	13.053	3733	3736	3738	rBV2	924	715	0.03%	0.004%
98	13.480	3867	3869	3872	rBV2	1077	482	0.02%	0.002%
99	13.561	3892	3894	3898	rVB3	1142	554	0.02%	0.003%
100	13.847	3980	3983	3984	rBV	936	476	0.02%	0.002%




Sum of corrected areas: 20064383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021099.D
Acq On : 22 Apr 2021 16:25
Operator : SY/MD
Sample : M2067-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

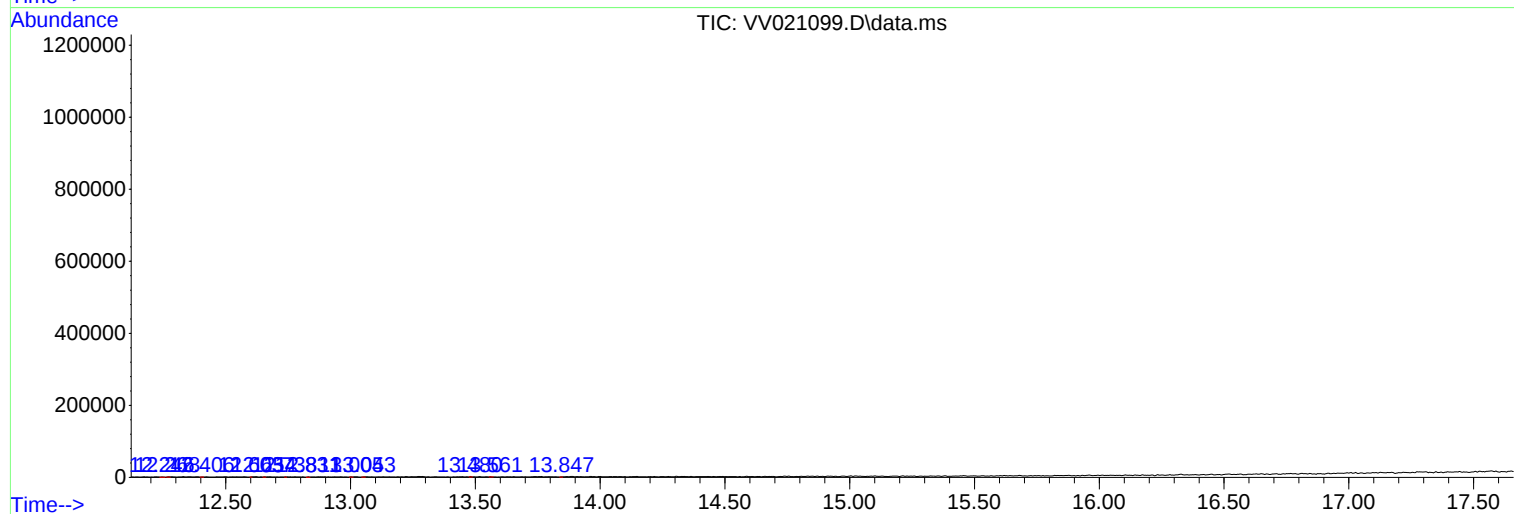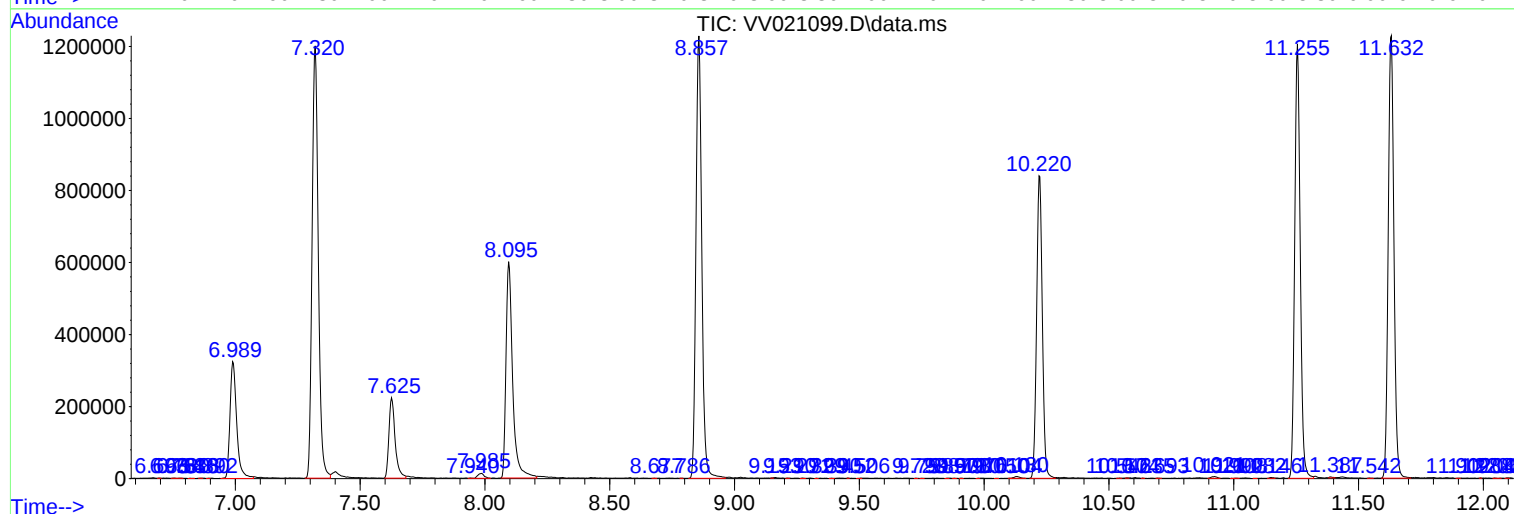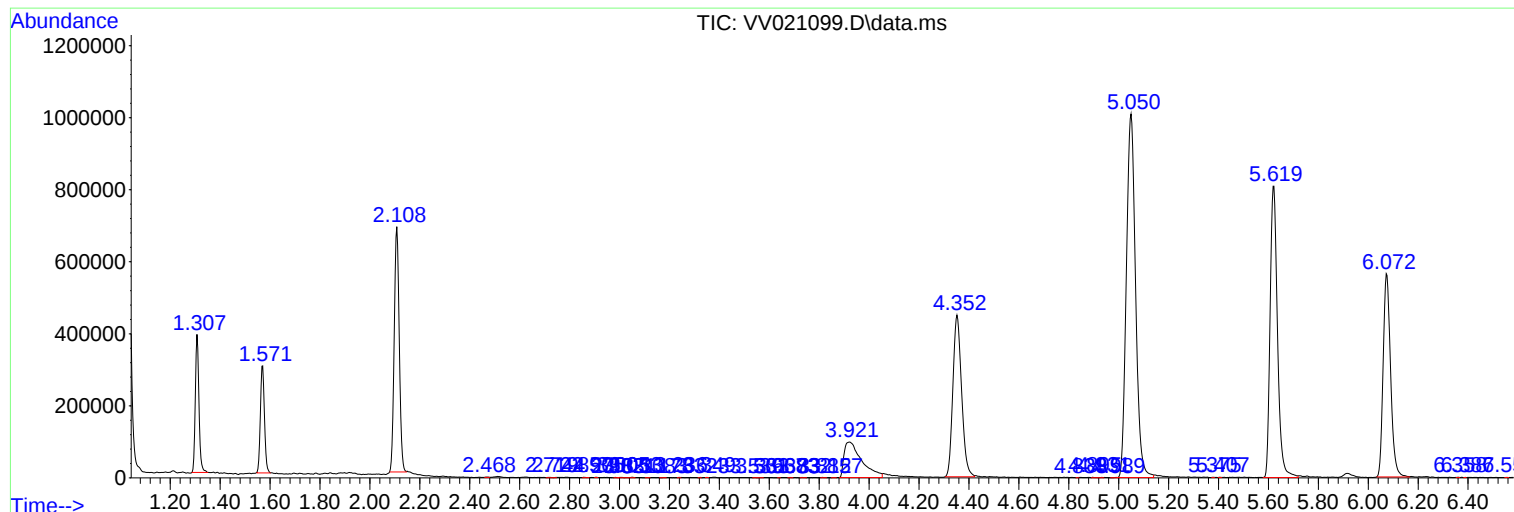

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021099.D
Acq On : 22 Apr 2021 16:25
Operator : SY/MD
Sample : M2067-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
Data File : VV021099.D
Acq On : 22 Apr 2021 16:25
Operator : SY/MD
Sample : M2067-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------