


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042221\
 Data File : VV021088.D
 Acq On : 22 Apr 2021 10:11
 Operator : SY/MD
 Sample : BFB87
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB187

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMV111820SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 30 17:18:00 2020

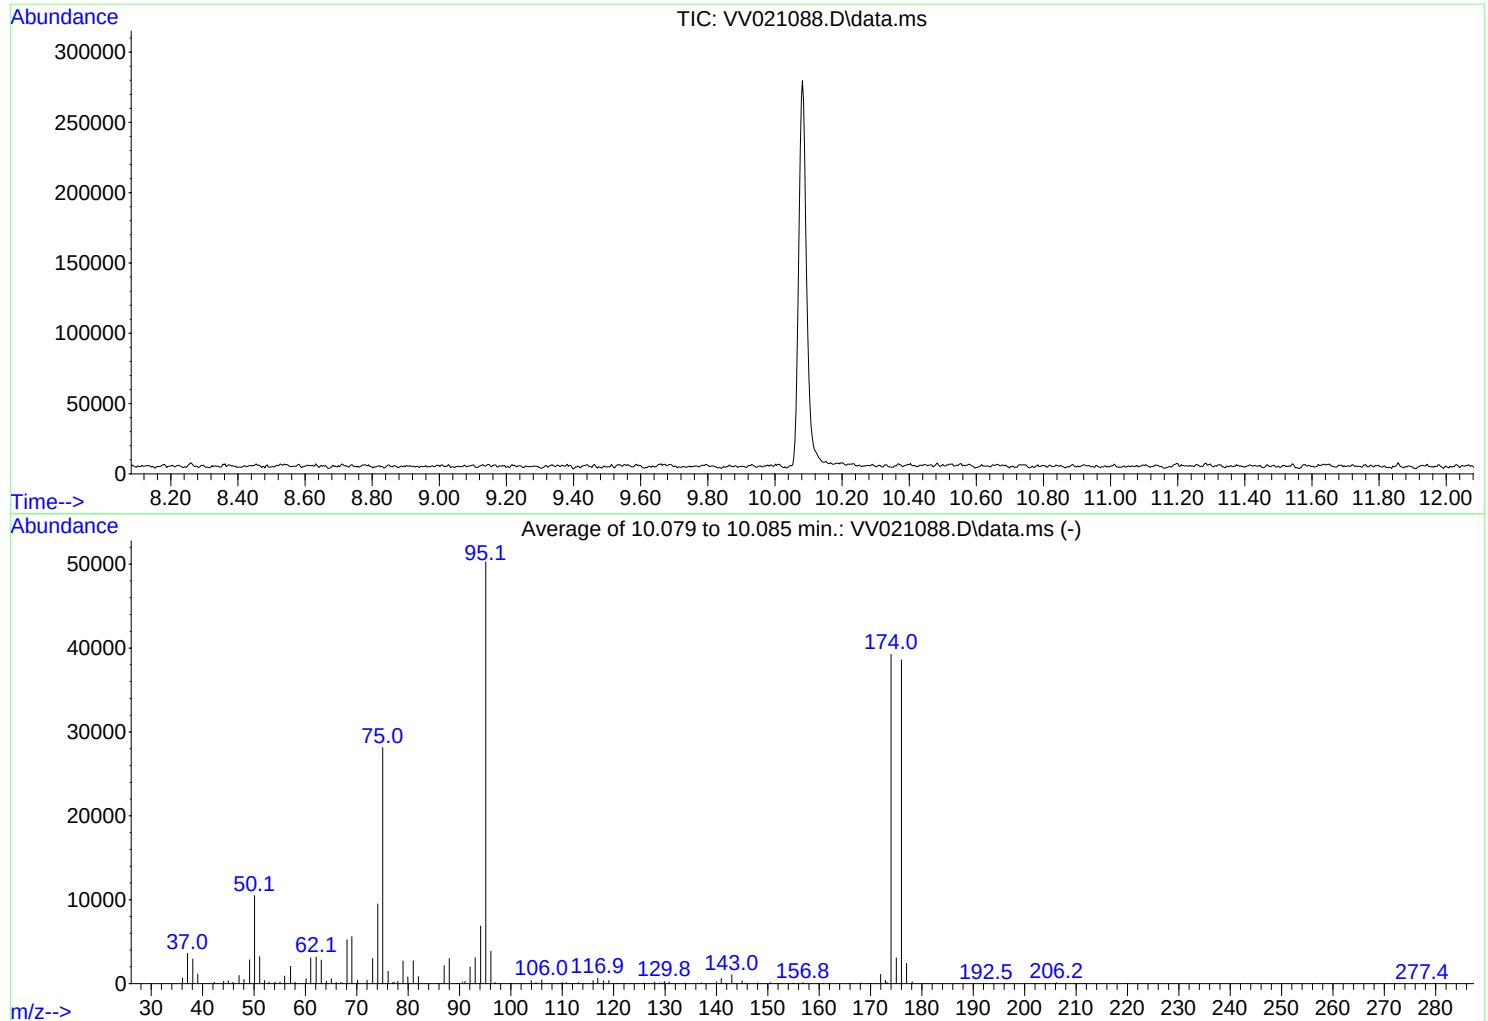

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	10485	PASS
75	95	30	80	56.0	28153	PASS
95	95	100	100	100.0	50275	PASS
96	95	5	9	7.7	3879	PASS
173	174	0.00	2	1.0	393	PASS
174	95	50	120	78.1	39253	PASS
175	174	5	9	7.8	3062	PASS
176	174	95	101	98.3	38587	PASS
177	176	5	9	6.2	2403	PASS

m/z	Abundance
36.20	817.0
37.10	3903.0
38.10	3087.0
39.10	1267.0
40.00	304.0
42.30	176.0
44.10	930.0
45.00	448.0
45.90	296.0
47.10	1056.0
48.10	521.0
49.20	2925.0
50.10	10768.0
51.10	3342.0
52.00	384.0
52.90	219.0
54.10	205.0
55.10	190.0
56.00	1087.0
57.10	2119.0
58.00	179.0
60.20	623.0
61.00	3210.0
62.10	3247.0
63.10	2862.0
64.10	255.0
65.00	599.0
66.00	132.0
66.90	205.0
68.10	5244.0
69.10	5849.0
70.10	519.0
72.00	429.0
73.10	3078.0
74.10	9556.0
75.10	29080.0
76.10	1578.0
77.00	347.0
78.00	256.0
79.00	2848.0
79.90	830.0
81.00	2811.0
82.00	917.0
87.00	2177.0
88.00	3248.0
90.60	317.0
91.10	379.0
92.10	2057.0
93.00	3303.0
94.10	7164.0
95.10	52024.0
96.10	4035.0
96.90	141.0
103.90	423.0
104.90	148.0
106.00	506.0
110.00	152.0
110.80	148.0
113.20	191.0
116.00	383.0
116.90	661.0
118.10	355.0
119.00	345.0
125.90	107.0
128.00	154.0
128.90	103.0
129.80	284.0
130.80	189.0
134.00	123.0
137.00	137.0
140.10	229.0
141.00	745.0
143.00	1087.0
145.00	362.0
145.70	126.0
148.10	146.0
150.50	159.0
155.00	101.0
156.90	154.0
169.70	101.0
172.00	1188.0
172.90	558.0
174.00	40560.0
175.00	3162.0
176.00	40104.0
177.00	2454.0
178.10	218.0
206.20	120.0
211.60	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB187

m/z	Abundance
36.10	816.0
37.10	3749.0
38.10	2976.0
39.10	1038.0
39.90	286.0
42.30	122.0
43.00	111.0
44.00	993.0
45.00	581.0
45.90	237.0
47.10	1123.0
48.00	470.0
49.20	2722.0
50.10	10258.0
51.10	3330.0
52.00	344.0
52.90	246.0
54.10	197.0
55.10	222.0
56.00	1004.0
57.10	2159.0
58.00	119.0
60.20	516.0
61.10	3027.0
62.10	3324.0
63.10	2662.0
64.10	286.0
65.00	581.0
66.00	119.0
67.20	207.0
68.10	5223.0
69.00	5483.0
70.10	611.0
72.00	276.0
73.10	3207.0
74.10	9437.0
75.10	28576.0
76.10	1678.0
77.00	399.0
78.00	362.0
79.00	2621.0
80.00	738.0
81.00	2625.0
82.00	711.0
85.80	123.0
87.00	1902.0
88.00	3014.0
89.60	105.0
91.00	310.0
92.00	1865.0
93.10	3117.0
94.10	6744.0
95.10	50088.0
96.10	3906.0
96.90	126.0
100.10	101.0
104.00	378.0
104.90	142.0
106.00	497.0
108.00	104.0
110.00	122.0
113.20	232.0
116.00	360.0
116.90	667.0
118.00	313.0
119.00	361.0
120.80	111.0
122.00	108.0
128.10	155.0
129.40	231.0
130.00	169.0
130.80	151.0
134.00	117.0
137.10	209.0
140.00	133.0
141.00	617.0
143.00	996.0
144.10	136.0
145.00	398.0
156.90	152.0
171.20	107.0
171.90	1206.0
172.90	620.0
174.00	37592.0
175.00	3087.0
176.00	38032.0
177.00	2151.0
178.10	204.0
192.50	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB187

m/z	Abundance
35.10	209.0
35.50	245.0
36.00	119.0
36.60	126.0
37.00	135.0
37.80	211.0
39.10	106.0
40.00	290.0
40.80	128.0
41.50	114.0
42.70	133.0
44.20	624.0
45.00	140.0
45.80	113.0
47.70	101.0
48.90	114.0
55.90	147.0
56.70	151.0
58.60	122.0
70.20	131.0
70.50	127.0
75.00	111.0
76.20	141.0
77.00	101.0
83.00	140.0
91.10	112.0
131.20	159.0
140.90	107.0
160.10	136.0
167.20	105.0
176.60	130.0
181.30	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB187

m/z	Abundance
35.10	122.0
36.20	744.0
37.10	3542.0
38.10	2734.0
39.00	1440.0
40.00	367.0
42.30	154.0
44.10	813.0
45.00	434.0
46.00	306.0
47.10	746.0
48.00	481.0
49.10	2804.0
50.10	10430.0
51.10	2999.0
52.10	351.0
52.90	129.0
54.10	173.0
55.00	151.0
56.00	1039.0
57.10	1877.0
58.00	224.0
58.80	118.0
60.10	649.0
61.00	2981.0
62.10	2846.0
63.10	2904.0
64.10	260.0
65.10	577.0
66.00	144.0
66.80	229.0
68.10	5236.0
69.10	5501.0
70.20	464.0
72.00	540.0
73.10	2685.0
74.10	9502.0
75.10	27136.0
76.10	1595.0
77.30	377.0
78.00	206.0
79.00	2624.0
79.90	837.0
81.00	2730.0
82.00	896.0
87.00	2345.0
88.00	2726.0
90.60	284.0
91.10	430.0
92.10	2041.0
93.00	2838.0
94.10	6687.0
95.10	48712.0
96.10	3697.0
97.00	163.0
97.90	126.0
103.90	370.0
104.90	115.0
106.00	384.0
109.60	142.0
110.00	139.0
110.80	184.0
112.90	101.0
116.00	341.0
116.90	627.0
118.10	342.0
119.10	376.0
123.30	117.0
125.90	123.0
127.90	162.0
129.00	160.0
129.80	369.0
130.80	160.0
140.10	244.0
141.00	786.0
141.80	104.0
143.00	1085.0
144.90	253.0
145.70	133.0
148.00	166.0
148.70	121.0
150.50	168.0
152.20	109.0
154.90	111.0
156.80	119.0
157.40	115.0
160.80	111.0
165.90	104.0
168.20	219.0
172.00	948.0
173.20	502.0
174.00	39608.0

Instrument :
MSVOA_V
ClientSampleId :
BFB187

175.00	2937.0
176.00	37624.0
177.00	2604.0
178.10	194.0
206.20	195.0
277.40	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB187