

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042224\
 Data File : VW035330.D
 Acq On : 22 Apr 2024 14:06
 Operator : SY/MD
 Sample : P2182-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 23 00:30:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 23 00:28:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	157192	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	136641	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	48751	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	51416	33.869	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 67.740%			
7) Chloroethane-d5	1.532	69	67912	51.505	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.000%			
11) 1,1-Dichloroethene-d2	2.057	65	17916	26.923	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 53.840%#			
21) 2-Butanone-d5	3.989	46	160	0.178	ug/L	0.20
Spiked Amount 100.000	Range 40 - 130		Recovery = 0.180%#			
24) Chloroform-d	4.249	84	177288	69.460	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 138.920%#			
26) 1,2-Dichloroethane-d4	4.941	65	143311	88.436	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 176.880%#			
32) Benzene-d6	4.960	84	256607	55.908	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.820%			
36) 1,2-Dichloropropane-d6	5.986	67	119573	82.040	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 164.080%#			
41) Toluene-d8	7.246	98	143158	34.633	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 69.260%#			
43) trans-1,3-Dichloroprop...	7.558	79	37934	53.537	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 107.080%			
47) 2-Hexanone-d5	8.027	63	52704	95.642	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 95.640%			
56) 1,1,2,2-Tetrachloroeth...	10.149	84	219173	109.200	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 218.400%#			
66) 1,2-Dichlorobenzene-d4	11.558	152	59658	54.504	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 109.000%			
Target Compounds					Qvalue	
13) Acetone	2.121	43	6418	7.764	ug/L	98
48) 2-Hexanone	8.092	43	15207	11.373	ug/L #	92
51) Chlorobenzene	8.822	112	6060	2.004	ug/L	92
65) 1,4-Dichlorobenzene	11.214	146	5069	3.035	ug/L	96
67) 1,2-Dichlorobenzene	11.577	146	4876	2.980	ug/L	95
69) 1,3,5-Trichlorobenzene	13.204	180	2374	2.006	ug/L	97
70) 1,2,4-trichlorobenzene	13.204	180	2374	2.183	ug/L	97
71) Naphthalene	13.455	128	2817	0.934	ug/L #	82
72) 1,2,3-Trichlorobenzene	13.683	180	983	0.917	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035330.D
Acq On : 22 Apr 2024 14:06
Operator : SY/MD
Sample : P2182-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 23 00:30:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 23 00:28:07 2024
Response via : Initial Calibration

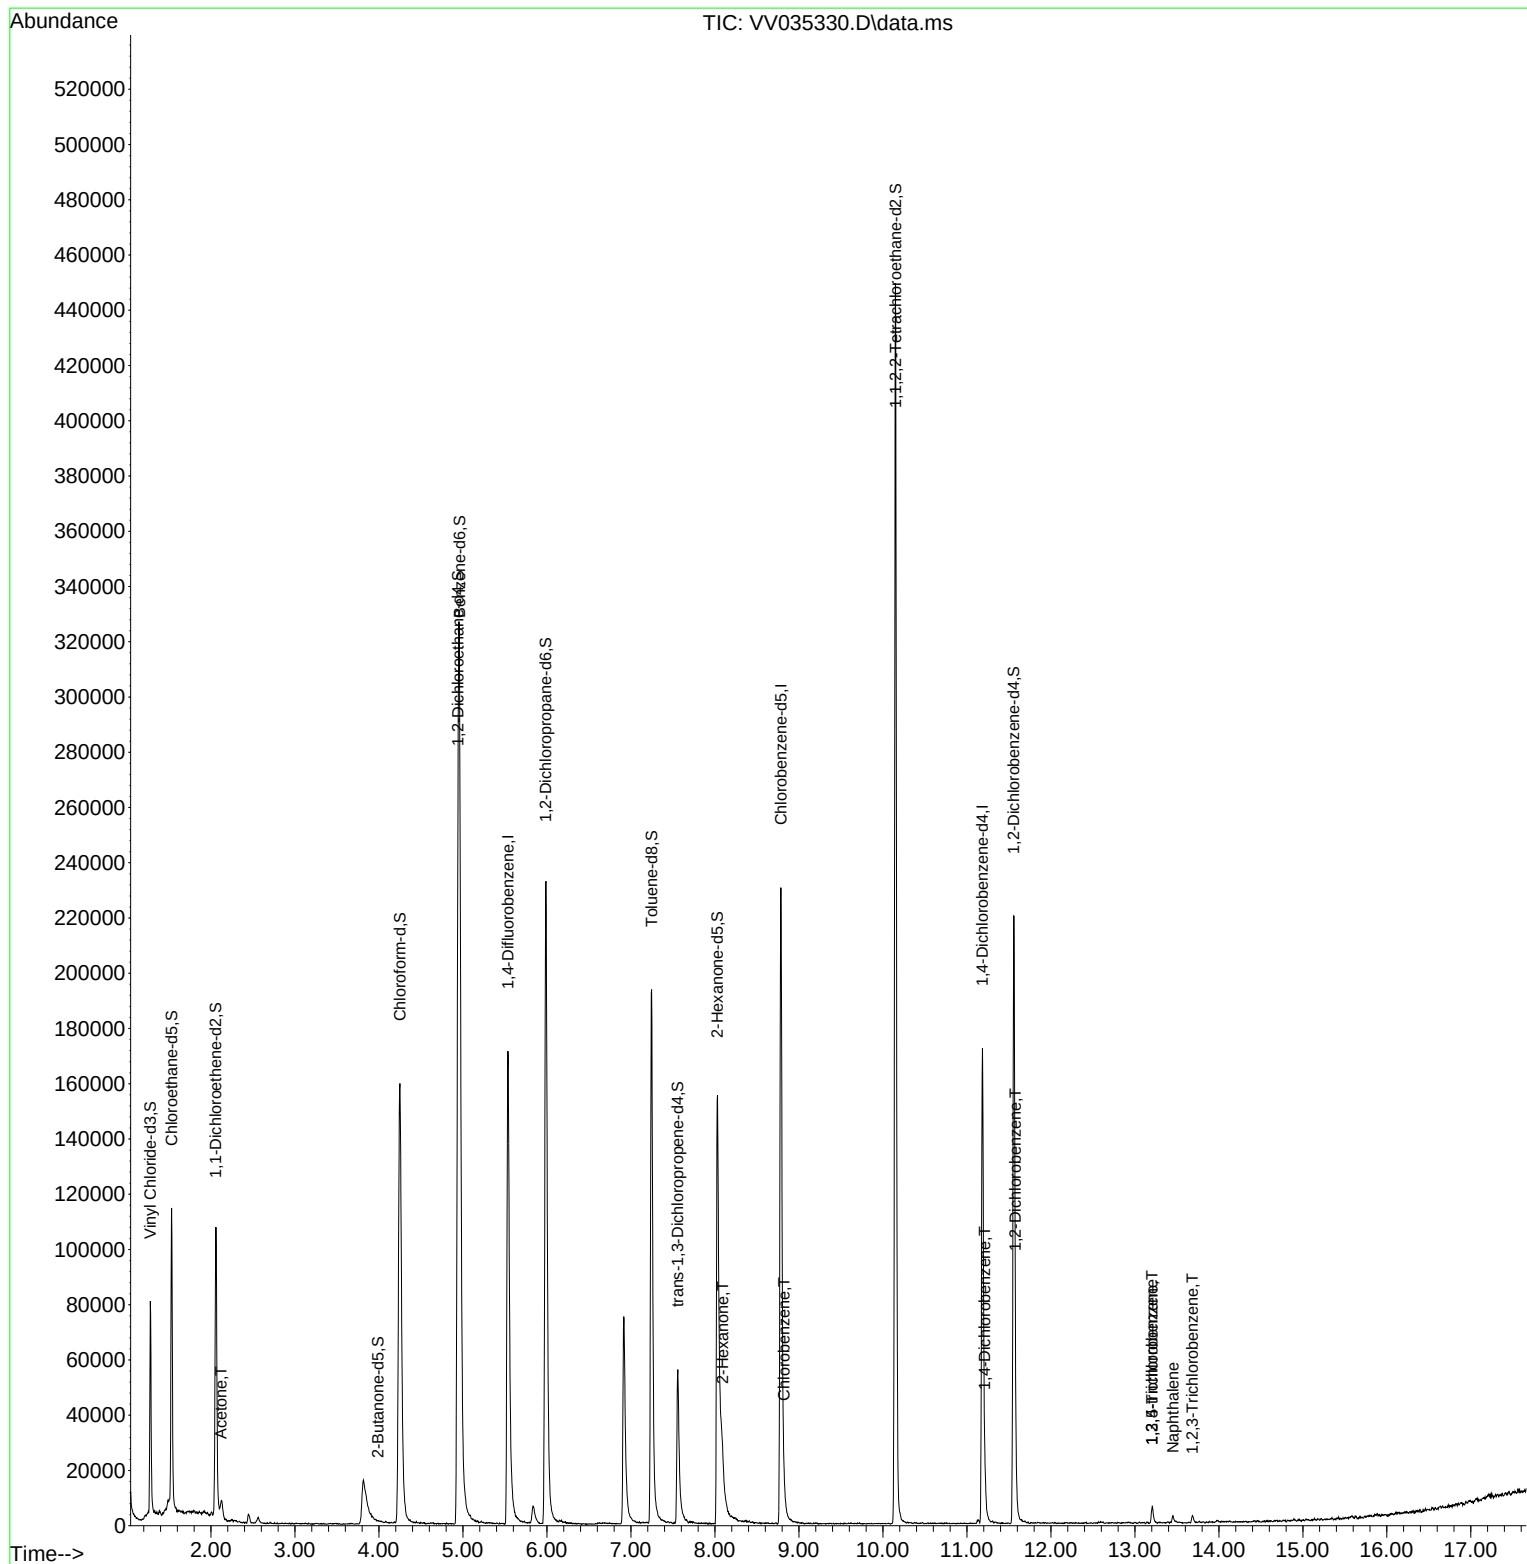

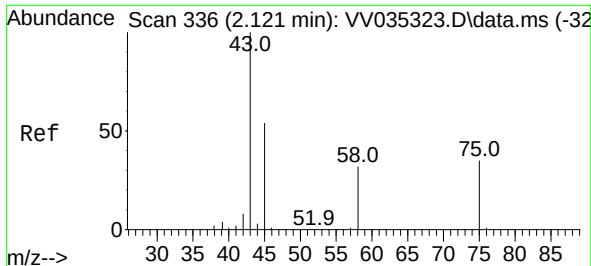

#13

Acetone

Concen: 7.764 ug/L

RT: 2.121 min Scan# 3

Delta R.T. 0.000 min


Lab File: VV035330.D

Acq: 22 Apr 2024 14:06

Instrument :

MSVOA_V

ClientSampleId :



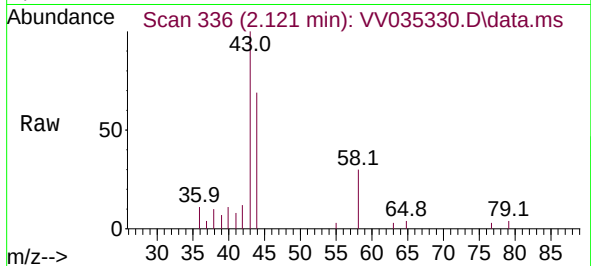


Tgt Ion: 43 Resp: 6418

Ion Ratio Lower Upper

43 100

58 31.9 0.0 66.0

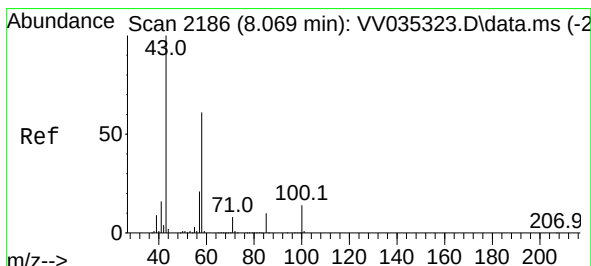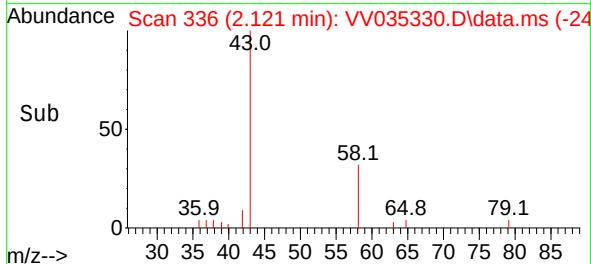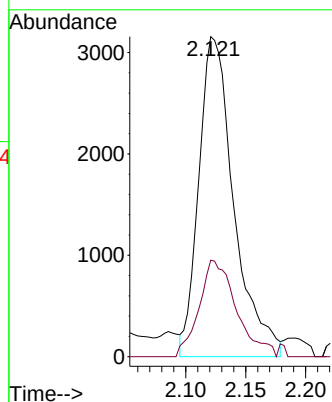

#48

2-Hexanone

Concen: 11.373 ug/L

RT: 8.092 min Scan# 2193

Delta R.T. 0.023 min

Lab File: VV035330.D

Acq: 22 Apr 2024 14:06

Tgt Ion: 43 Resp: 15207




Ion Ratio Lower Upper


43 100

58 52.7 45.4 68.2

57 18.3 16.2 24.4

100 2.4 10.1 15.1#

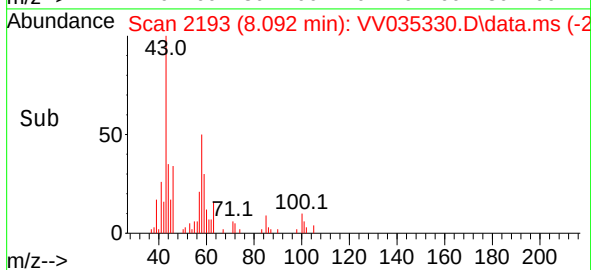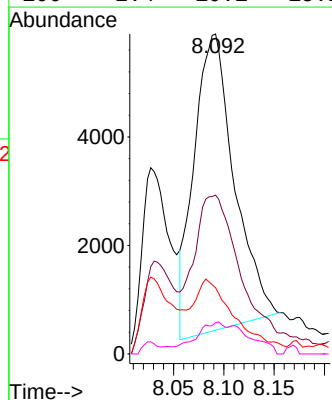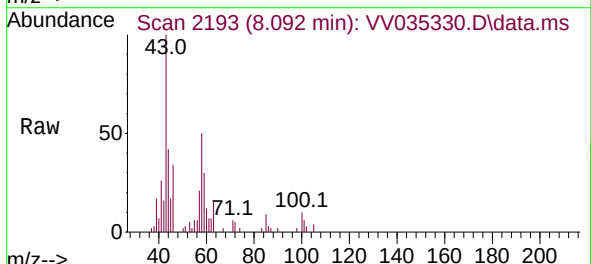



#51

Chlorobenzene

Concen: 2.004 ug/L

RT: 8.822 min Scan# 2416

Delta R.T. 0.013 min

Lab File: VV035330.D





Acq: 22 Apr 2024 14:06

Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion:112	Resp:	6060
Ion Ratio	Lower	Upper
112	100	
114	38.5	22.0 41.0
77	63.8	47.4 71.2

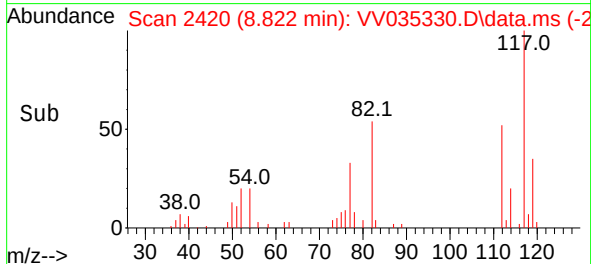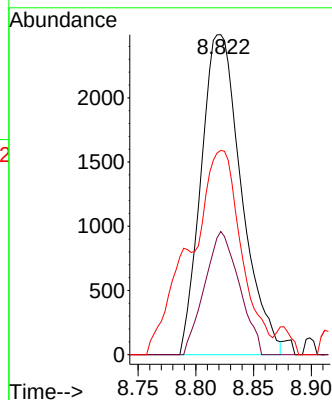

#65

1,4-Dichlorobenzene

Concen: 3.035 ug/L




RT: 11.214 min Scan# 3164


Delta R.T. 0.010 min

Lab File: VV035330.D

Acq: 22 Apr 2024 14:06


Tgt Ion:146	Resp:	5069
Ion Ratio	Lower	Upper
146	100	
111	34.7	27.4 50.8
148	65.2	44.2 82.2

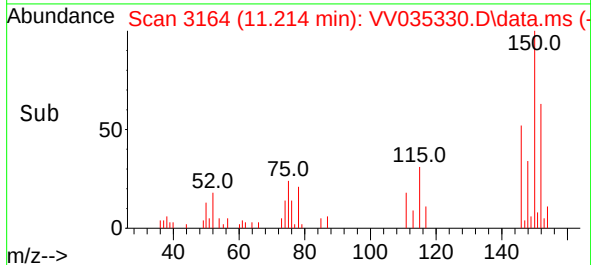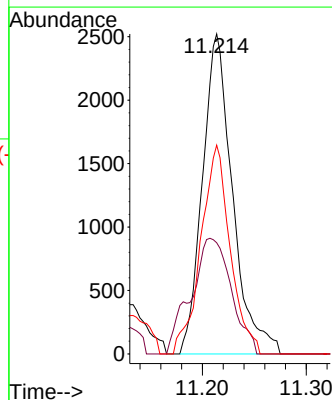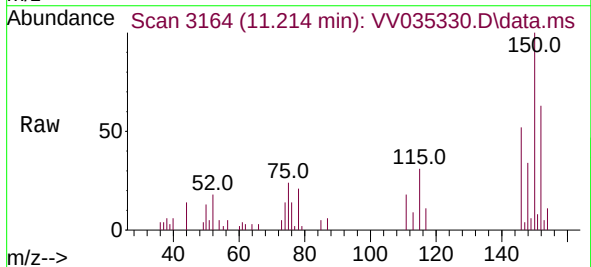






#67
1,2-Dichlorobenzene
Concen: 2.980 ug/L
RT: 11.577 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV035330.D
Acq: 22 Apr 2024 14:06

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion:146 Resp: 4876
Ion Ratio Lower Upper
146 100
111 50.9 34.6 52.0
148 64.4 51.5 77.3

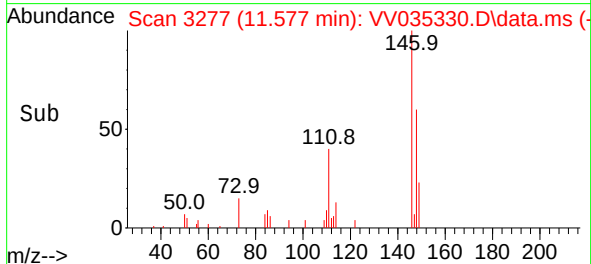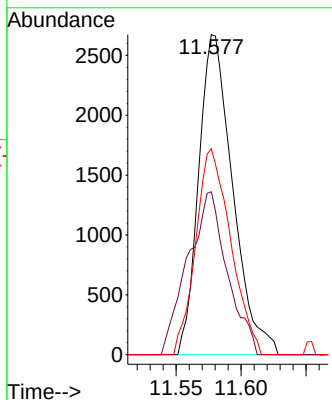

#69
1,3,5-Trichlorobenzene
Concen: 2.006 ug/L
RT: 13.204 min Scan# 3783
Delta R.T. 0.627 min
Lab File: VV035330.D
Acq: 22 Apr 2024 14:06

Tgt Ion:180 Resp: 2374
Ion Ratio Lower Upper
180 100
182 97.3 74.7 112.1
184 30.9 24.0 36.0
145 29.3 23.6 35.4

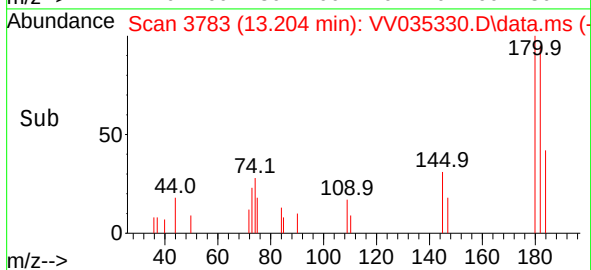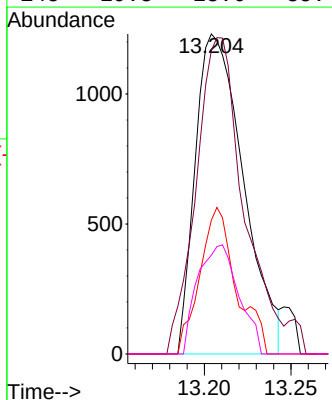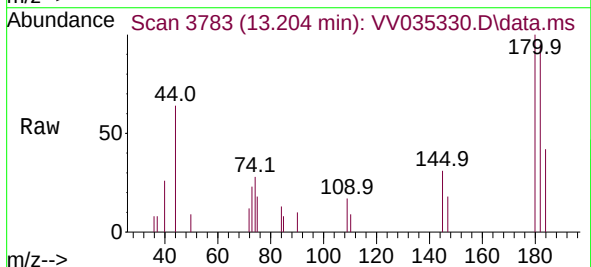



#70

1,2,4-trichlorobenzene

Concen: 2.183 ug/L

RT: 13.204 min Scan# 3783

Delta R.T. 0.010 min

Lab File: VV035330.D





Acq: 22 Apr 2024 14:06

Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion:180	Resp:	2374
Ion Ratio	Lower	Upper
180	100	
182	97.3	75.6 113.4
145	29.3	24.1 36.1

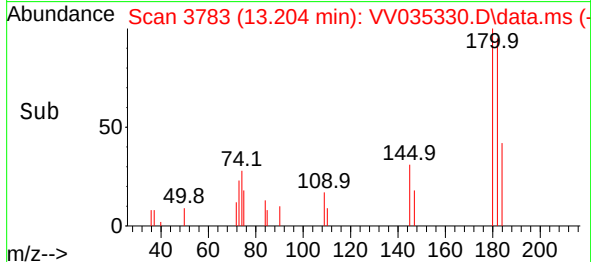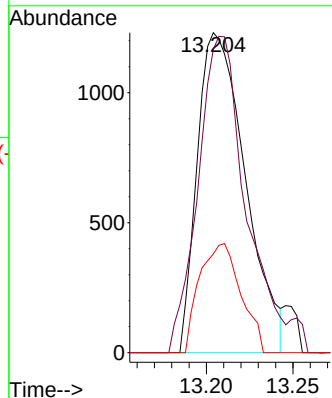

#71

Naphthalene

Concen: 0.934 ug/L




RT: 13.455 min Scan# 3861


Delta R.T. 0.019 min

Lab File: VV035330.D

Acq: 22 Apr 2024 14:06

Tgt Ion:128	Resp:	2817
Ion Ratio	Lower	Upper
128	100	
127	5.4	10.5 15.7#
129	4.5	8.7 13.1#

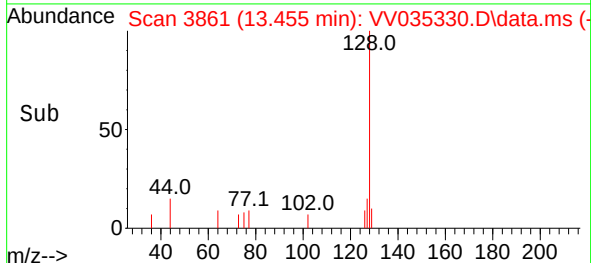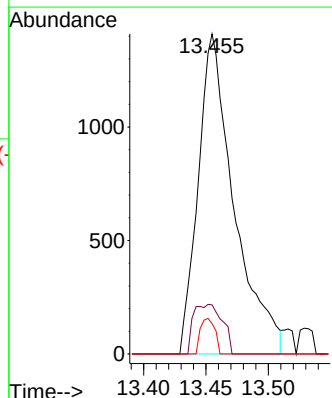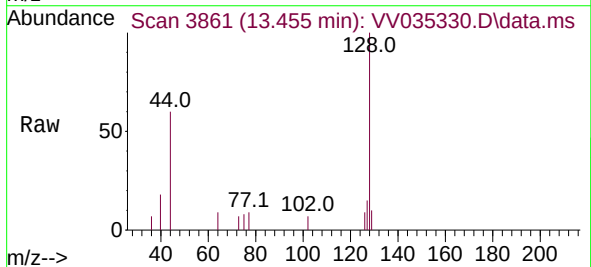



#72

1,2,3-Trichlorobenzene

Concen: 0.917 ug/L

RT: 13.683 min Scan# 3932

Delta R.T. 0.006 min


Lab File: VV035330.D

Acq: 22 Apr 2024 14:06

Instrument :

MSVOA_V

ClientSampleId :

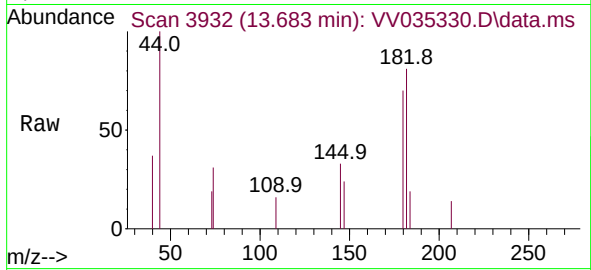

Tgt Ion:180 Resp: 983

Ion Ratio Lower Upper

180 100

182 108.3 76.2 114.2

145 37.2 25.8 38.6

