

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035324.D
 Acq On : 22 Apr 2024 11:49
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rBV	304853	327035	16.34%	2.288%
2	1.535	146	154	167	rVB	250085	294301	14.70%	2.059%
3	2.059	308	317	341	rVB	477873	695724	34.76%	4.868%
4	2.452	430	439	450	rVB6	2826	5062	0.25%	0.035%
5	2.551	467	470	471	rBV	452	267	0.01%	0.002%
6	2.793	543	545	548	rBV2	284	144	0.01%	0.001%
7	3.008	610	612	616	rBV2	218	120	0.01%	0.001%
8	3.143	651	654	656	rBV	152	105	0.01%	0.001%
9	3.204	670	673	678	rBV	206	137	0.01%	0.001%
10	3.230	679	681	684	rBV2	126	73	0.00%	0.001%
11	3.275	693	695	696	rBV	184	64	0.00%	0.000%
12	3.397	729	733	737	rBV3	216	201	0.01%	0.001%
13	3.413	737	738	740	rVB	136	27	0.00%	0.000%
14	3.439	740	746	748	rBV3	446	355	0.02%	0.002%
15	3.587	788	792	794	rBV	366	228	0.01%	0.002%
16	3.603	794	797	803	rVB	341	280	0.01%	0.002%
17	3.638	803	808	810	rBV2	363	272	0.01%	0.002%
18	3.719	831	833	838	rBV2	240	173	0.01%	0.001%
19	3.757	843	845	847	rBV2	215	118	0.01%	0.001%
20	3.793	847	856	901	rBV2	119232	384368	19.20%	2.689%
21	4.246	982	997	1029	rBV	307868	790744	39.50%	5.532%
22	4.866	1186	1190	1191	rBV2	313	190	0.01%	0.001%
23	4.953	1201	1217	1259	rBV2	754783	2001688	100.00%	14.005%
24	5.423	1360	1363	1365	rBV2	424	283	0.01%	0.002%
25	5.532	1386	1397	1437	rBV	466548	974511	48.68%	6.818%
26	5.834	1481	1491	1517	rVB3	10743	27871	1.39%	0.195%
27	5.924	1517	1519	1521	rBV2	358	147	0.01%	0.001%
28	5.985	1525	1538	1570	rBV	432323	903852	45.15%	6.324%
29	6.326	1642	1644	1647	rBV2	322	219	0.01%	0.002%
30	6.432	1674	1677	1679	rBV3	536	301	0.02%	0.002%
31	6.503	1696	1699	1701	rBV	217	126	0.01%	0.001%
32	6.535	1705	1709	1713	rVB3	399	351	0.02%	0.002%
33	6.558	1713	1716	1720	rBV2	287	221	0.01%	0.002%
34	6.577	1720	1722	1725	rVB2	365	157	0.01%	0.001%
35	6.593	1725	1727	1728	rBV2	258	108	0.01%	0.001%
36	6.616	1732	1734	1735	rBV	126	47	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035324.D
 Acq On : 22 Apr 2024 11:49
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.706	1760	1762	1763	rBV	449	158	0.01%	0.001%
38	6.725	1766	1768	1770	rVV2	527	238	0.01%	0.002%
39	6.738	1770	1772	1775	rVB2	459	213	0.01%	0.001%
40	6.789	1785	1788	1792	rVB2	311	201	0.01%	0.001%
41	6.808	1792	1794	1796	rBV	214	86	0.00%	0.001%
42	6.911	1816	1826	1855	rBV	212509	411391	20.55%	2.878%
43	7.239	1917	1928	1955	rBV	886139	1562496	78.06%	10.932%
44	7.551	2015	2025	2066	rBV	147265	283196	14.15%	1.981%
45	8.024	2163	2172	2219	rBV2	344240	831096	41.52%	5.815%
46	8.644	2363	2365	2366	rBV	398	157	0.01%	0.001%
47	8.699	2380	2382	2383	rBV	444	233	0.01%	0.002%
48	8.722	2387	2389	2393	rBV	191	86	0.00%	0.001%
49	8.783	2397	2408	2436	rBV	737512	1220624	60.98%	8.540%
50	9.185	2532	2533	2536	rBV2	157	101	0.01%	0.001%
51	9.313	2571	2573	2575	rVB2	340	137	0.01%	0.001%
52	9.336	2575	2580	2585	rBV3	431	526	0.03%	0.004%
53	9.374	2588	2592	2595	rVV2	226	172	0.01%	0.001%
54	9.390	2595	2597	2599	rVV2	377	228	0.01%	0.002%
55	9.413	2602	2604	2605	rVB2	210	60	0.00%	0.000%
56	9.487	2621	2627	2632	rBV4	936	1160	0.06%	0.008%
57	9.587	2656	2658	2661	rBV2	339	208	0.01%	0.001%
58	9.619	2665	2668	2669	rBV	192	114	0.01%	0.001%
59	9.657	2677	2680	2683	rVB2	407	220	0.01%	0.002%
60	9.677	2683	2686	2691	rBV4	465	368	0.02%	0.003%
61	9.873	2739	2747	2755	rBV4	1184	1833	0.09%	0.013%
62	10.005	2786	2788	2789	rBV	164	71	0.00%	0.000%
63	10.021	2790	2793	2798	rVB2	258	224	0.01%	0.002%
64	10.050	2798	2802	2804	rBV2	316	268	0.01%	0.002%
65	10.149	2820	2833	2866	rBV	589665	942979	47.11%	6.597%
66	10.487	2930	2938	2942	rBV3	1318	1615	0.08%	0.011%
67	10.535	2951	2953	2957	rVB3	186	65	0.00%	0.000%
68	10.677	2995	2997	3002	rBV	290	172	0.01%	0.001%
69	10.860	3049	3054	3058	rBV4	1235	1464	0.07%	0.010%
70	11.043	3108	3111	3115	rVB2	266	180	0.01%	0.001%
71	11.066	3115	3118	3120	rBV2	202	141	0.01%	0.001%
72	11.127	3130	3137	3144	rBV3	4074	6440	0.32%	0.045%
73	11.181	3144	3154	3180	rVV	686559	1111540	55.53%	7.777%
74	11.557	3259	3271	3297	rBV	861209	1382303	69.06%	9.671%
75	11.953	3392	3394	3395	rBV	450	191	0.01%	0.001%
76	12.168	3457	3461	3463	rBV2	361	313	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035324.D
Acq On : 22 Apr 2024 11:49
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	12.586	3585	3591	3605	rVB3	4932	8447	0.42%	0.059%
78	13.117	3753	3756	3760	rBV2	493	325	0.02%	0.002%
79	13.201	3773	3782	3793	rBV2	13657	22121	1.11%	0.155%
80	13.442	3848	3857	3874	rBV	39528	67363	3.37%	0.471%
81	13.683	3924	3932	3947	rVB2	14008	21748	1.09%	0.152%




Sum of corrected areas: 14293142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035324.D
Acq On : 22 Apr 2024 11:49
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

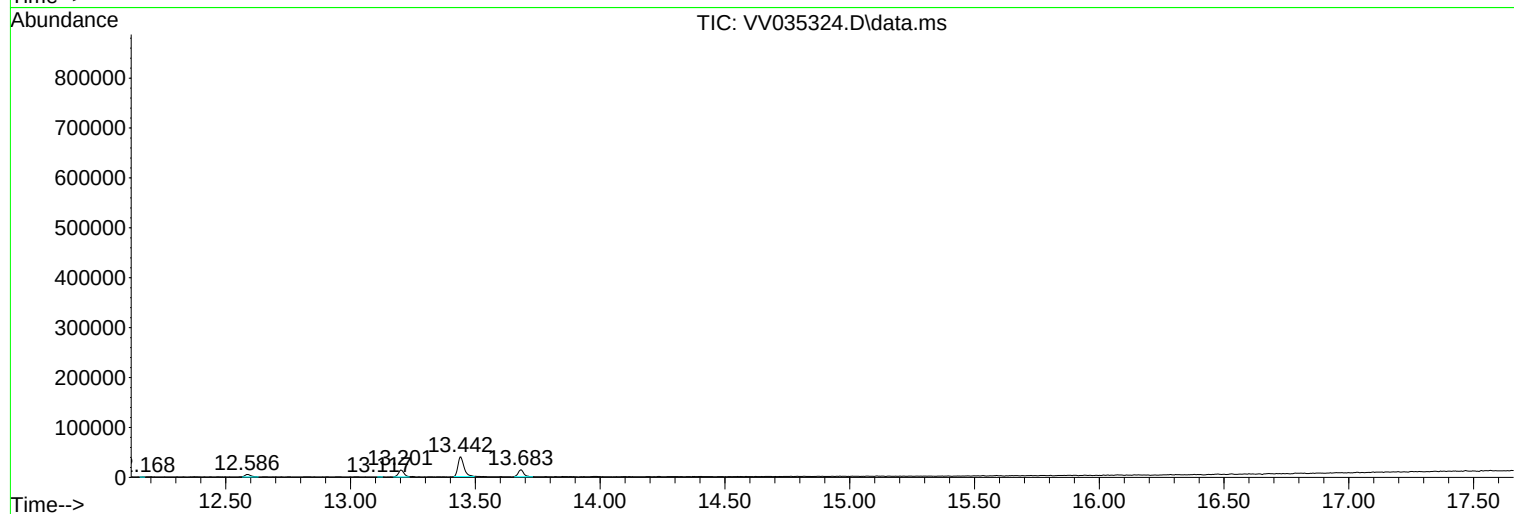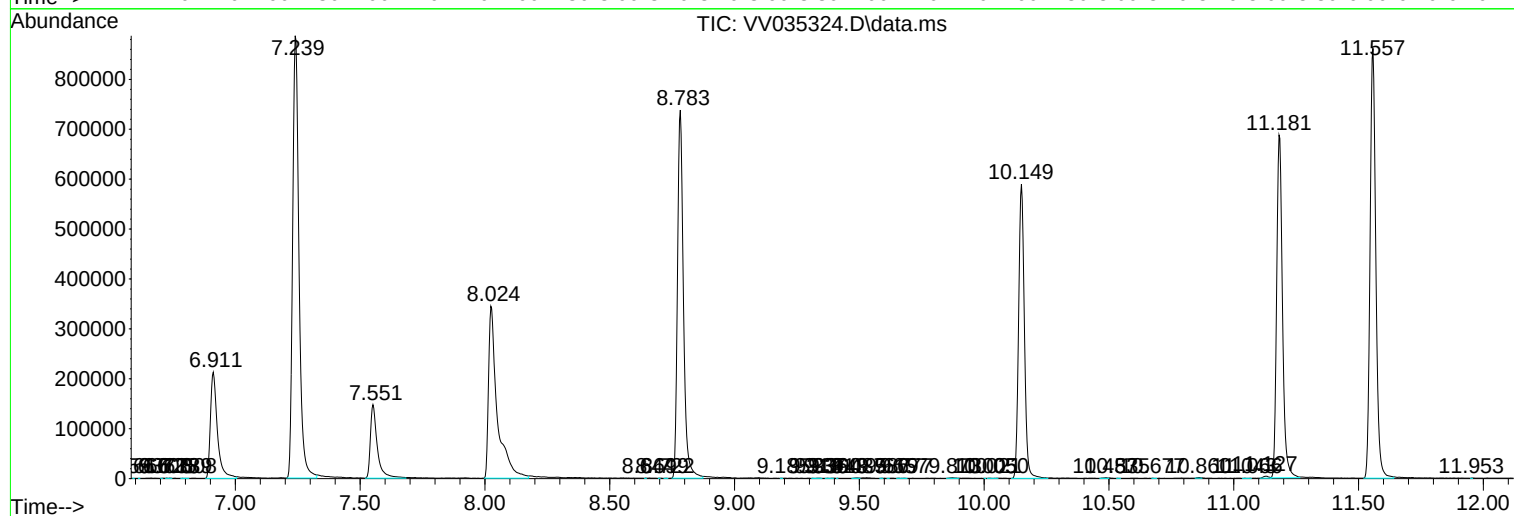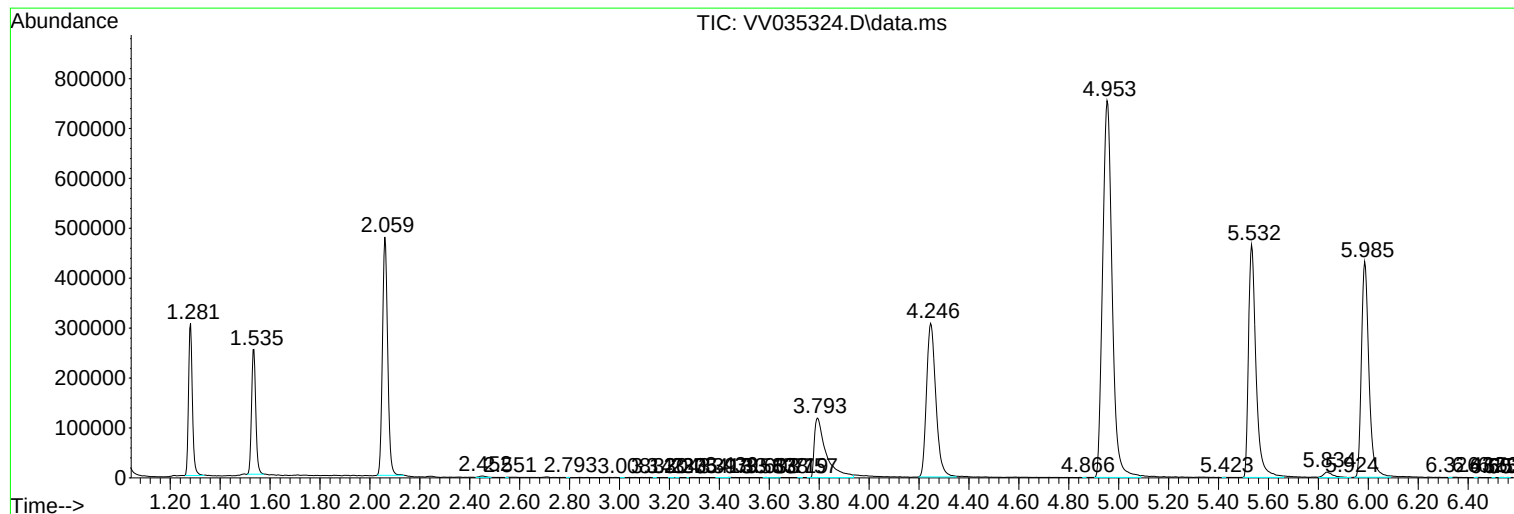

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035324.D
Acq On : 22 Apr 2024 11:49
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035324.D
Acq On : 22 Apr 2024 11:49
Operator : SY/MD
Sample : VV0422WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
