

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035325.D
 Acq On : 22 Apr 2024 12:12
 Operator : SY/MD
 Sample : P2182-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rBV	137670	143650	9.93%	1.534%
2	1.532	147	153	169	rVB	147826	176155	12.18%	1.881%
3	2.060	308	317	332	rBV	202229	296902	20.52%	3.170%
4	2.449	432	438	445	rBV6	2316	3372	0.23%	0.036%
5	2.545	465	468	469	rBV2	803	503	0.03%	0.005%
6	2.687	510	512	513	rBV	482	174	0.01%	0.002%
7	2.809	548	550	551	rBV	206	94	0.01%	0.001%
8	2.851	561	563	569	rBV	250	191	0.01%	0.002%
9	2.986	601	605	610	rBV2	439	448	0.03%	0.005%
10	3.056	625	627	630	rVB	357	116	0.01%	0.001%
11	3.085	633	636	637	rBV	190	105	0.01%	0.001%
12	3.137	650	652	654	rVV	505	205	0.01%	0.002%
13	3.150	654	656	658	rVB	296	129	0.01%	0.001%
14	3.253	686	688	690	rBV2	194	127	0.01%	0.001%
15	3.288	695	699	705	rBV3	323	356	0.02%	0.004%
16	3.327	709	711	713	rVB	140	65	0.00%	0.001%
17	3.352	713	719	720	rBV2	119	103	0.01%	0.001%
18	3.359	720	721	728	rVB2	286	220	0.02%	0.002%
19	3.410	728	737	739	rBV2	327	504	0.03%	0.005%
20	3.452	745	750	752	rBV	249	198	0.01%	0.002%
21	3.497	761	764	767	rBV2	190	161	0.01%	0.002%
22	3.542	775	778	780	rBV	137	66	0.00%	0.001%
23	3.558	780	783	784	rBV	146	95	0.01%	0.001%
24	3.581	787	790	792	rBV2	226	119	0.01%	0.001%
25	3.632	802	806	808	rBV2	327	257	0.02%	0.003%
26	3.674	816	819	824	rVB2	206	160	0.01%	0.002%
27	3.696	824	826	827	rBV2	160	71	0.00%	0.001%
28	3.764	845	847	849	rVB	250	126	0.01%	0.001%
29	3.831	849	868	877	rBV2	8245	26783	1.85%	0.286%
30	4.249	979	998	1036	rBV	220330	582110	40.24%	6.215%
31	4.616	1110	1112	1117	rVB2	426	285	0.02%	0.003%
32	4.638	1117	1119	1120	rBV	163	87	0.01%	0.001%
33	4.696	1135	1137	1139	rBV2	187	80	0.01%	0.001%
34	4.735	1143	1149	1156	rVB5	625	920	0.06%	0.010%
35	4.796	1165	1168	1171	rBV	253	163	0.01%	0.002%
36	4.825	1175	1177	1179	rBV	202	123	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035325.D
 Acq On : 22 Apr 2024 12:12
 Operator : SY/MD
 Sample : P2182-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.953	1202	1217	1265	rBV2	483106	1446700	100.00%	15.445%
38	5.413	1355	1360	1361	rBV2	318	253	0.02%	0.003%
39	5.420	1361	1362	1366	rVV	355	197	0.01%	0.002%
40	5.532	1383	1397	1425	rBV	318648	681099	47.08%	7.271%
41	5.838	1482	1492	1511	rVB6	7754	17425	1.20%	0.186%
42	5.986	1526	1538	1567	rBV	315219	658959	45.55%	7.035%
43	6.323	1641	1643	1646	rBV2	191	79	0.01%	0.001%
44	6.349	1649	1651	1654	rVB3	630	245	0.02%	0.003%
45	6.397	1664	1666	1669	rVB2	218	116	0.01%	0.001%
46	6.439	1675	1679	1680	rBV	164	114	0.01%	0.001%
47	6.510	1698	1701	1702	rBV	265	101	0.01%	0.001%
48	6.564	1715	1718	1723	rVB2	287	265	0.02%	0.003%
49	6.619	1731	1735	1737	rBV3	291	260	0.02%	0.003%
50	6.815	1794	1796	1800	rVB	292	186	0.01%	0.002%
51	6.838	1800	1803	1805	rBV2	319	236	0.02%	0.003%
52	6.870	1811	1813	1814	rBV	308	151	0.01%	0.002%
53	6.915	1817	1827	1855	rBV	113586	228030	15.76%	2.434%
54	7.243	1918	1929	1967	rBV	401893	733226	50.68%	7.828%
55	7.555	2017	2026	2050	rBV	80699	160377	11.09%	1.712%
56	7.860	2119	2121	2124	rBV	472	369	0.03%	0.004%
57	7.912	2135	2137	2139	rVB2	424	173	0.01%	0.002%
58	7.950	2146	2149	2153	rBV	285	222	0.02%	0.002%
59	8.031	2165	2174	2208	rBV2	147613	378274	26.15%	4.038%
60	8.529	2324	2329	2334	rBV4	606	812	0.06%	0.009%
61	8.564	2338	2340	2341	rBV4	297	132	0.01%	0.001%
62	8.667	2370	2372	2374	rVB4	240	71	0.00%	0.001%
63	8.719	2385	2388	2390	rBV2	301	162	0.01%	0.002%
64	8.783	2397	2408	2414	rBV	479109	796483	55.06%	8.503%
65	9.153	2520	2523	2525	rBV2	301	194	0.01%	0.002%
66	9.252	2549	2554	2558	rBV2	430	454	0.03%	0.005%
67	9.310	2570	2572	2575	rBV3	244	158	0.01%	0.002%
68	9.403	2599	2601	2602	rBV	182	87	0.01%	0.001%
69	9.413	2602	2604	2606	rVV	216	87	0.01%	0.001%
70	9.448	2613	2615	2618	rVB2	325	168	0.01%	0.002%
71	9.468	2618	2621	2625	rBV3	233	219	0.02%	0.002%
72	9.712	2694	2697	2698	rBV	230	133	0.01%	0.001%
73	9.764	2710	2713	2715	rBV	199	147	0.01%	0.002%
74	9.812	2726	2728	2732	rVB	200	110	0.01%	0.001%
75	9.831	2732	2734	2736	rBV	258	115	0.01%	0.001%
76	9.870	2743	2746	2749	rBV3	631	450	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035325.D
 Acq On : 22 Apr 2024 12:12
 Operator : SY/MD
 Sample : P2182-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.002	2784	2787	2792	rVB2	418	409	0.03%	0.004%
78	10.034	2792	2797	2798	rBV	302	262	0.02%	0.003%
79	10.085	2810	2813	2818	rVB2	209	131	0.01%	0.001%
80	10.149	2821	2833	2861	rBV	518735	828933	57.30%	8.850%
81	10.400	2908	2911	2912	rBV	271	146	0.01%	0.002%
82	10.442	2922	2924	2927	rVB	225	135	0.01%	0.001%
83	10.551	2954	2958	2963	rBV2	324	359	0.02%	0.004%
84	10.603	2971	2974	2976	rBV	238	167	0.01%	0.002%
85	10.699	3002	3004	3010	rVB2	240	176	0.01%	0.002%
86	10.728	3010	3013	3014	rBV	273	147	0.01%	0.002%
87	10.918	3069	3072	3074	rBV	367	179	0.01%	0.002%
88	10.998	3094	3097	3104	rBV2	348	311	0.02%	0.003%
89	11.079	3118	3122	3125	rBV2	388	329	0.02%	0.004%
90	11.120	3126	3135	3145	rBV	32631	53063	3.67%	0.566%
91	11.185	3145	3155	3183	rVB2	390128	847713	58.60%	9.050%
92	11.403	3220	3223	3226	rBV2	412	351	0.02%	0.004%
93	11.561	3259	3272	3309	rBV3	508076	1096786	75.81%	11.709%
94	11.815	3349	3351	3356	rVB2	622	430	0.03%	0.005%
95	12.243	3482	3484	3487	rBV	340	216	0.01%	0.002%
96	12.590	3585	3592	3603	rVB6	2882	4951	0.34%	0.053%
97	13.201	3772	3782	3798	rBV	67963	110575	7.64%	1.180%
98	13.339	3821	3825	3828	rBV2	466	374	0.03%	0.004%
99	13.442	3849	3857	3875	rBV	17776	31168	2.15%	0.333%
100	13.680	3921	3931	3945	rBV2	29777	47371	3.27%	0.506%




Sum of corrected areas: 9366944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035325.D
Acq On : 22 Apr 2024 12:12
Operator : SY/MD
Sample : P2182-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

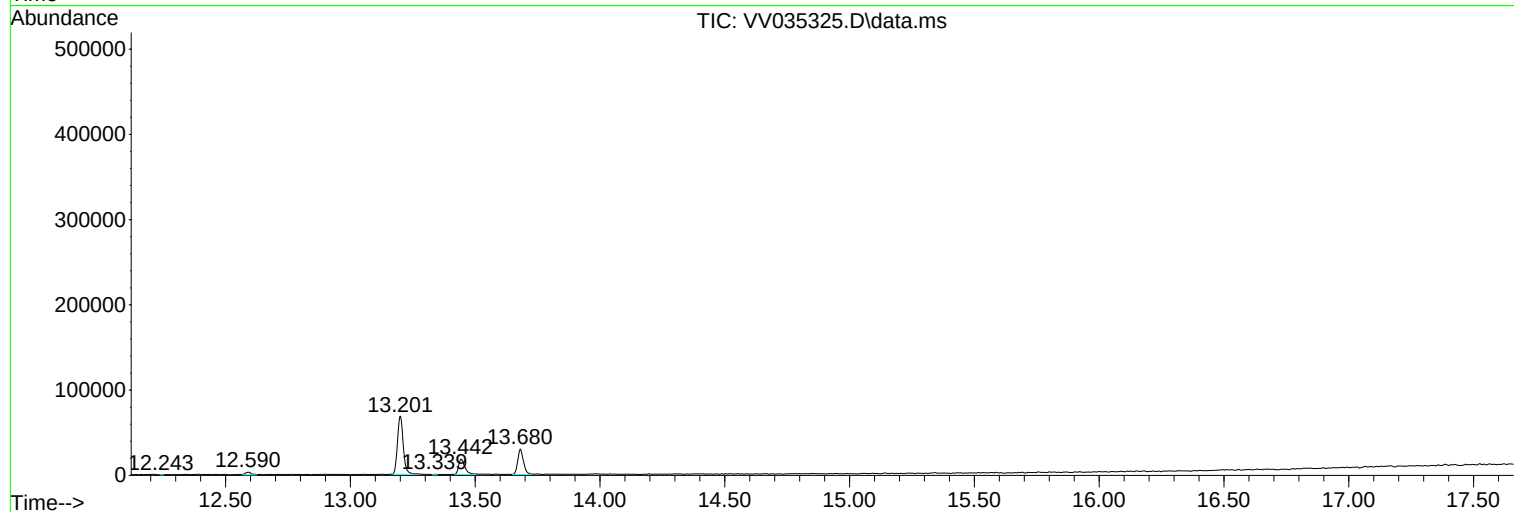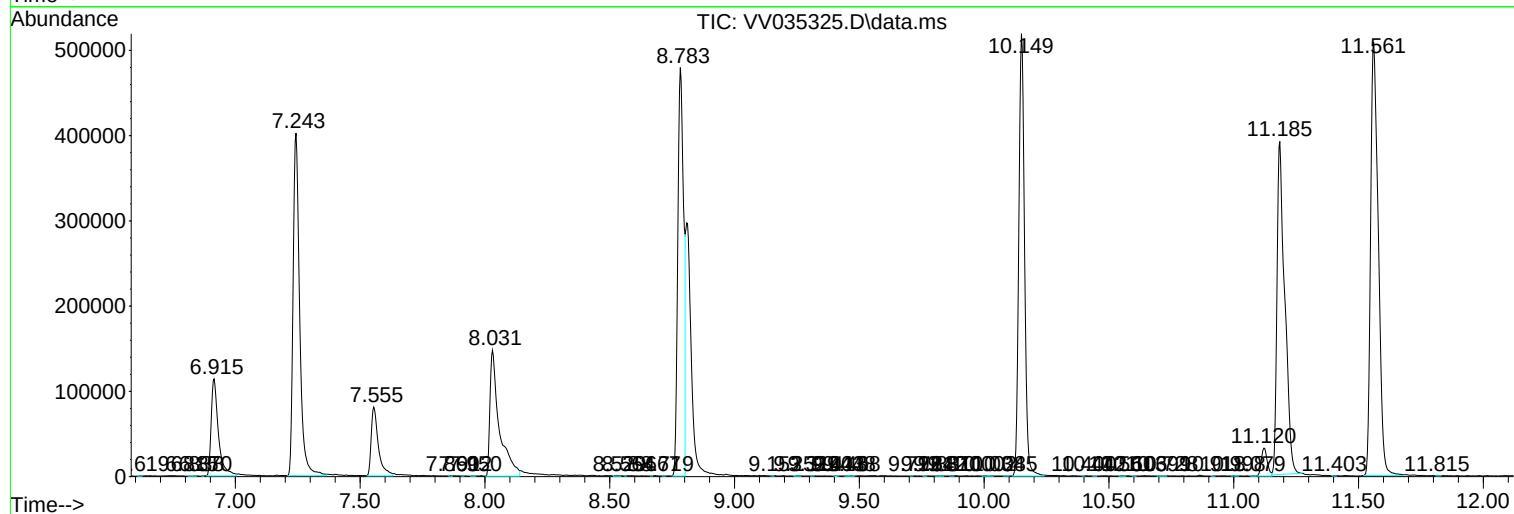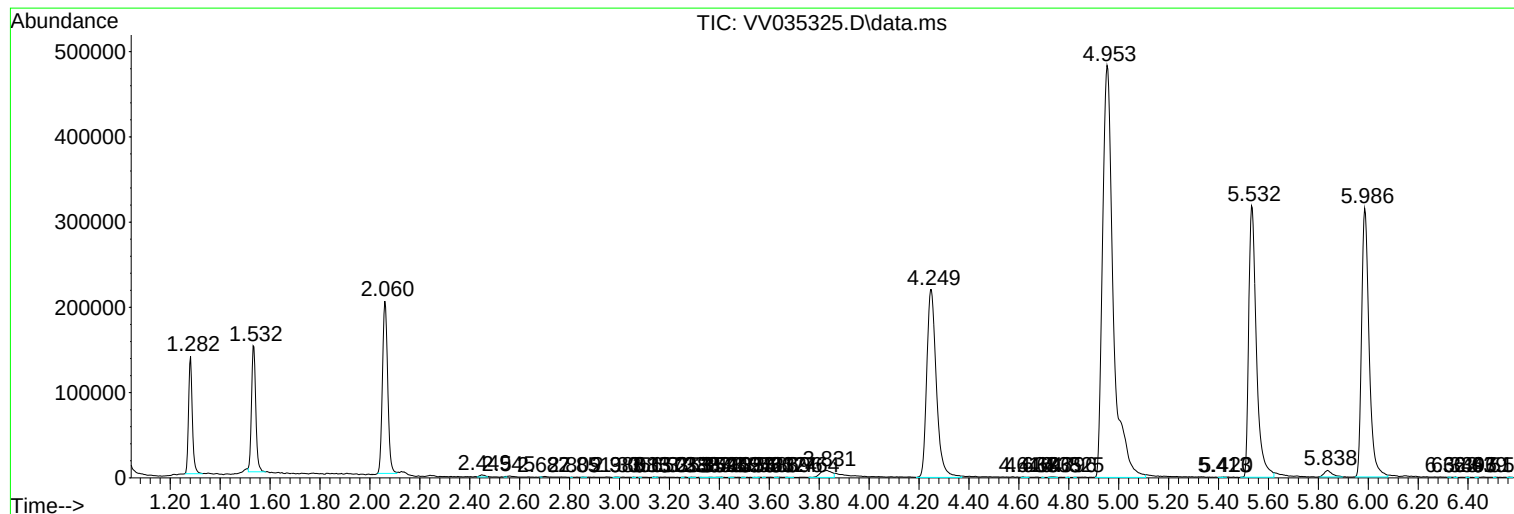

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035325.D
Acq On : 22 Apr 2024 12:12
Operator : SY/MD
Sample : P2182-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035325.D
Acq On : 22 Apr 2024 12:12
Operator : SY/MD
Sample : P2182-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc