

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035326.D
 Acq On : 22 Apr 2024 12:35
 Operator : SY/MD
 Sample : P2182-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	122757	132621	0.65%	0.333%
2	1.532	147	153	169	rVB	143527	169155	0.82%	0.425%
3	2.060	308	317	329	rBV	177532	258277	1.26%	0.649%
4	2.452	430	439	450	rVB2	7605	12625	0.06%	0.032%
5	2.664	502	505	510	rBV3	358	284	0.00%	0.001%
6	2.703	514	517	519	rVV2	487	302	0.00%	0.001%
7	2.719	519	522	525	rVB3	348	269	0.00%	0.001%
8	2.735	525	527	529	rBV2	465	198	0.00%	0.000%
9	2.764	534	536	538	rBV	258	121	0.00%	0.000%
10	2.857	560	565	572	rBV3	312	508	0.00%	0.001%
11	2.889	572	575	578	rBV	286	189	0.00%	0.000%
12	2.957	594	596	602	rVB2	583	355	0.00%	0.001%
13	2.989	602	606	609	rBV2	334	305	0.00%	0.001%
14	3.008	609	612	613	rBV2	316	162	0.00%	0.000%
15	3.040	619	622	626	rVB2	349	227	0.00%	0.001%
16	3.066	626	630	631	rVV	198	104	0.00%	0.000%
17	3.079	631	634	639	rVB2	216	176	0.00%	0.000%
18	3.150	653	656	660	rVB2	383	283	0.00%	0.001%
19	3.223	673	679	680	rBV	269	214	0.00%	0.001%
20	3.272	690	694	697	rBV2	182	177	0.00%	0.000%
21	3.426	739	742	746	rVB3	221	137	0.00%	0.000%
22	3.449	746	749	751	rBV2	338	206	0.00%	0.001%
23	3.513	765	769	770	rBV2	170	110	0.00%	0.000%
24	3.519	770	771	775	rVB	393	152	0.00%	0.000%
25	3.558	780	783	788	rVB3	300	279	0.00%	0.001%
26	3.584	788	791	794	rBV2	289	156	0.00%	0.000%
27	3.606	794	798	800	rBV	113	83	0.00%	0.000%
28	3.619	800	802	804	rVB	183	91	0.00%	0.000%
29	3.641	804	809	812	rBV3	168	145	0.00%	0.000%
30	3.664	812	816	817	rBV2	415	270	0.00%	0.001%
31	3.712	827	831	833	rBV	156	125	0.00%	0.000%
32	3.738	837	839	843	rVB2	230	171	0.00%	0.000%
33	3.764	843	847	849	rBV2	296	210	0.00%	0.001%
34	3.825	850	866	884	rBV2	8895	36338	0.18%	0.091%
35	4.249	983	998	1033	rBV	210751	558306	2.72%	1.402%
36	4.481	1068	1070	1074	rBV2	377	195	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035326.D
 Acq On : 22 Apr 2024 12:35
 Operator : SY/MD
 Sample : P2182-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.641	1119	1120	1124	rBV	235	129	0.00%	0.000%
38	4.738	1147	1150	1155	rVB3	344	273	0.00%	0.001%
39	4.764	1155	1158	1160	rBV	143	94	0.00%	0.000%
40	4.780	1160	1163	1166	rVB	390	206	0.00%	0.001%
41	4.821	1173	1176	1180	rBV2	129	107	0.00%	0.000%
42	4.844	1180	1183	1187	rBV2	203	173	0.00%	0.000%
43	4.883	1193	1195	1198	rBV2	186	90	0.00%	0.000%
44	4.957	1201	1218	1222	rBV2	480103	1044230	5.09%	2.622%
45	5.535	1387	1398	1437	rBV	283833	609636	2.97%	1.531%
46	5.834	1482	1491	1494	rBV4	4955	7162	0.03%	0.018%
47	5.985	1526	1538	1572	rBV	298326	631616	3.08%	1.586%
48	6.329	1642	1645	1646	rBV2	386	181	0.00%	0.000%
49	6.407	1666	1669	1674	rVB	339	270	0.00%	0.001%
50	6.439	1677	1679	1684	rVV	247	160	0.00%	0.000%
51	6.468	1684	1688	1690	rVV3	285	231	0.00%	0.001%
52	6.487	1691	1694	1696	rVV2	209	114	0.00%	0.000%
53	6.500	1696	1698	1700	rVB	198	78	0.00%	0.000%
54	6.513	1700	1702	1707	rVB2	234	141	0.00%	0.000%
55	6.545	1709	1712	1716	rVB3	166	129	0.00%	0.000%
56	6.590	1723	1726	1728	rBV	144	85	0.00%	0.000%
57	6.619	1731	1735	1738	rVV2	454	376	0.00%	0.001%
58	6.728	1767	1769	1773	rVB3	346	139	0.00%	0.000%
59	6.770	1779	1782	1784	rVB4	657	412	0.00%	0.001%
60	6.786	1784	1787	1788	rBV	309	136	0.00%	0.000%
61	6.812	1793	1795	1799	rBV2	264	170	0.00%	0.000%
62	6.850	1804	1807	1810	rBV	389	233	0.00%	0.001%
63	6.915	1817	1827	1852	rBV	108733	217599	1.06%	0.546%
64	7.101	1883	1885	1886	rBV	447	139	0.00%	0.000%
65	7.243	1919	1929	1954	rBV	361738	649782	3.16%	1.632%
66	7.555	2018	2026	2050	rBV	76914	147963	0.72%	0.372%
67	7.780	2093	2096	2099	rVB3	599	332	0.00%	0.001%
68	7.837	2112	2114	2117	rBV	336	180	0.00%	0.000%
69	7.876	2123	2126	2131	rVB3	401	336	0.00%	0.001%
70	7.899	2131	2133	2135	rBV2	277	127	0.00%	0.000%
71	7.911	2135	2137	2140	rBV2	521	401	0.00%	0.001%
72	7.969	2152	2155	2160	rVB2	401	258	0.00%	0.001%
73	7.995	2160	2163	2165	rBV2	302	239	0.00%	0.001%
74	8.030	2165	2174	2212	rBV2	167082	410971	2.00%	1.032%
75	8.545	2333	2334	2336	rBV	285	120	0.00%	0.000%
76	8.590	2346	2348	2349	rBV	247	103	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035326.D
 Acq On : 22 Apr 2024 12:35
 Operator : SY/MD
 Sample : P2182-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	8.619	2355	2357	2363	rBV2	338	381	0.00%	0.001%
78	8.680	2374	2376	2377	rBV	249	108	0.00%	0.000%
79	8.812	2397	2417	2463	rBV	12485961	20533571	100.00%	51.559%
80	9.805	2724	2726	2728	rBV2	424	249	0.00%	0.001%
81	9.870	2743	2746	2754	rBV6	618	666	0.00%	0.002%
82	9.947	2768	2770	2773	rVB	318	155	0.00%	0.000%
83	9.988	2781	2783	2786	rBV	315	194	0.00%	0.000%
84	10.005	2786	2788	2791	rVV4	394	242	0.00%	0.001%
85	10.101	2817	2818	2821	rBV	197	124	0.00%	0.000%
86	10.149	2821	2833	2863	rBV	515534	818620	3.99%	2.056%
87	10.323	2885	2887	2890	rBV2	457	255	0.00%	0.001%
88	10.468	2927	2932	2933	rBV2	491	471	0.00%	0.001%
89	10.689	2997	3001	3005	rBV2	380	331	0.00%	0.001%
90	10.757	3016	3022	3025	rBV4	400	447	0.00%	0.001%
91	10.841	3045	3048	3050	rBV2	298	227	0.00%	0.001%
92	10.908	3066	3069	3072	rVB3	452	267	0.00%	0.001%
93	11.117	3123	3134	3145	rBV	145199	231379	1.13%	0.581%
94	11.204	3146	3161	3190	rVB	3821589	6253352	30.45%	15.702%
95	11.574	3260	3276	3306	rBV2	4029430	6798604	33.11%	17.071%
96	11.969	3397	3399	3406	rVB6	754	648	0.00%	0.002%
97	12.127	3446	3448	3449	rBV6	401	148	0.00%	0.000%
98	13.197	3771	3781	3802	rBV	128592	208791	1.02%	0.524%
99	13.445	3851	3858	3869	rBV	11241	19049	0.09%	0.048%
100	13.680	3922	3931	3945	rBV	36003	58510	0.28%	0.147%




Sum of corrected areas: 39825436

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035326.D
Acq On : 22 Apr 2024 12:35
Operator : SY/MD
Sample : P2182-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

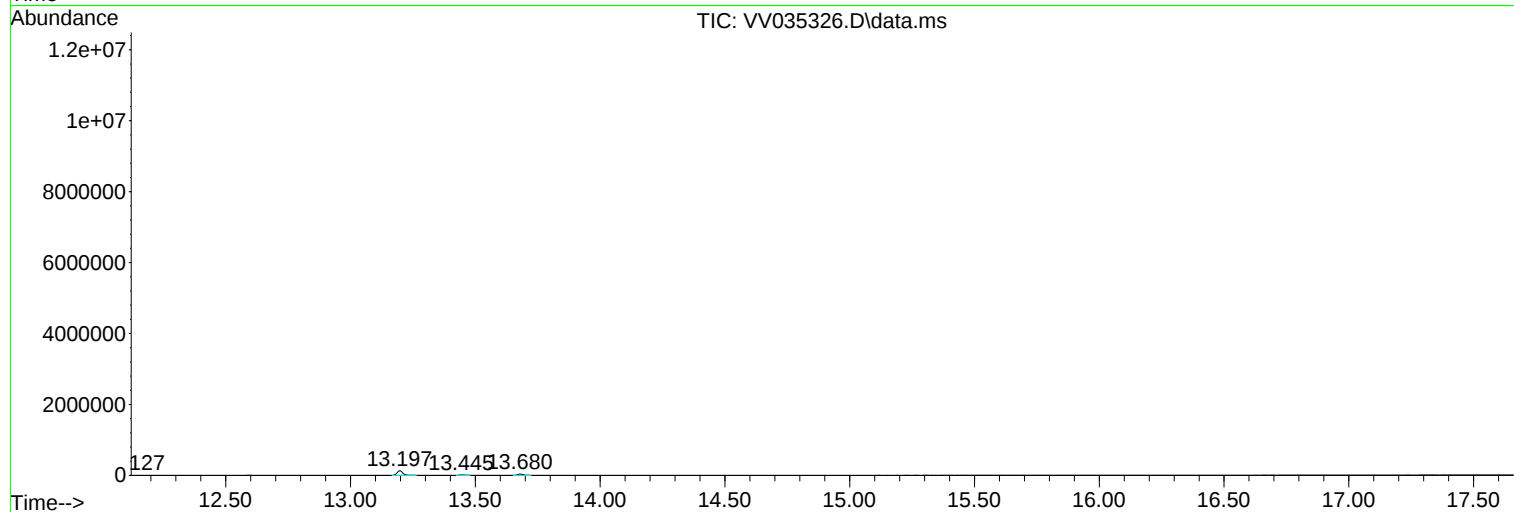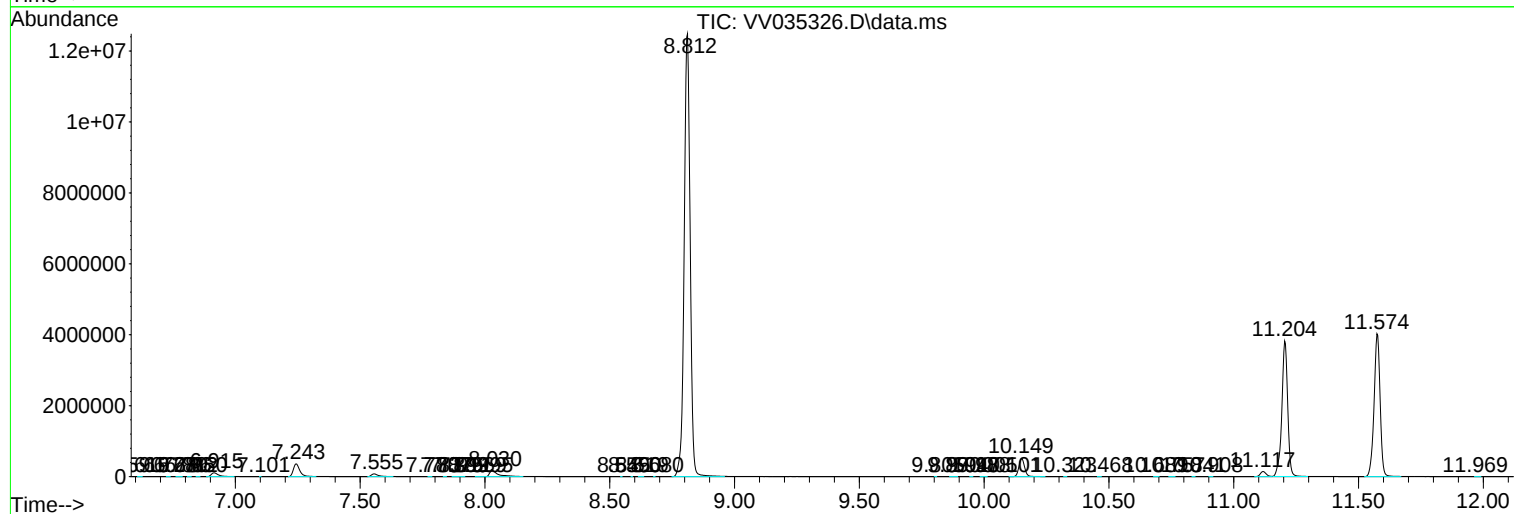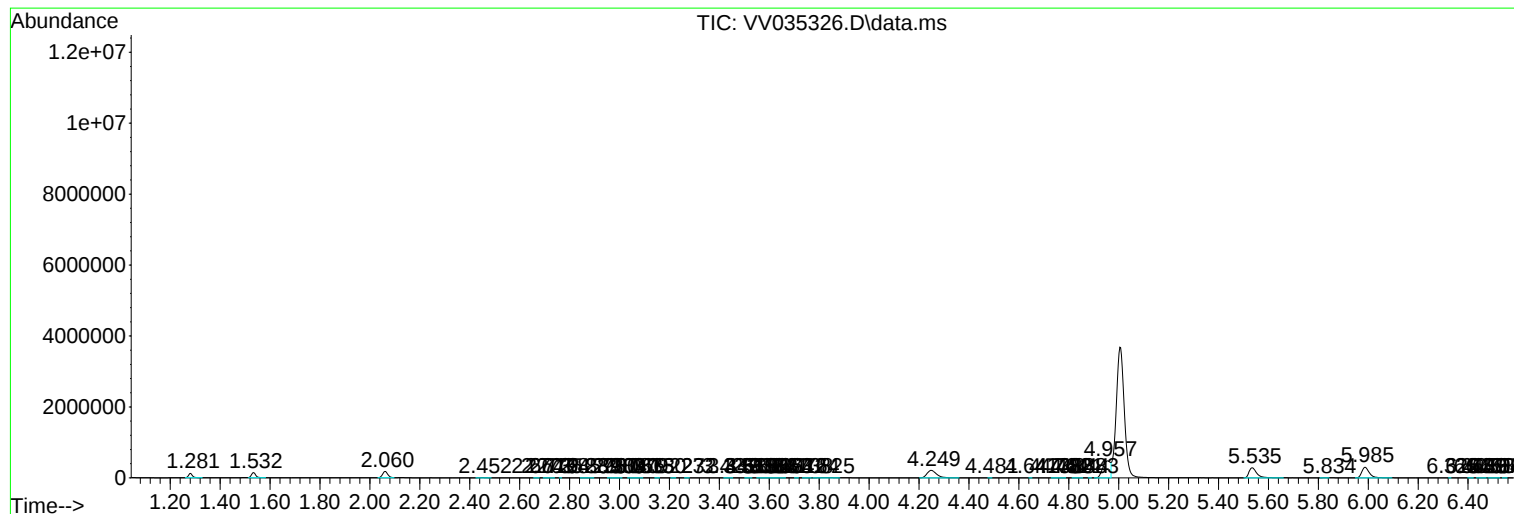

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035326.D
Acq On : 22 Apr 2024 12:35
Operator : SY/MD
Sample : P2182-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035326.D
Acq On : 22 Apr 2024 12:35
Operator : SY/MD
Sample : P2182-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------