

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035327.D
 Acq On : 22 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2182-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	101968	110734	2.93%	0.732%
2	1.532	147	153	173	rVB	133993	157820	4.18%	1.043%
3	2.060	308	317	331	rBV	151166	223997	5.94%	1.480%
4	2.423	428	430	432	rBV2	344	229	0.01%	0.002%
5	2.452	432	439	448	rVB4	3052	4641	0.12%	0.031%
6	2.561	463	473	475	rBV5	1686	2662	0.07%	0.018%
7	2.687	509	512	515	rBV2	301	163	0.00%	0.001%
8	2.773	535	539	544	rBV2	281	242	0.01%	0.002%
9	2.793	544	545	547	rBV2	212	94	0.00%	0.001%
10	2.860	564	566	568	rBV2	168	77	0.00%	0.001%
11	2.886	571	574	575	rBV	366	180	0.00%	0.001%
12	3.031	616	619	628	rVB3	374	468	0.01%	0.003%
13	3.085	634	636	637	rBV	227	93	0.00%	0.001%
14	3.188	665	668	670	rBV	196	132	0.00%	0.001%
15	3.252	687	688	689	rBV	167	54	0.00%	0.000%
16	3.307	704	705	706	rBB	69	30	0.00%	0.000%
17	3.320	707	709	712	rVB	383	168	0.00%	0.001%
18	3.336	712	714	716	rBV2	247	149	0.00%	0.001%
19	3.368	722	724	725	rBV2	104	23	0.00%	0.000%
20	3.378	725	727	730	rBV	140	78	0.00%	0.001%
21	3.394	730	732	736	rBV2	227	137	0.00%	0.001%
22	3.445	746	748	753	rVB2	259	179	0.00%	0.001%
23	3.471	753	756	759	rBV2	255	171	0.00%	0.001%
24	3.487	759	761	765	rVB	236	166	0.00%	0.001%
25	3.593	791	794	798	rVB2	214	177	0.00%	0.001%
26	3.613	798	800	803	rBV2	358	216	0.01%	0.001%
27	3.651	809	812	815	rBV2	473	298	0.01%	0.002%
28	3.667	815	817	821	rVV4	353	265	0.01%	0.002%
29	3.732	834	837	840	rBV2	164	138	0.00%	0.001%
30	3.802	847	859	896	rBV3	61260	209745	5.56%	1.386%
31	4.249	983	998	1034	rBV	191545	491503	13.03%	3.247%
32	4.568	1095	1097	1098	rBV	380	152	0.00%	0.001%
33	4.741	1149	1151	1152	rBV	186	78	0.00%	0.001%
34	4.751	1152	1154	1156	rVB	282	135	0.00%	0.001%
35	4.767	1156	1159	1163	rVB2	343	202	0.01%	0.001%
36	4.786	1163	1165	1166	rBV2	202	101	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035327.D
 Acq On : 22 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2182-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.895	1196	1199	1200	rBV2	357	200	0.01%	0.001%
38	4.957	1203	1218	1233	rBV2	406478	1134285	30.06%	7.493%
39	5.410	1357	1359	1362	rBV2	234	150	0.00%	0.001%
40	5.426	1362	1364	1367	rVB2	352	141	0.00%	0.001%
41	5.535	1387	1398	1428	rBV	250512	536077	14.21%	3.541%
42	5.838	1484	1492	1510	rVB7	5073	12167	0.32%	0.080%
43	5.989	1526	1539	1581	rBV	272141	578733	15.34%	3.823%
44	6.336	1643	1647	1649	rBV	501	382	0.01%	0.003%
45	6.381	1659	1661	1662	rVB	258	77	0.00%	0.001%
46	6.394	1663	1665	1669	rBV	287	209	0.01%	0.001%
47	6.493	1695	1696	1701	rBV3	220	186	0.00%	0.001%
48	6.558	1715	1716	1717	rBV3	111	33	0.00%	0.000%
49	6.609	1730	1732	1735	rBV	185	85	0.00%	0.001%
50	6.629	1735	1738	1739	rBV	189	118	0.00%	0.001%
51	6.725	1765	1768	1771	rBV2	456	271	0.01%	0.002%
52	6.857	1805	1809	1811	rBV2	197	134	0.00%	0.001%
53	6.870	1811	1813	1815	rVB3	170	77	0.00%	0.001%
54	6.915	1816	1827	1854	rBV	95787	196324	5.20%	1.297%
55	7.243	1919	1929	1953	rBV	314998	576418	15.28%	3.808%
56	7.558	2016	2027	2053	rBV	70109	141615	3.75%	0.935%
57	7.847	2114	2117	2122	rBV2	694	541	0.01%	0.004%
58	7.908	2134	2136	2139	rBV	268	123	0.00%	0.001%
59	8.027	2163	2173	2220	rBV2	256402	603270	15.99%	3.985%
60	8.542	2331	2333	2337	rBV2	252	147	0.00%	0.001%
61	8.596	2347	2350	2352	rBV2	390	211	0.01%	0.001%
62	8.699	2379	2382	2383	rBV	149	76	0.00%	0.001%
63	8.809	2398	2416	2460	rBV2	1920223	3773254	100.00%	24.926%
64	9.304	2567	2570	2572	rBV2	313	243	0.01%	0.002%
65	9.455	2615	2617	2618	rBV2	227	109	0.00%	0.001%
66	9.481	2622	2625	2627	rBV	302	169	0.00%	0.001%
67	9.506	2627	2633	2635	rBV	760	620	0.02%	0.004%
68	9.542	2641	2644	2645	rBV2	309	166	0.00%	0.001%
69	9.599	2660	2662	2663	rBV	343	122	0.00%	0.001%
70	9.661	2679	2681	2683	rBV2	279	148	0.00%	0.001%
71	9.712	2695	2697	2699	rBV	448	226	0.01%	0.001%
72	9.757	2709	2711	2713	rBV2	261	143	0.00%	0.001%
73	9.799	2722	2724	2726	rBV	223	97	0.00%	0.001%
74	9.844	2736	2738	2742	rBV3	273	225	0.01%	0.001%
75	9.924	2760	2763	2766	rBV2	486	360	0.01%	0.002%
76	9.966	2773	2776	2777	rBV2	232	147	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035327.D
 Acq On : 22 Apr 2024 12:57
 Operator : SY/MD
 Sample : P2182-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.017	2789	2792	2794	rBV2	228	146	0.00%	0.001%
78	10.062	2803	2806	2810	rBV3	287	243	0.01%	0.002%
79	10.149	2821	2833	2859	rBV	482743	775845	20.56%	5.125%
80	10.461	2927	2930	2933	rBV	372	281	0.01%	0.002%
81	10.532	2948	2952	2954	rBV3	315	225	0.01%	0.001%
82	10.664	2990	2993	2996	rBV3	448	284	0.01%	0.002%
83	10.966	3085	3087	3090	rBV2	263	159	0.00%	0.001%
84	11.011	3098	3101	3105	rBV2	280	245	0.01%	0.002%
85	11.117	3124	3134	3145	rBV	125319	200195	5.31%	1.322%
86	11.204	3146	3161	3189	rVB2	837703	1796458	47.61%	11.867%
87	11.574	3260	3276	3299	rBV2	1623435	3019992	80.04%	19.950%
88	12.024	3414	3416	3419	rBV	436	251	0.01%	0.002%
89	12.349	3513	3517	3519	rBV2	1109	733	0.02%	0.005%
90	12.905	3686	3690	3692	rBV3	380	320	0.01%	0.002%
91	13.111	3751	3754	3757	rBV	446	440	0.01%	0.003%
92	13.197	3770	3781	3798	rBV	266406	420250	11.14%	2.776%
93	13.445	3852	3858	3869	rBV	7581	12802	0.34%	0.085%
94	13.680	3920	3931	3946	rBV	87456	145278	3.85%	0.960%




Sum of corrected areas: 15137923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035327.D
Acq On : 22 Apr 2024 12:57
Operator : SY/MD
Sample : P2182-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

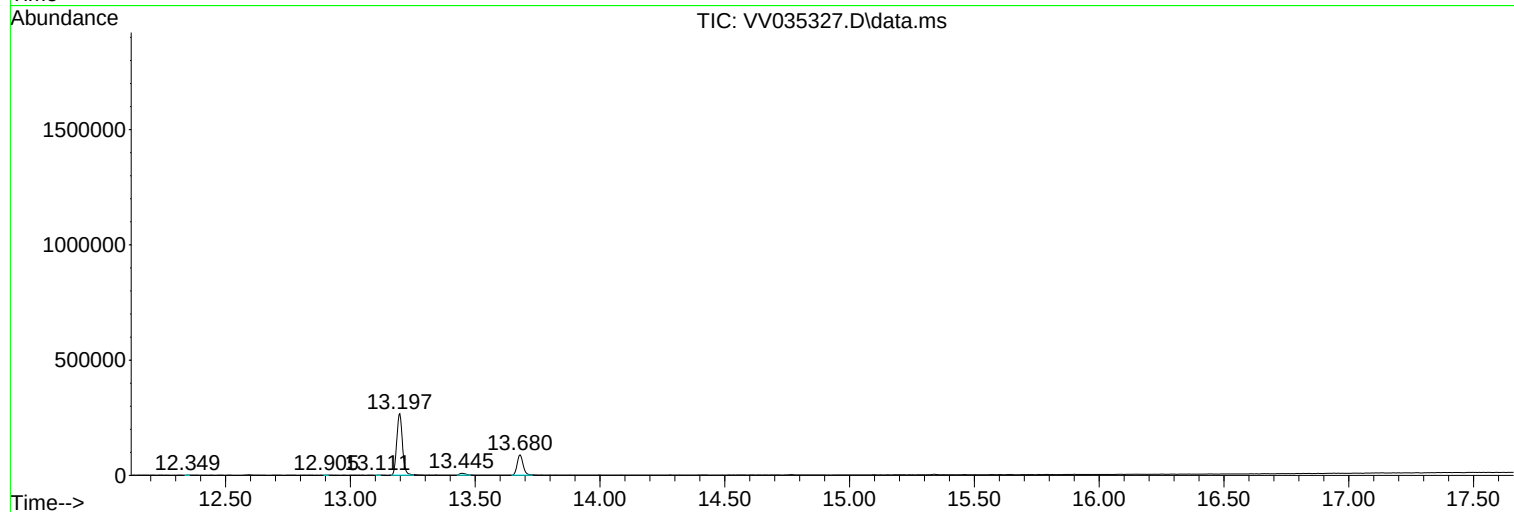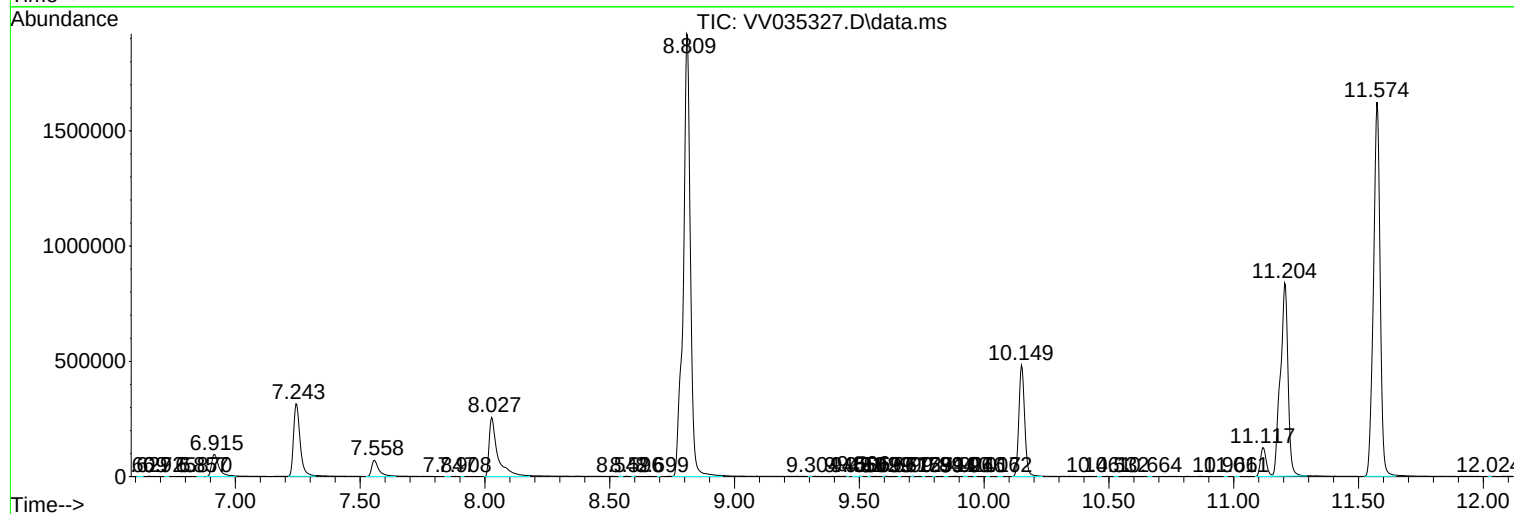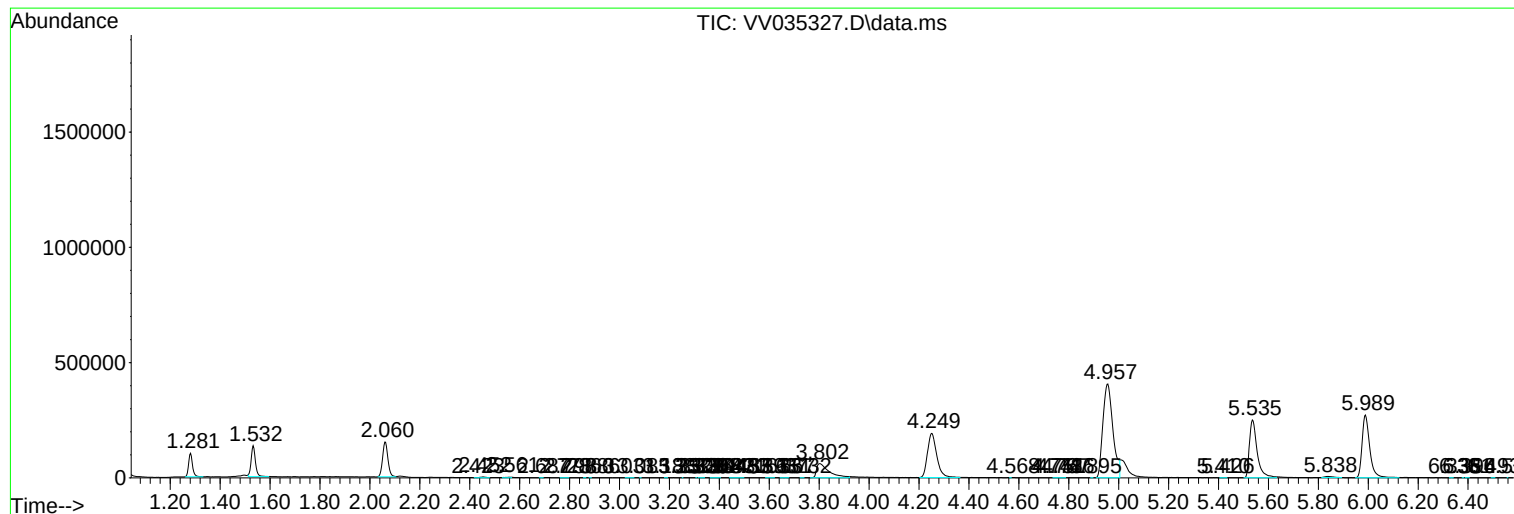

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035327.D
Acq On : 22 Apr 2024 12:57
Operator : SY/MD
Sample : P2182-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035327.D
Acq On : 22 Apr 2024 12:57
Operator : SY/MD
Sample : P2182-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc